


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011737.D
 Acq On : 19 Sep 2022 16:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 04:42:52 2022

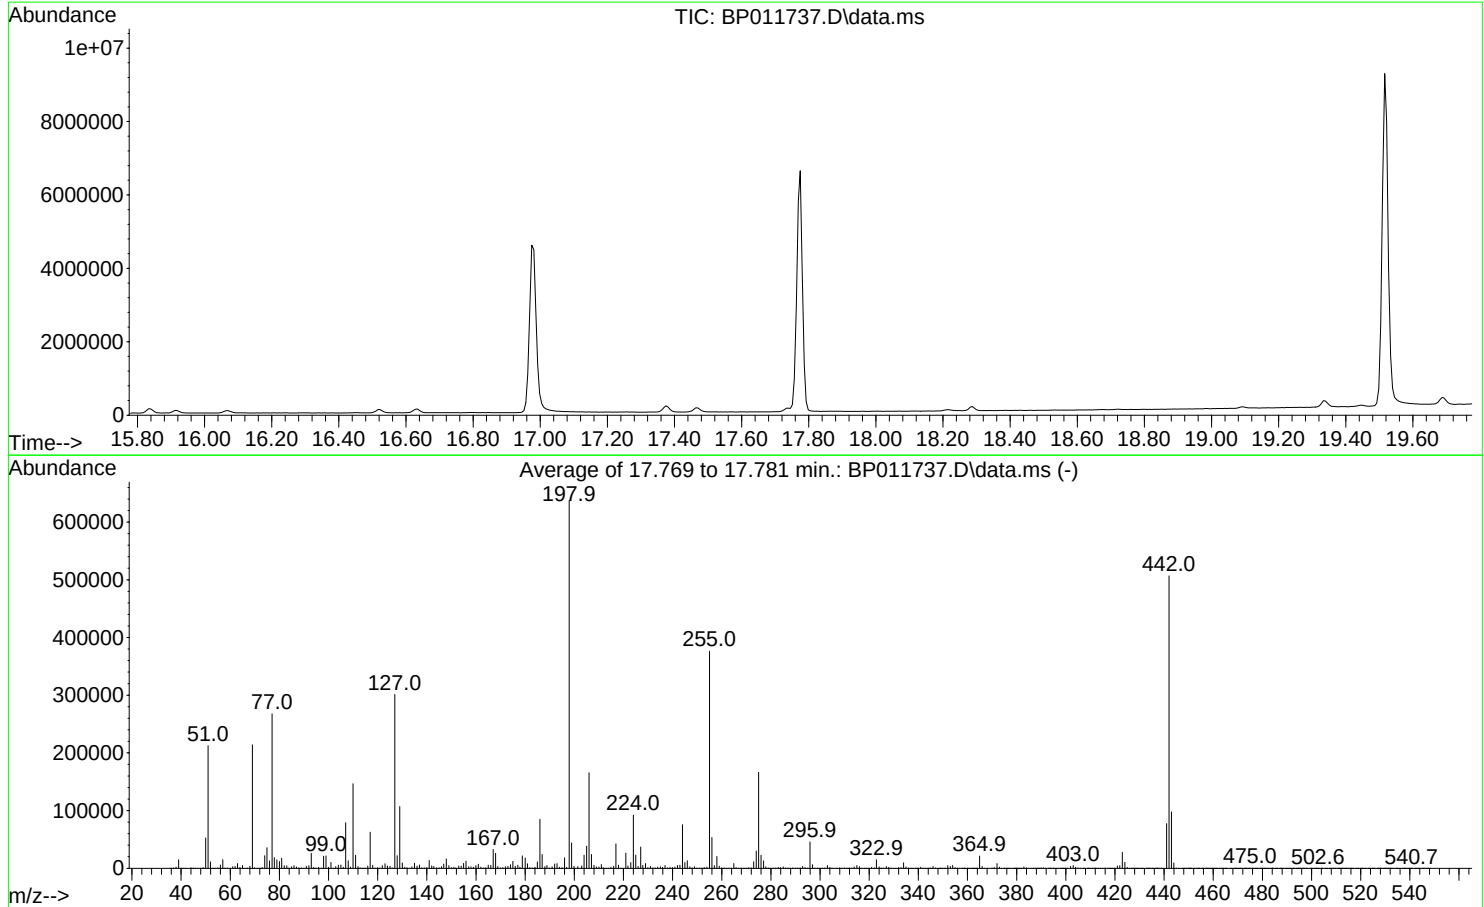




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	212646	PASS
68	69	0.00	2	1.6	3504	PASS
69	198	0.00	100	33.6	213923	PASS
70	69	0.00	2	0.5	1098	PASS
127	198	10	80	47.3	301376	PASS
197	198	0.00	2	0.3	1649	PASS
198	198	100	100	100.0	637577	PASS
199	198	5	9	6.9	43984	PASS
275	198	10	60	26.1	166243	PASS
365	198	1	100	3.3	21272	PASS
441	198	0.01	100	12.2	77467	PASS
442	442	100	100	100.0	506789	PASS
443	442	15	24	19.3	97911	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011737.D
 Acq On : 19 Sep 2022 16:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 20 07:05:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 04:42:52 2022
 Response via : Initial Calibration

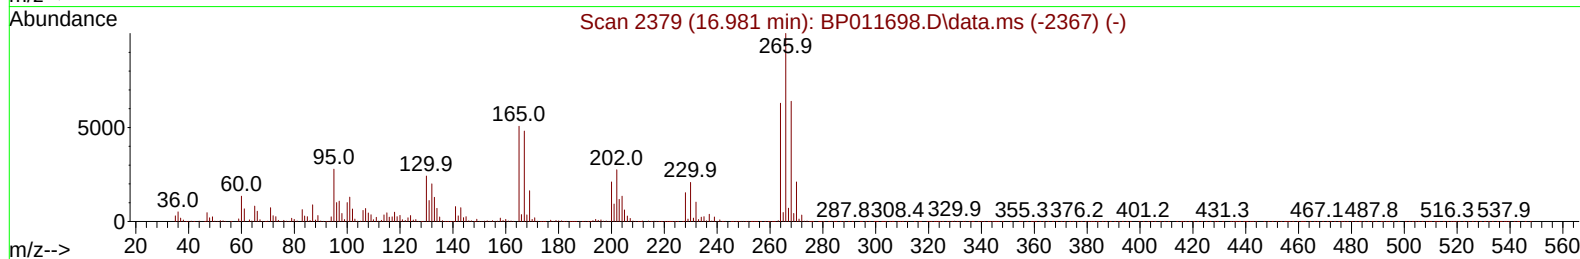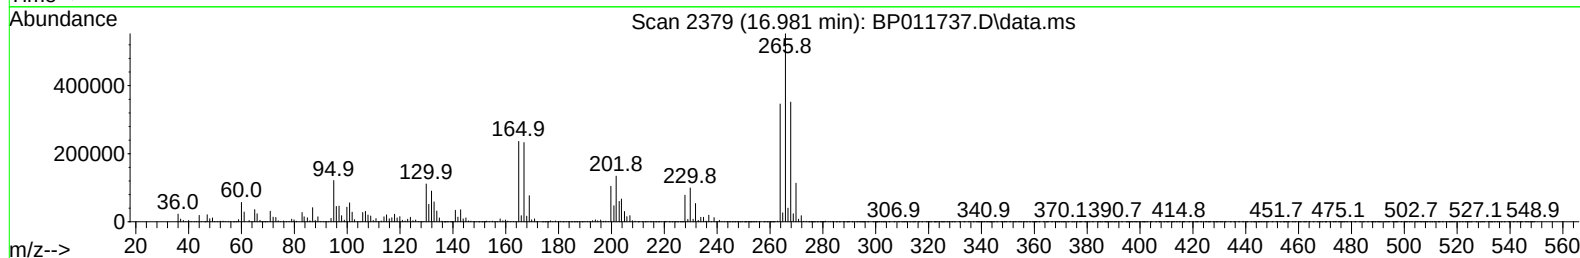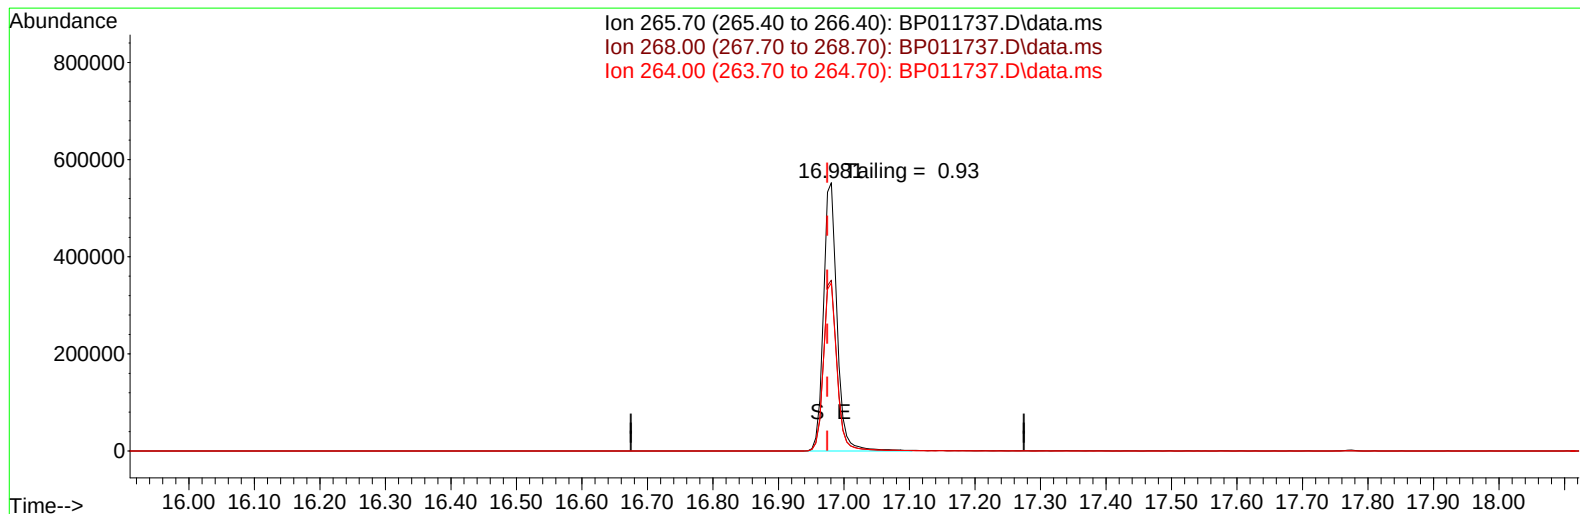

TIC: BP011737.D\data.ms

(70) Pentachlorophenol (C)

16.981min (+ 0.006) 72116.88 ng




response 797505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.70
264.00	63.00	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011737.D
Acq On : 19 Sep 2022 16:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 20 07:05:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 04:42:52 2022
Response via : Initial Calibration

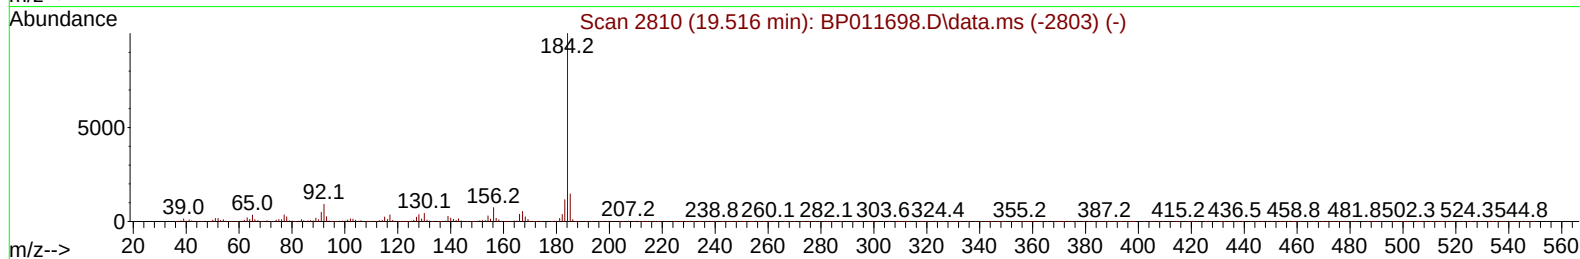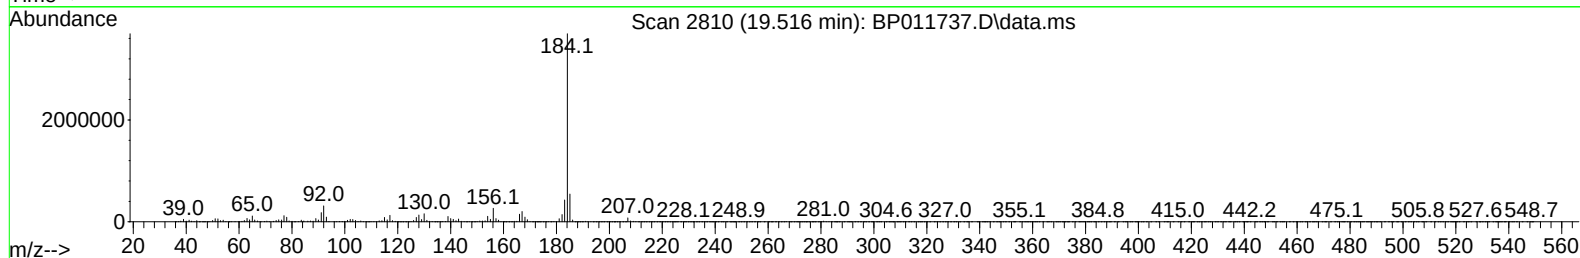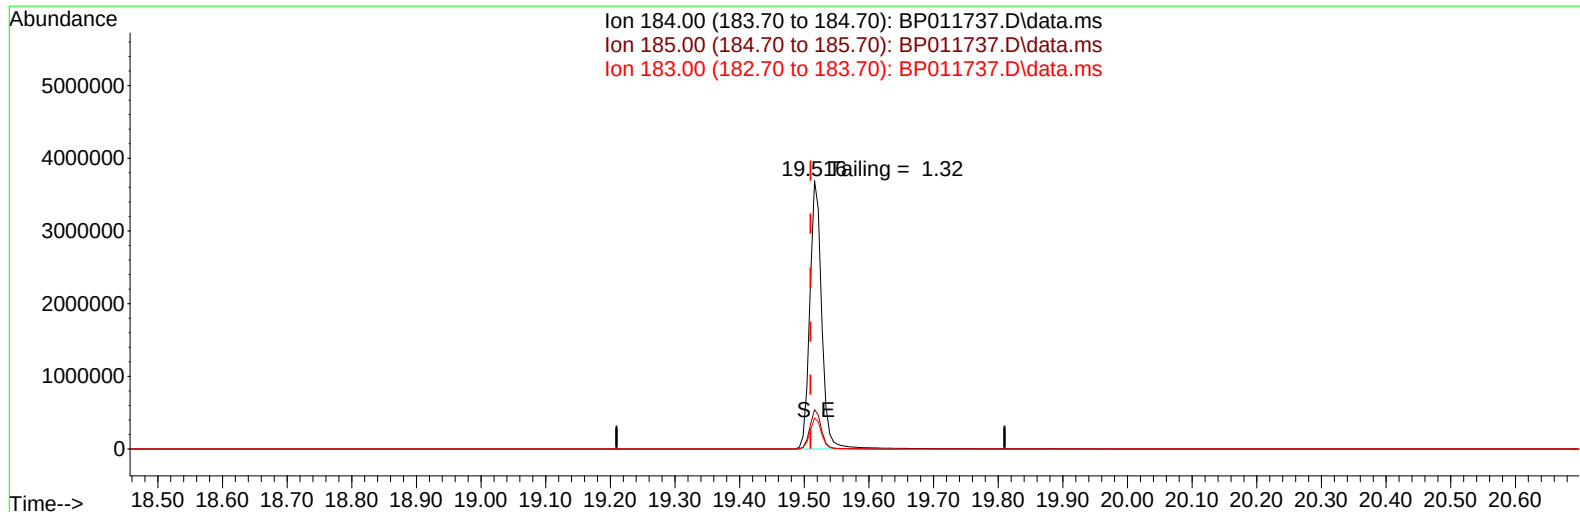

TIC: BP011737.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 43204.73 ng

response 4736696

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.70
183.00	11.30	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2022	BNA_P	<u>BP011737.D</u>
Compound Name	Response	Retention Time
DDT	2203755	20.716
DDD	16958	20.286
DDE	4656	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21614	2225369	0.97

Instrument :
BNA_P
ClientSampleId :
DFTPP