
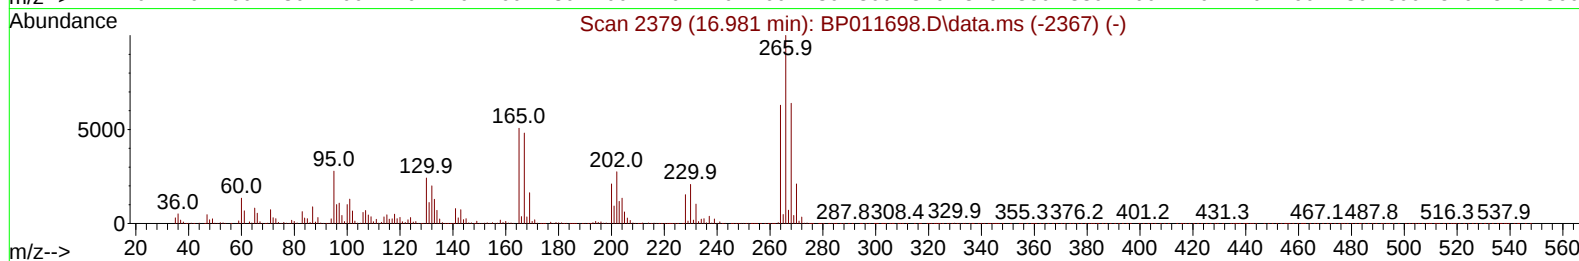
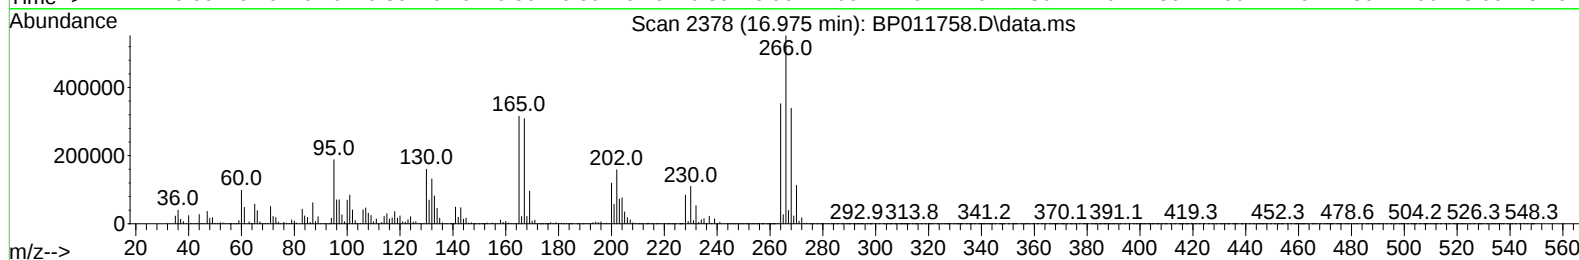


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092022\
 Data File : BP011758.D
 Acq On : 20 Sep 2022 12:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 07:20:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 04:42:52 2022
 Response via : Initial Calibration

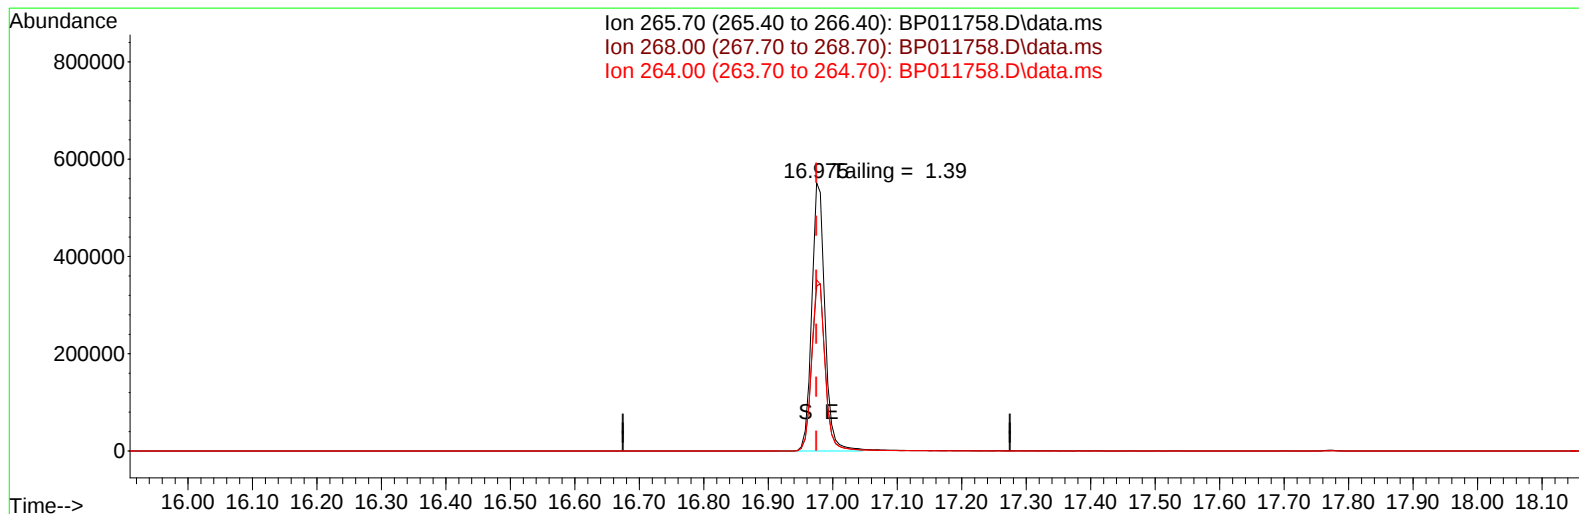

TIC: BP011758.D\data.ms

(70) Pentachlorophenol (C)




16.975min (+ 0.000) 235339.60 ng

response 796255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.42
264.00	63.00	63.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092022\
Data File : BP011758.D
Acq On : 20 Sep 2022 12:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 07:20:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 04:42:52 2022
Response via : Initial Calibration

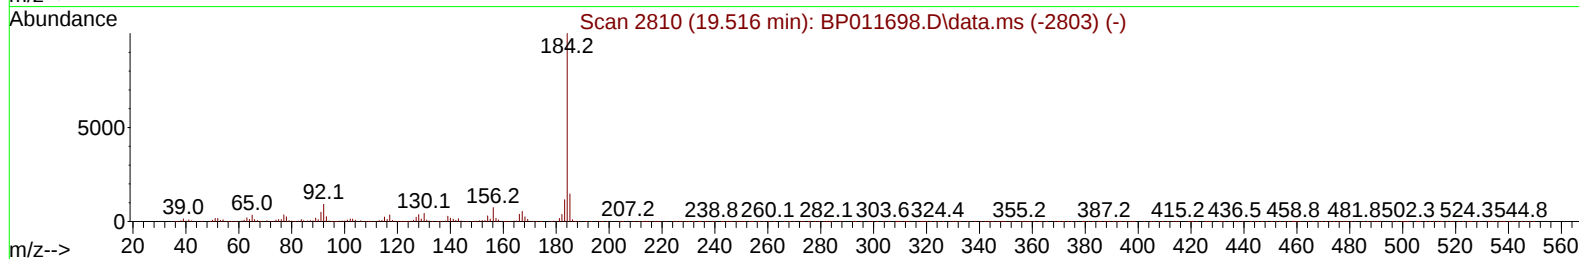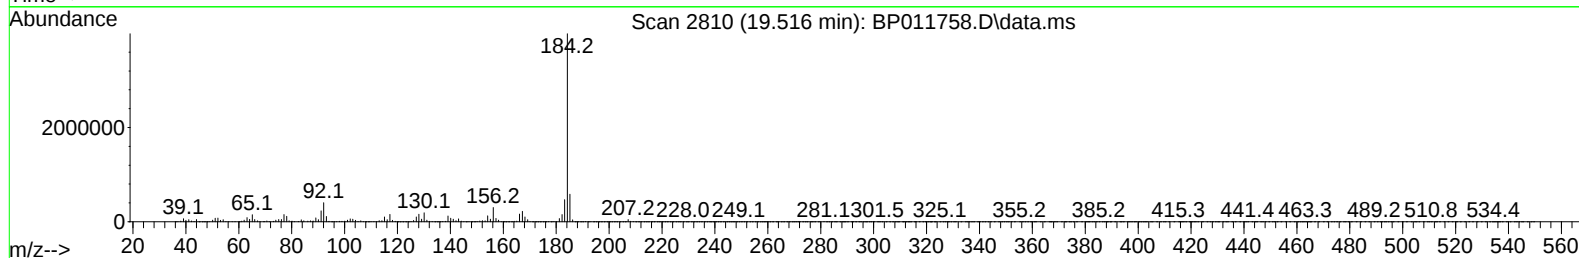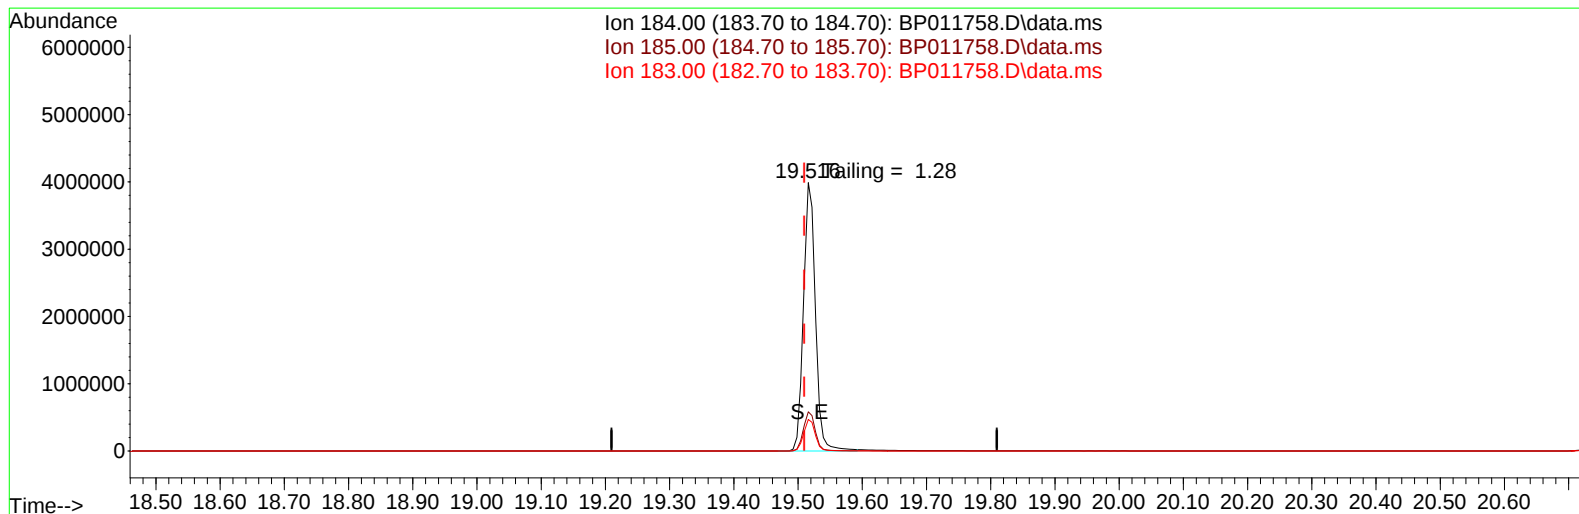

TIC: BP011758.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 1928430.51 ng

response 5228199

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.65
183.00	11.30	11.77
0.00	0.00	0.00