


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092022\
 Data File : BP011758.D
 Acq On : 20 Sep 2022 12:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 04:42:52 2022

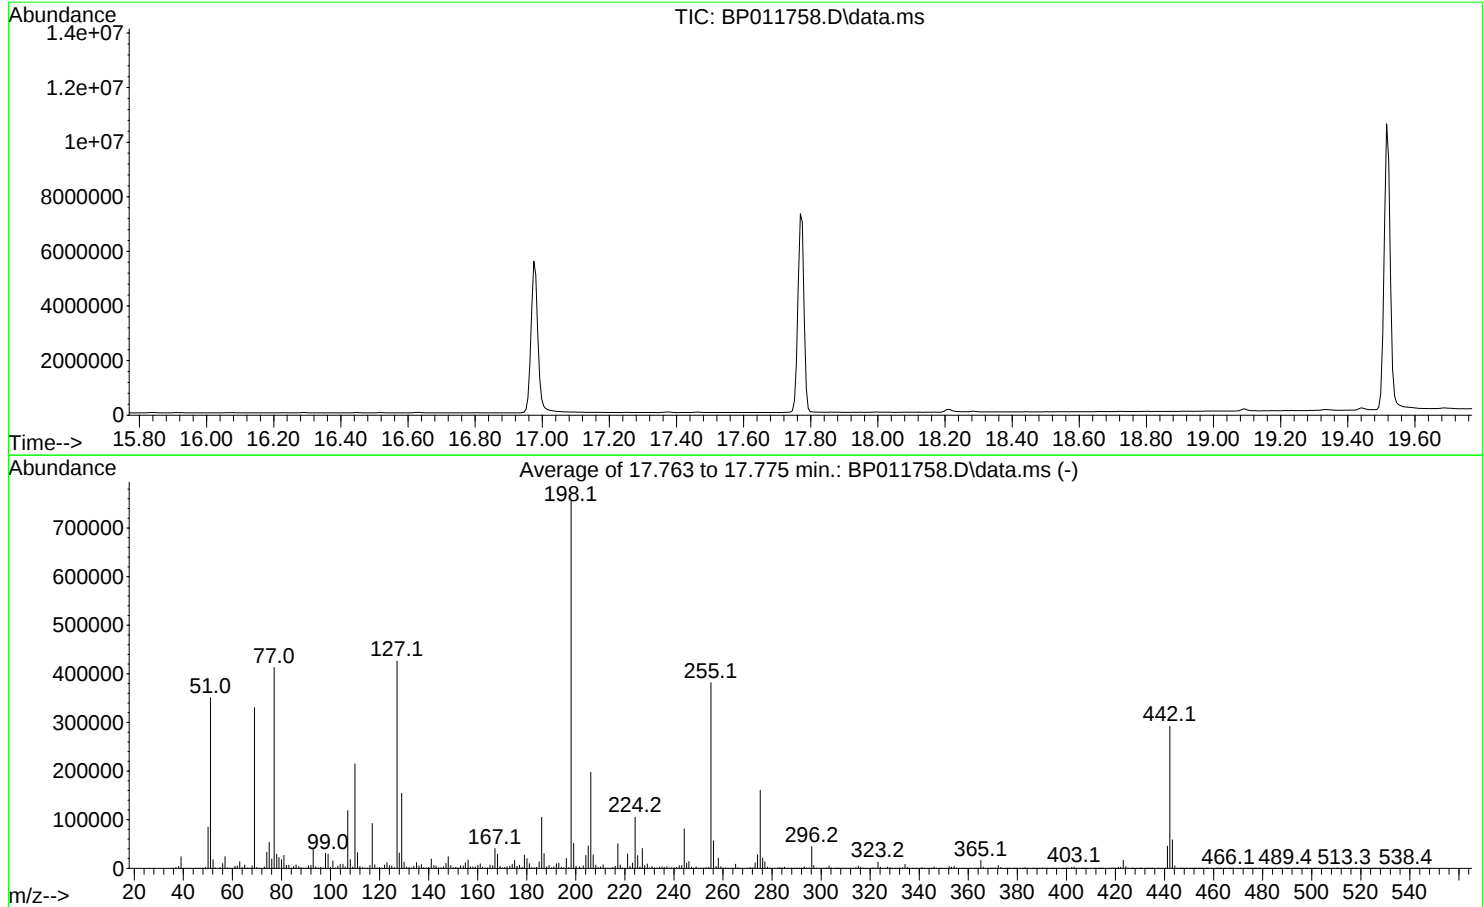




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	350674	PASS
68	69	0.00	2	1.6	5178	PASS
69	198	0.00	100	43.7	330788	PASS
70	69	0.00	2	0.5	1741	PASS
127	198	10	80	56.3	426163	PASS
197	198	0.00	2	0.2	1525	PASS
198	198	100	100	100.0	756700	PASS
199	198	5	9	6.8	51500	PASS
275	198	10	60	21.2	160597	PASS
365	198	1	100	2.1	16017	PASS
441	198	0.01	100	6.0	45752	PASS
442	442	100	100	100.0	292196	PASS
443	442	15	24	20.0	58301	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092022\
Data File : BP011758.D
Acq On : 20 Sep 2022 12:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 21 07:20:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 04:42:52 2022
Response via : Initial Calibration

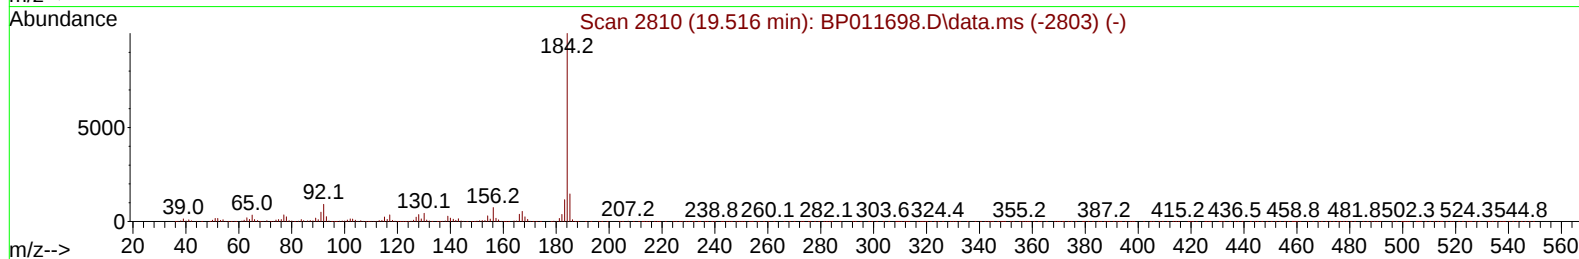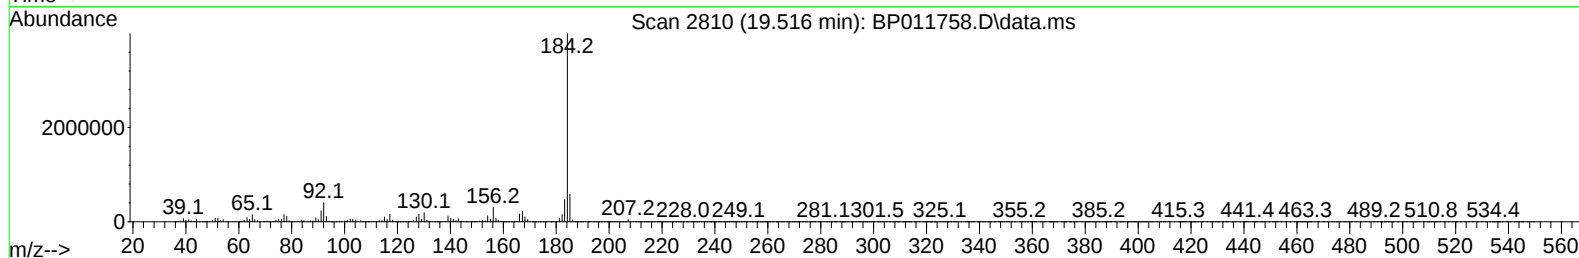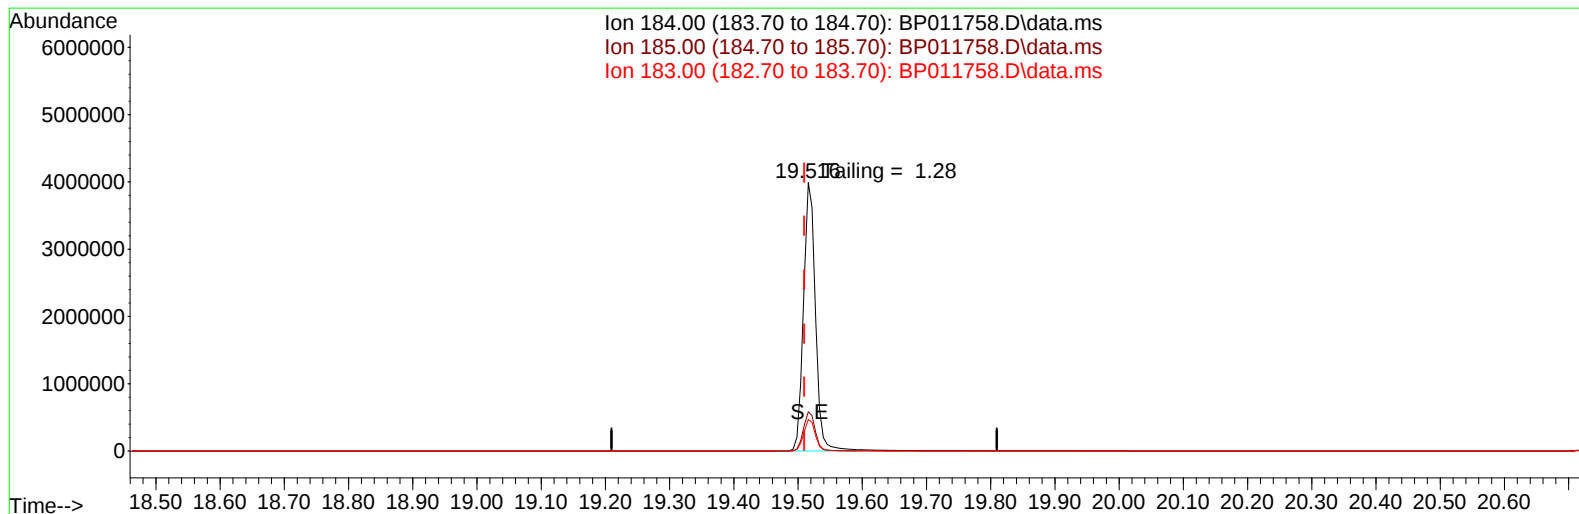

TIC: BP011758.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 1928430.51 ng

response 5228199

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.65
183.00	11.30	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2022	BNA_P	<u>BP011758.D</u>
Compound Name	Response	Retention Time
DDT	2579359	20.71
DDD	12079	20.28
DDE	1091	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13170	2592529	0.51

Instrument :
BNA_P
ClientSampleId :
DFTPP