
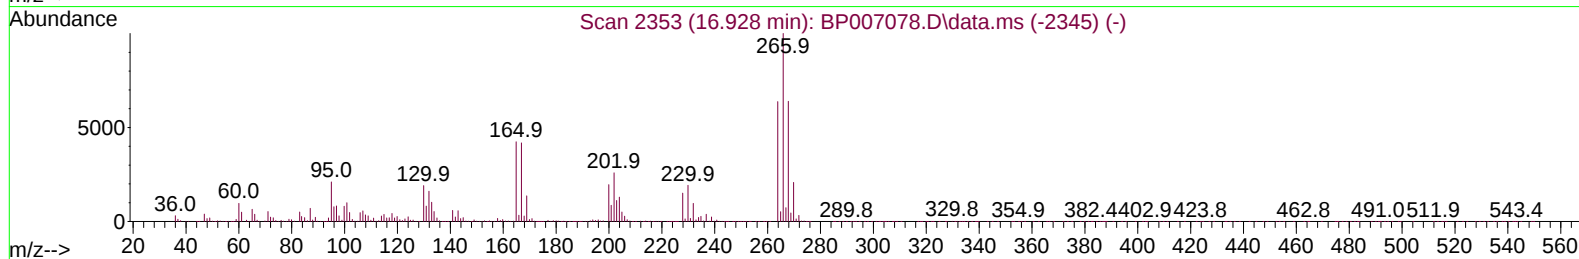
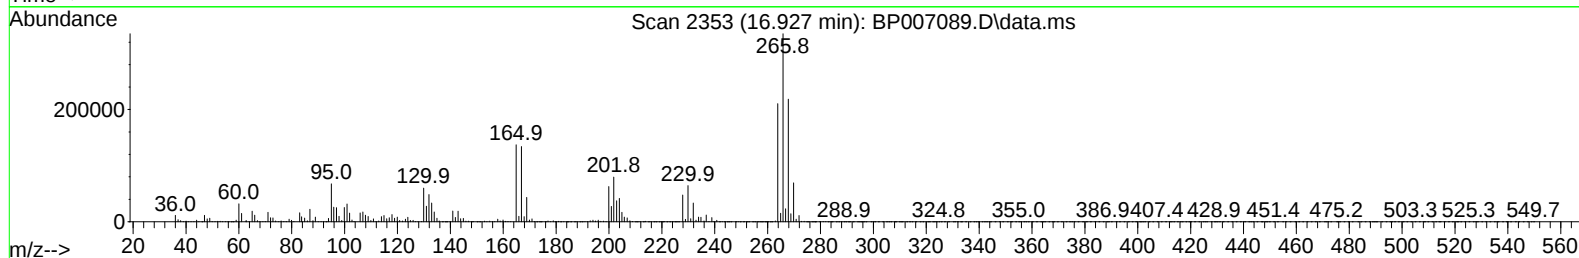


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092221\  
Data File : BP007089.D  
Acq On : 22 Sep 2021 09:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 11:31:48 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 21 16:50:24 2021  
Response via : Initial Calibration

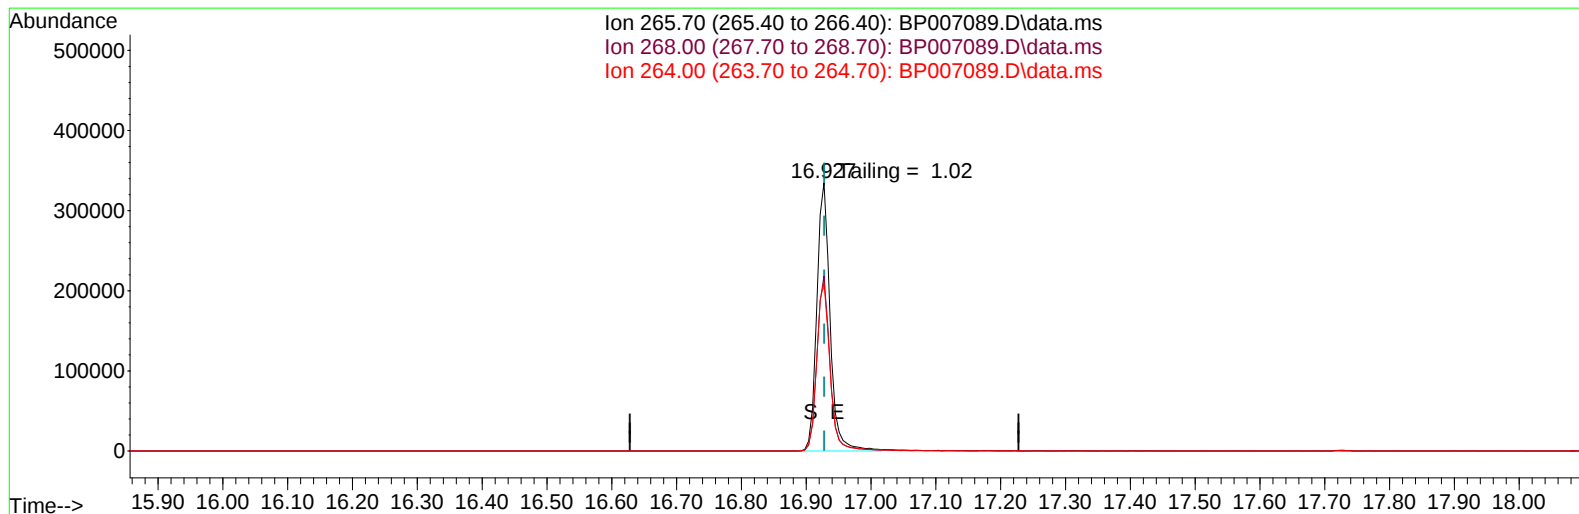

TIC: BP007089.D\data.ms

**(70) Pentachlorophenol (C)**




16.927min (-0.000) 3559193.41 ng

response 481922

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 65.17  |
| 264.00 | 62.90  | 62.82  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP092221\  
 Data File : BP007089.D  
 Acq On : 22 Sep 2021 09:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 11:31:48 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP092121.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Sep 21 16:50:24 2021  
 Response via : Initial Calibration

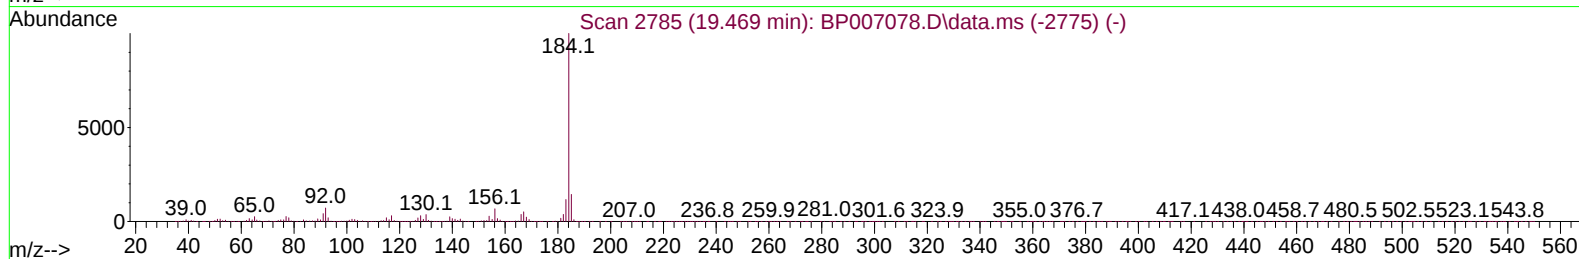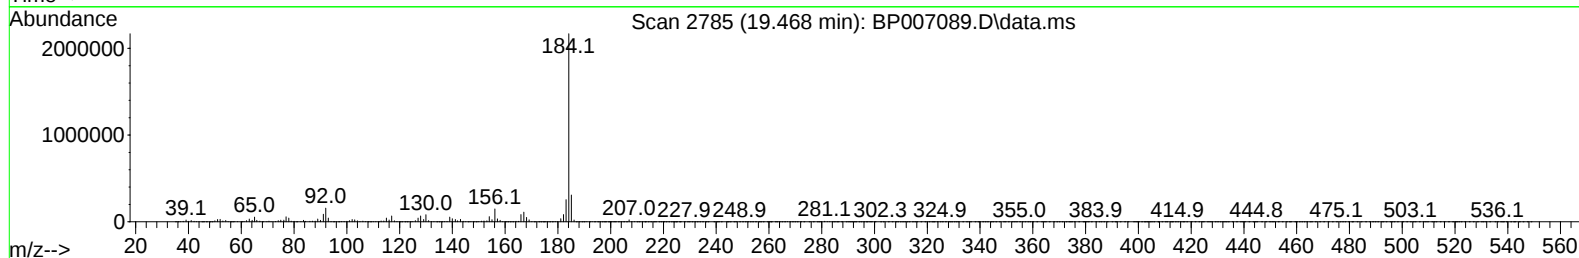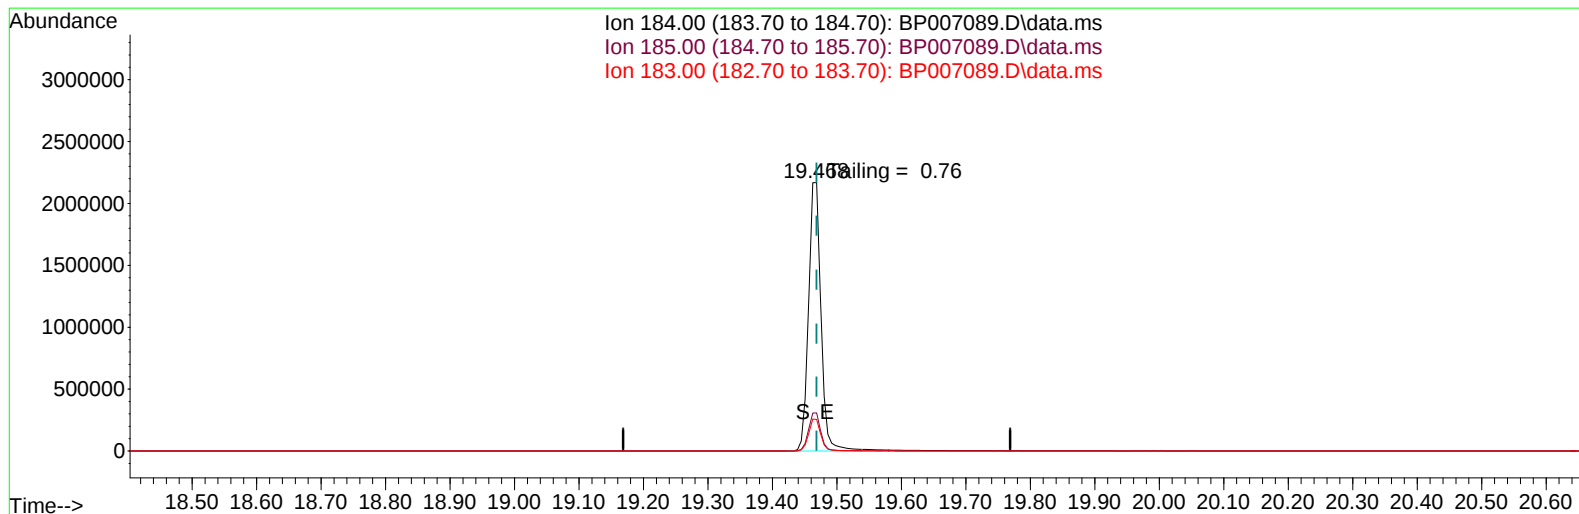

TIC: BP007089.D\data.ms

**(77) Benzidine****19.468min (-0.000) 704682.65 ng****response 2945216**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.70  | 14.23  |
| 183.00 | 11.90  | 11.78  |
| 0.00   | 0.00   | 0.00   |