
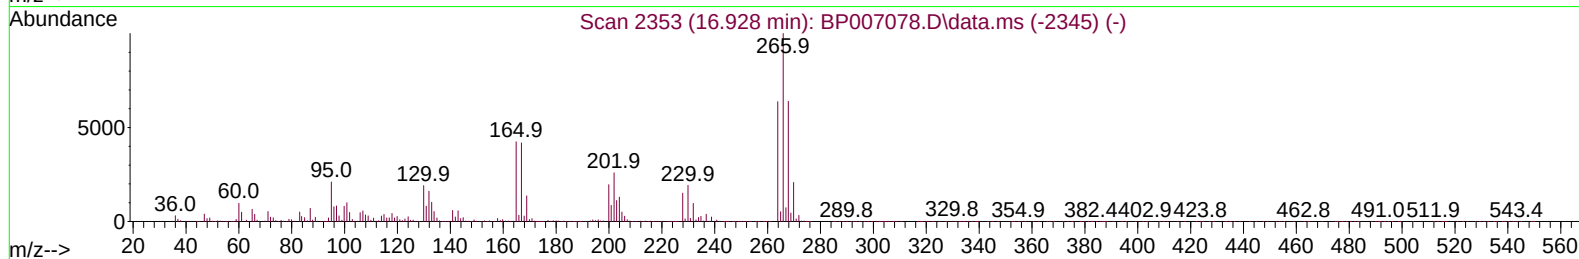
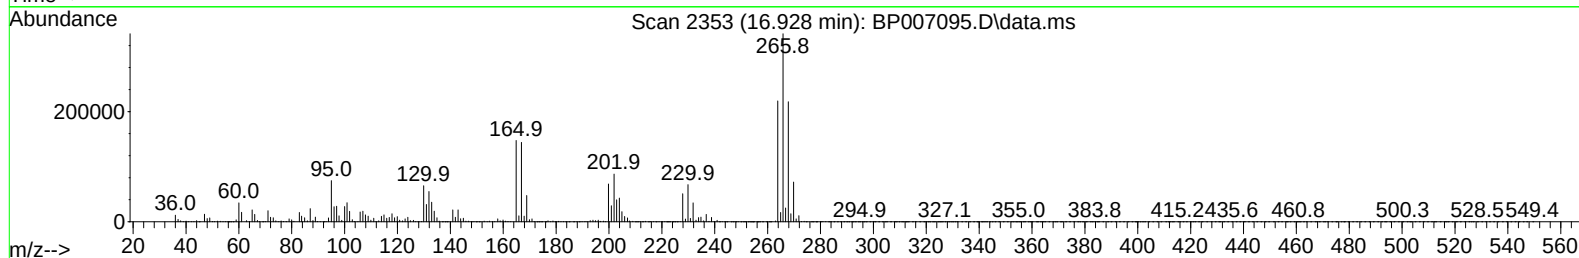


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007095.D
 Acq On : 22 Sep 2021 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 14:19:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 16:50:24 2021
 Response via : Initial Calibration

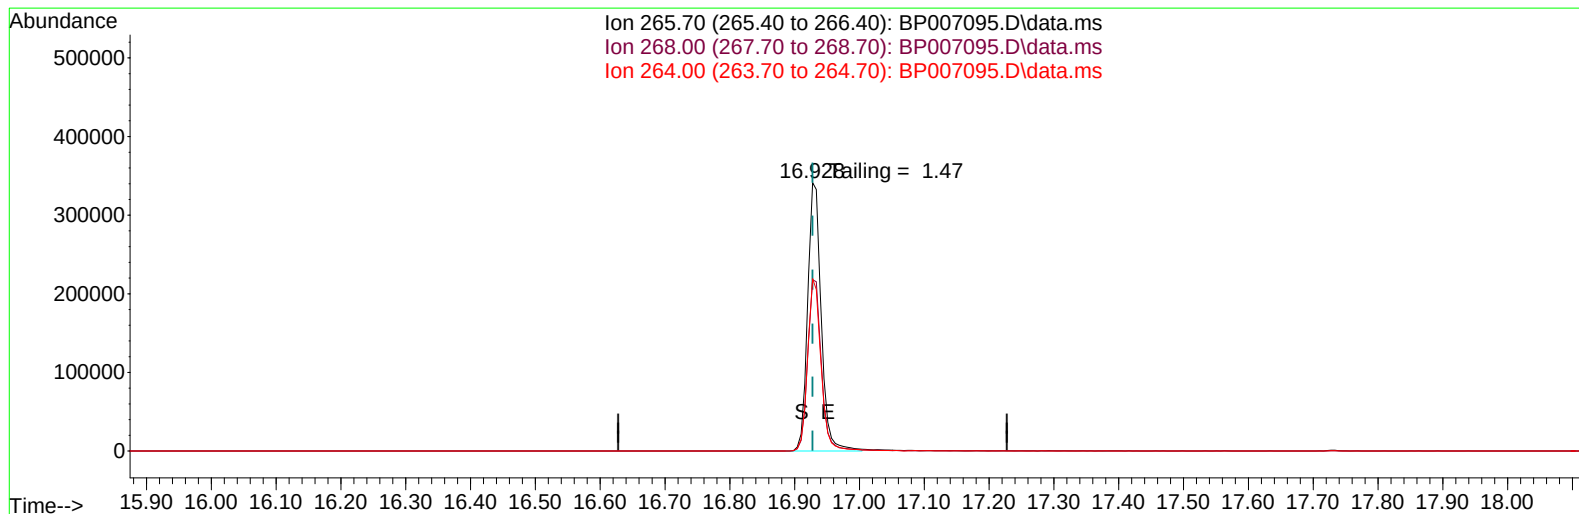

TIC: BP007095.D\data.ms

(70) Pentachlorophenol (C)




16.928min (-0.000) 67839.39 ng

response 501125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.80
264.00	62.90	64.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007095.D
Acq On : 22 Sep 2021 13:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 14:19:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 16:50:24 2021
Response via : Initial Calibration

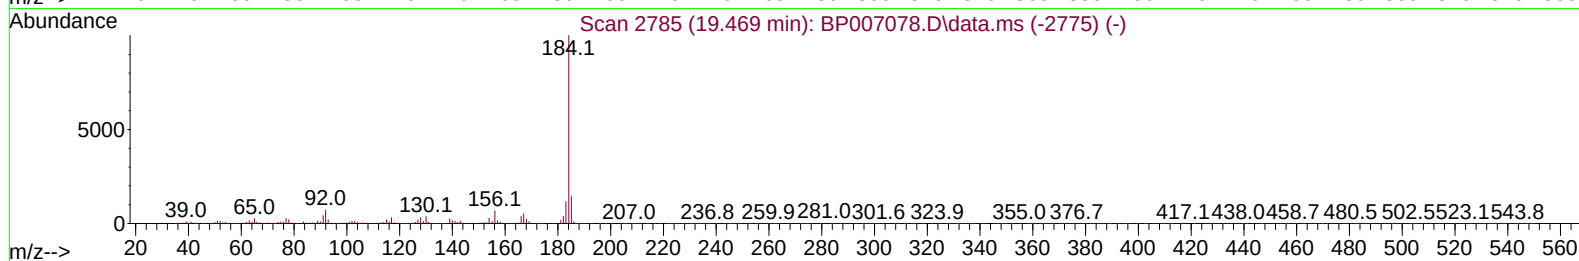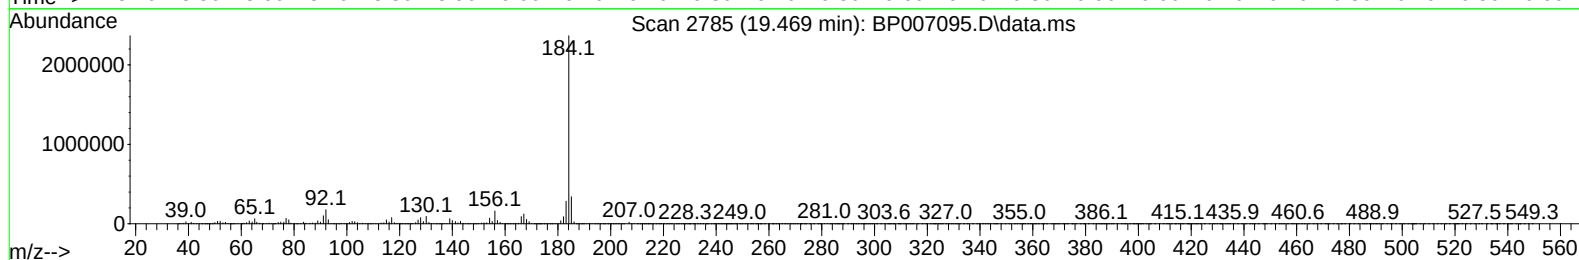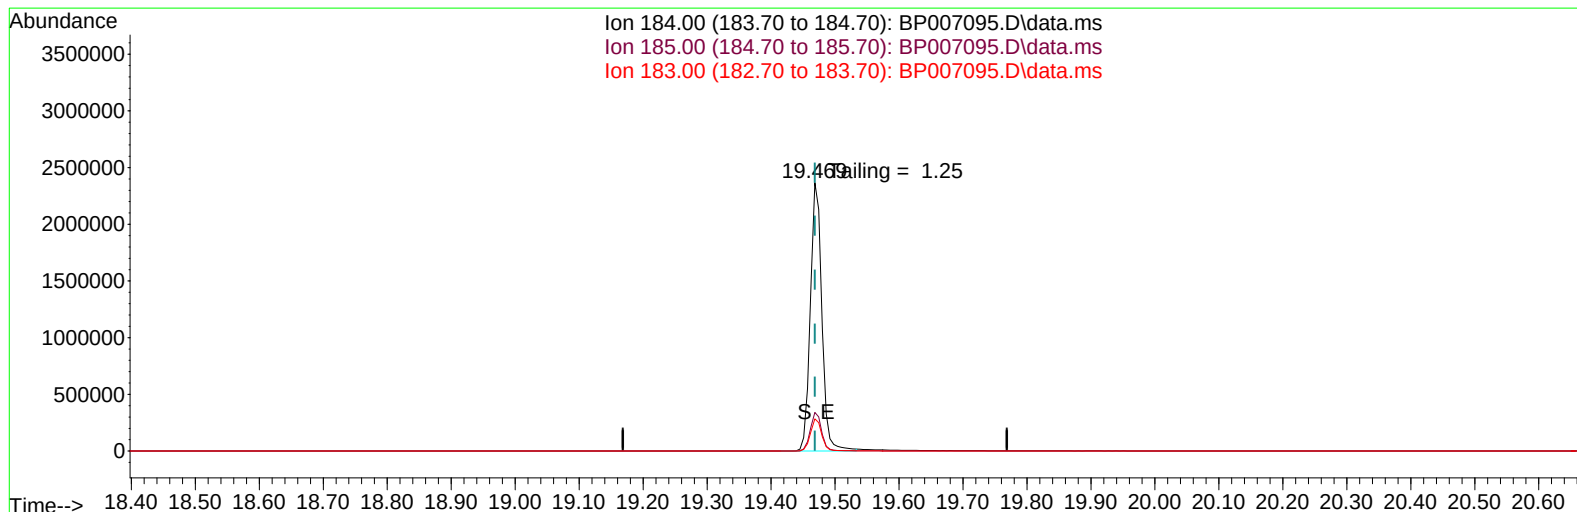

TIC: BP007095.D\data.ms

(77) Benzidine**19.469min (-0.000) 39704.98 ng****response 3034628**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.37
183.00	11.90	11.98
0.00	0.00	0.00