

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007091.D
 Acq On : 22 Sep 2021 10:40
 Operator : CG/JU
 Sample : PB139216BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139216BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.470	399	405	426	rBV	4302156	6156443	39.82%	9.320%
2	7.064	667	676	692	rBV	3810633	6104348	39.48%	9.241%
3	7.899	811	818	827	rBV	913829	1438696	9.31%	2.178%
4	9.063	1007	1016	1031	rBV	2254357	3808069	24.63%	5.765%
5	10.699	1286	1294	1310	rBV	1191911	2027045	13.11%	3.069%
6	13.157	1704	1712	1727	rBV	6377473	9559040	61.83%	14.471%
7	14.528	1936	1945	1958	rBV	1880488	2811624	18.19%	4.256%
8	16.016	2191	2198	2218	rBV	5184784	7324798	47.38%	11.089%
9	17.281	2405	2413	2427	rBV	2357827	3524451	22.80%	5.336%
10	19.834	2842	2847	2858	rBV	12045513	15460844	100.00%	23.406%
11	21.363	3102	3107	3116	rBV	3038688	3892733	25.18%	5.893%
12	23.774	3511	3517	3528	rVB2	1992947	3948020	25.54%	5.977%




Sum of corrected areas: 66056111

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007091.D
Acq On : 22 Sep 2021 10:40
Operator : CG/JU
Sample : PB139216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

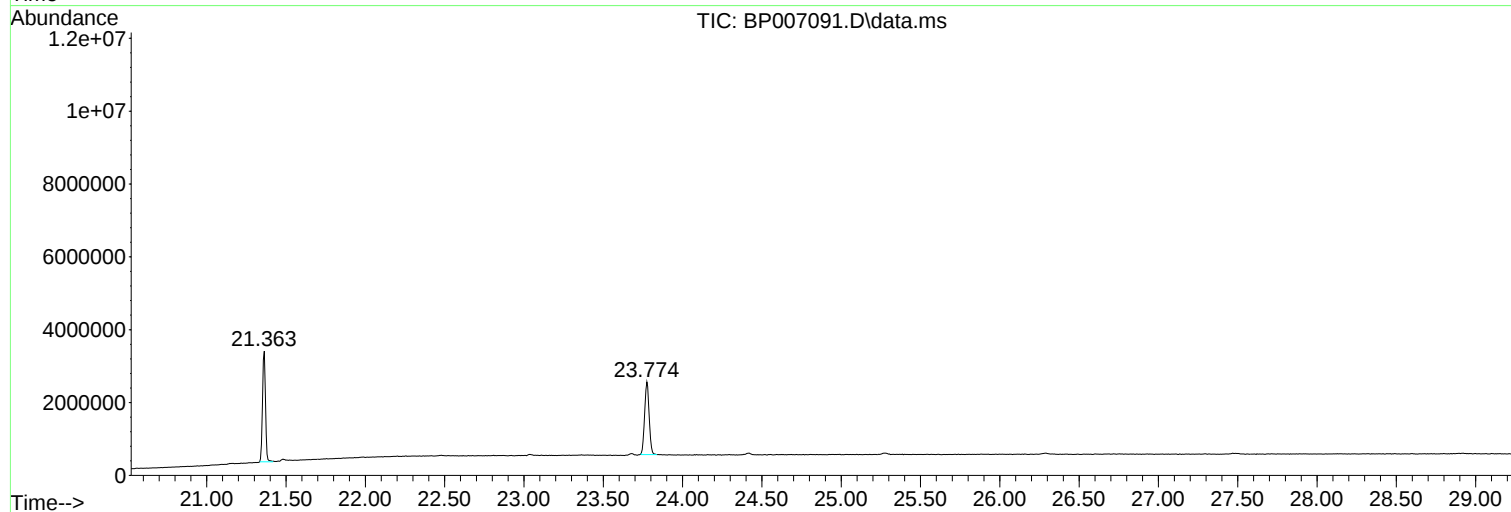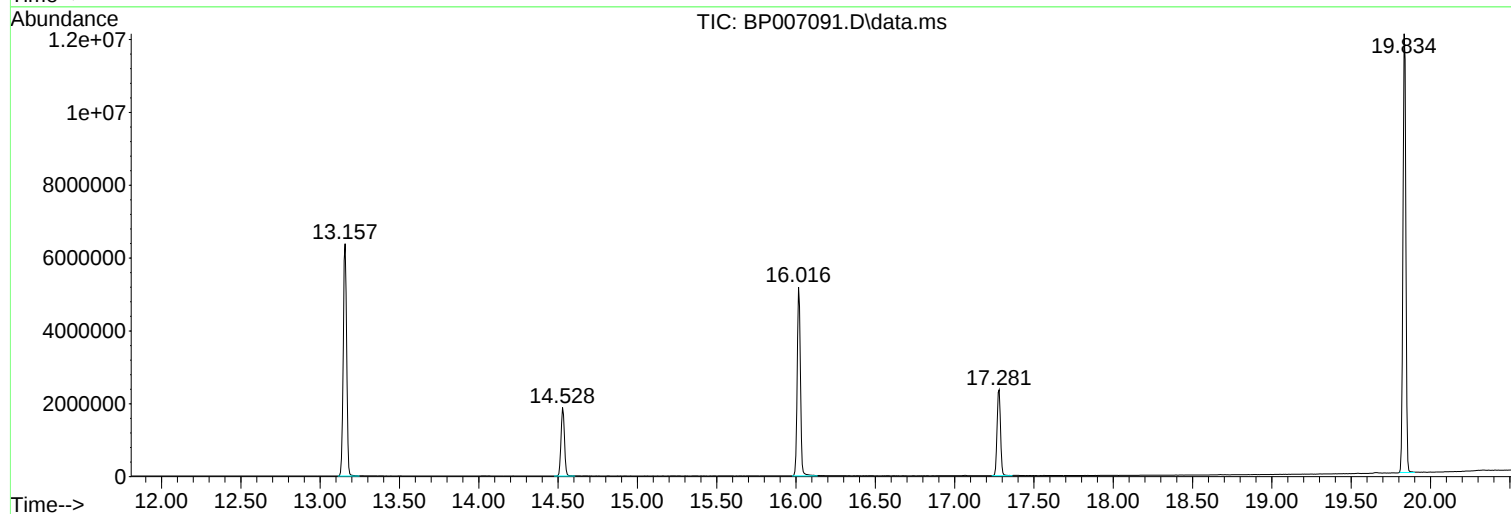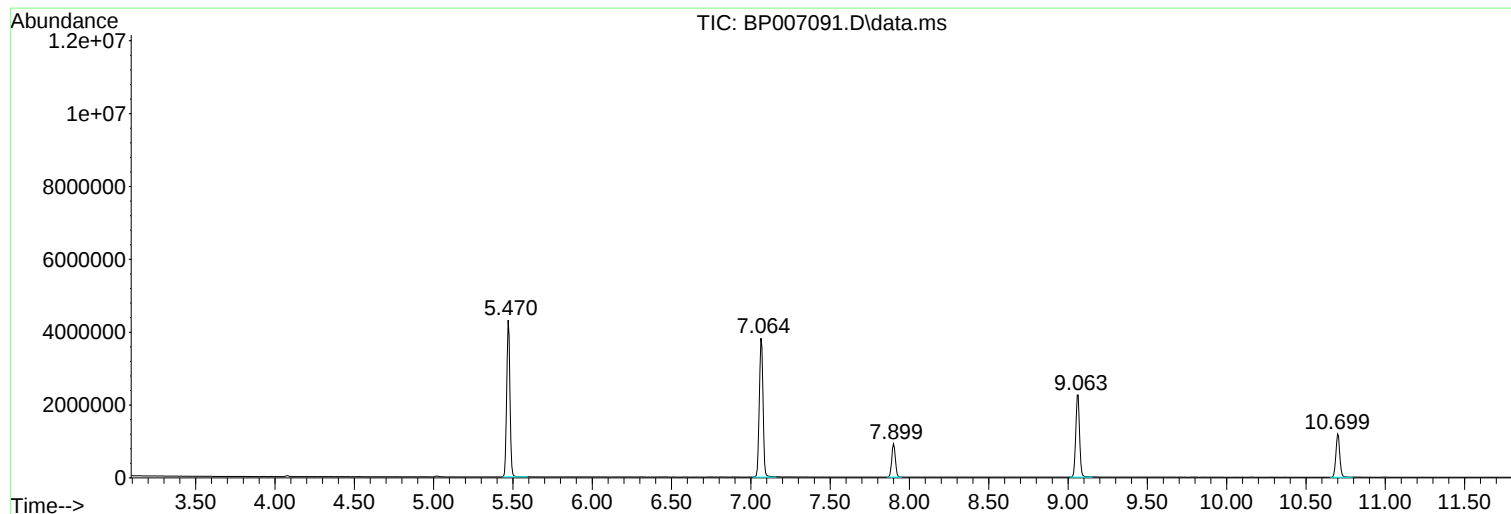

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007091.D
Acq On : 22 Sep 2021 10:40
Operator : CG/JU
Sample : PB139216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007091.D
Acq On : 22 Sep 2021 10:40
Operator : CG/JU
Sample : PB139216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------