

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007097.D
 Acq On : 22 Sep 2021 14:20
 Operator : CG/JU
 Sample : PB139245BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139245BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	399	406	420	rBV	4325654	6375526	40.18%	9.308%
2	7.069	669	677	695	rBV	3906980	6339966	39.96%	9.256%
3	7.899	811	818	827	rBV	931784	1486204	9.37%	2.170%
4	9.063	1007	1016	1038	rBV	2358328	3977941	25.07%	5.808%
5	10.704	1286	1295	1309	rBV	1216467	2113892	13.32%	3.086%
6	13.157	1704	1712	1727	rBV	6845426	9973468	62.86%	14.561%
7	14.528	1938	1945	1955	rBV	1904042	2943585	18.55%	4.298%
8	16.016	2191	2198	2220	rBV	5214956	7601926	47.91%	11.099%
9	17.280	2406	2413	2427	rBV	2535807	3693830	23.28%	5.393%
10	19.839	2842	2848	2853	rBV	13207842	15867236	100.00%	23.166%
11	21.363	3102	3107	3117	rBV	3201311	4036058	25.44%	5.893%
12	23.780	3512	3518	3533	rVB2	2057995	4083036	25.73%	5.961%




Sum of corrected areas: 68492668

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007097.D
Acq On : 22 Sep 2021 14:20
Operator : CG/JU
Sample : PB139245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

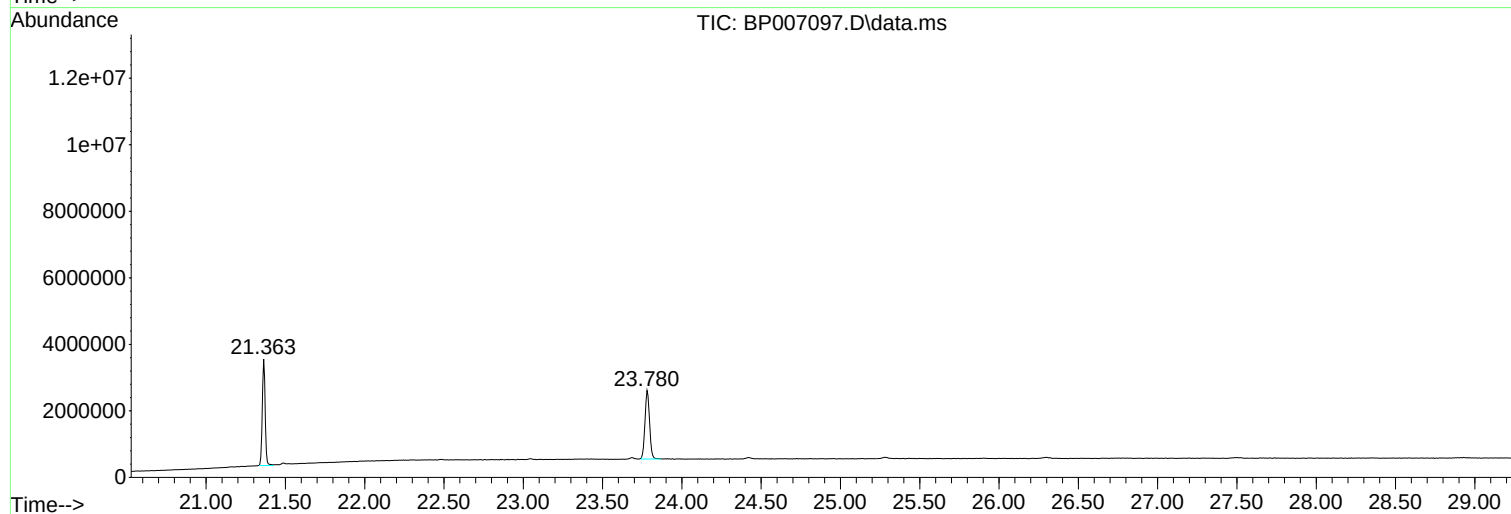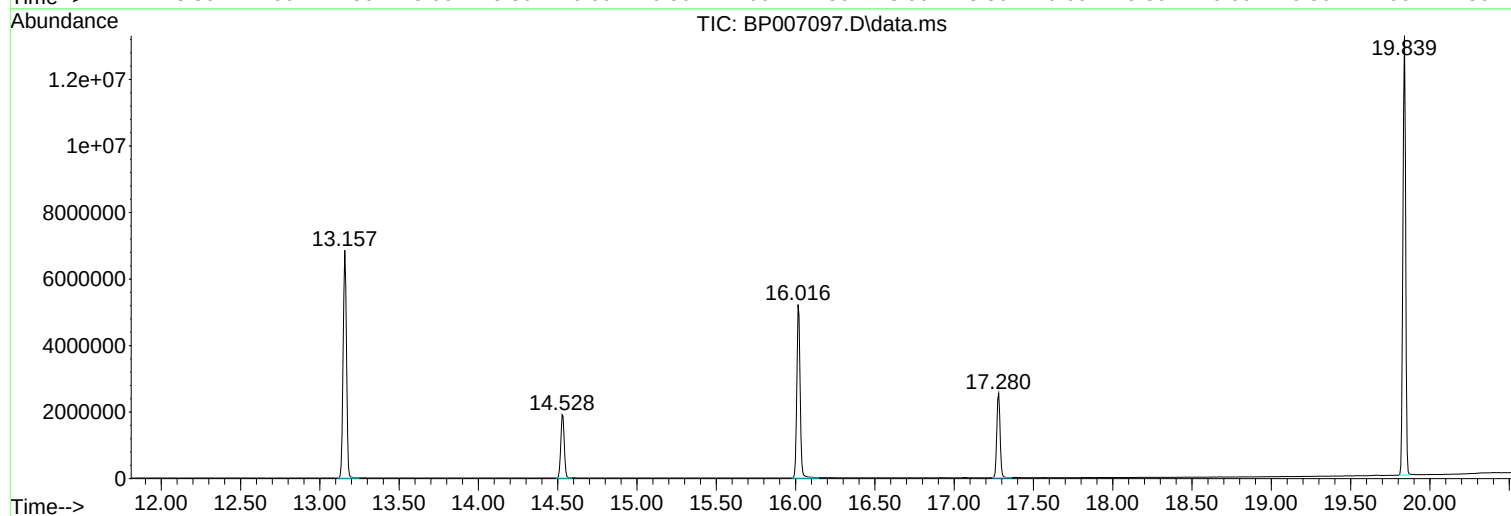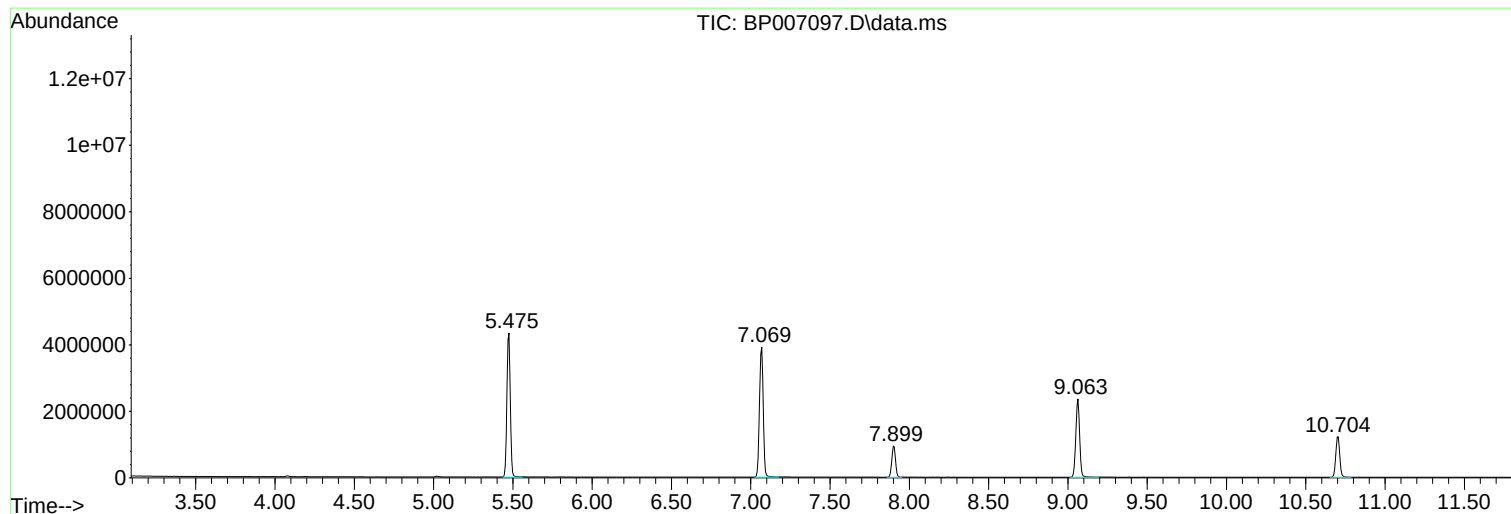

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007097.D
Acq On : 22 Sep 2021 14:20
Operator : CG/JU
Sample : PB139245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007097.D
Acq On : 22 Sep 2021 14:20
Operator : CG/JU
Sample : PB139245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------