
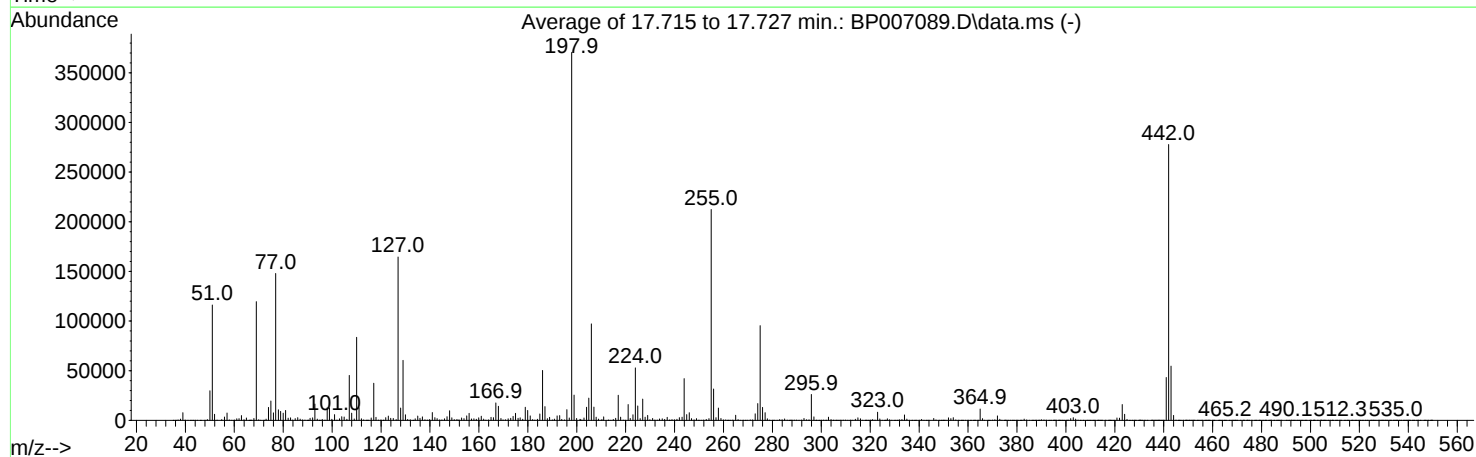


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007089.D
 Acq On : 22 Sep 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 16:50:24 2021

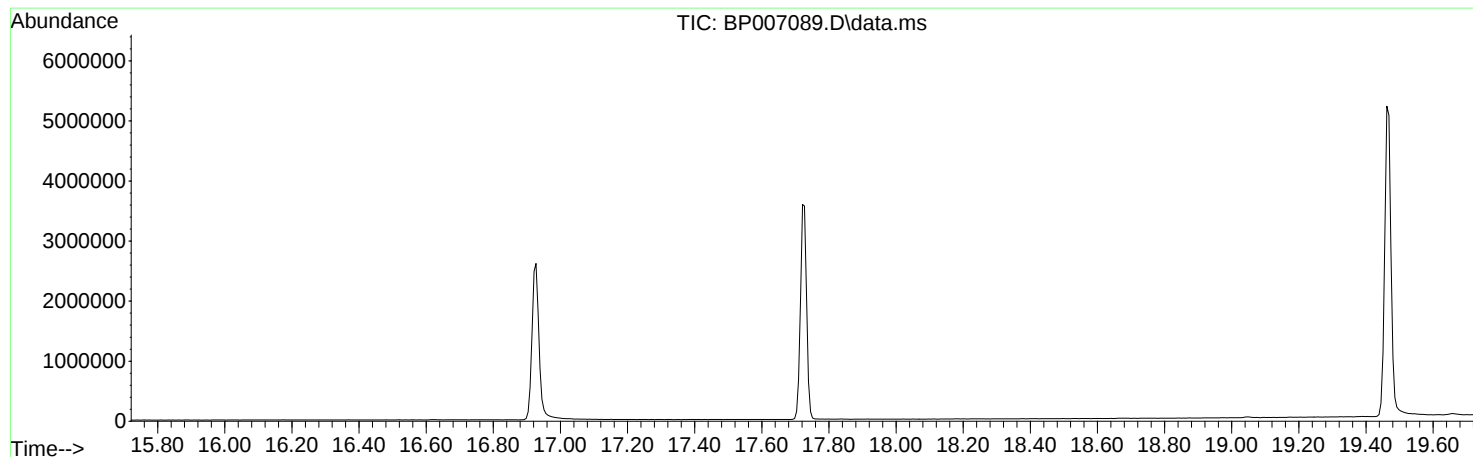

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	116170	PASS
68	69	0.00	2	1.7	1997	PASS
69	198	0.00	100	32.3	119499	PASS
70	69	0.00	2	0.5	652	PASS
127	198	10	80	44.4	164471	PASS
197	198	0.00	2	0.7	2483	PASS
198	198	100	100	100.0	370431	PASS
199	198	5	9	6.9	25419	PASS
275	198	10	60	25.8	95437	PASS
365	198	1	100	3.1	11390	PASS
441	198	0.01	100	11.7	43171	PASS
442	442	100	100	100.0	277794	PASS
443	442	15	24	19.7	54636	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2021	BNA_P	<u>BP007089.D</u>
Compound Name	Response	Retention Time
DDT	1393795	20.66
DDD	3596	20.23
DDE	1459	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5055	1398850	0.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007089.D
 Acq On : 22 Sep 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 11:31:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 16:50:24 2021
 Response via : Initial Calibration

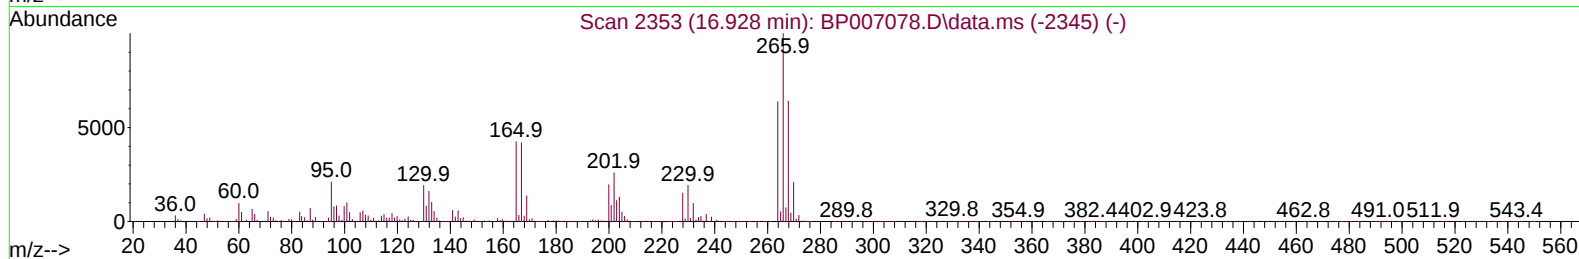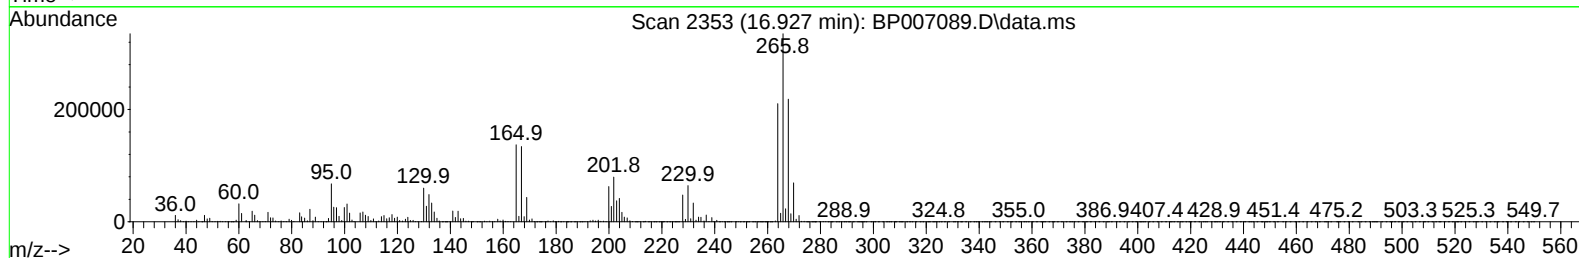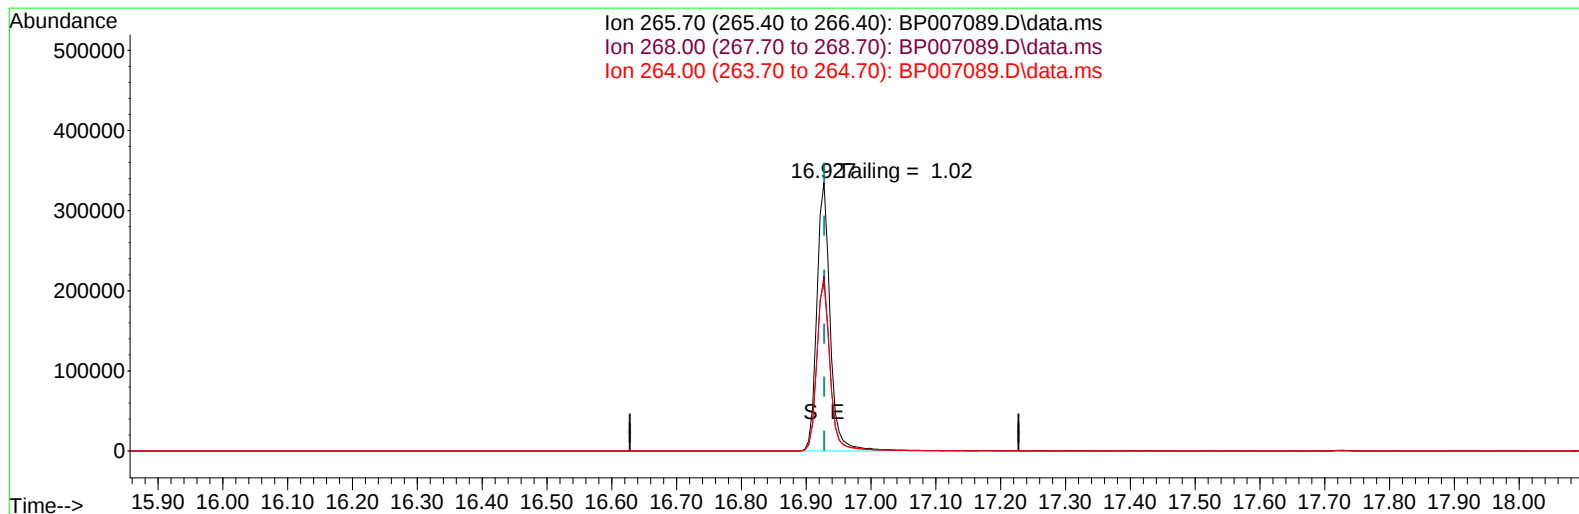

TIC: BP007089.D\data.ms

(70) Pentachlorophenol (C)

16.927min (-0.000) 3559193.41 ng




response 481922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.17
264.00	62.90	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007089.D
 Acq On : 22 Sep 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 11:31:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 16:50:24 2021
 Response via : Initial Calibration

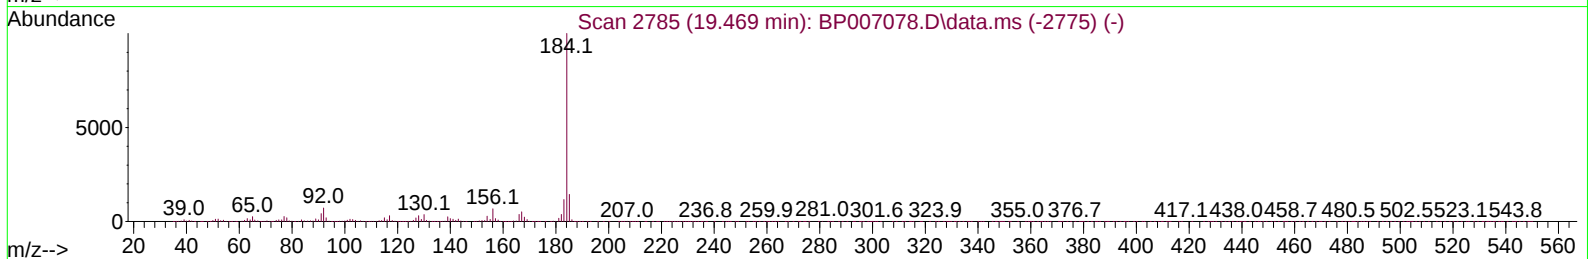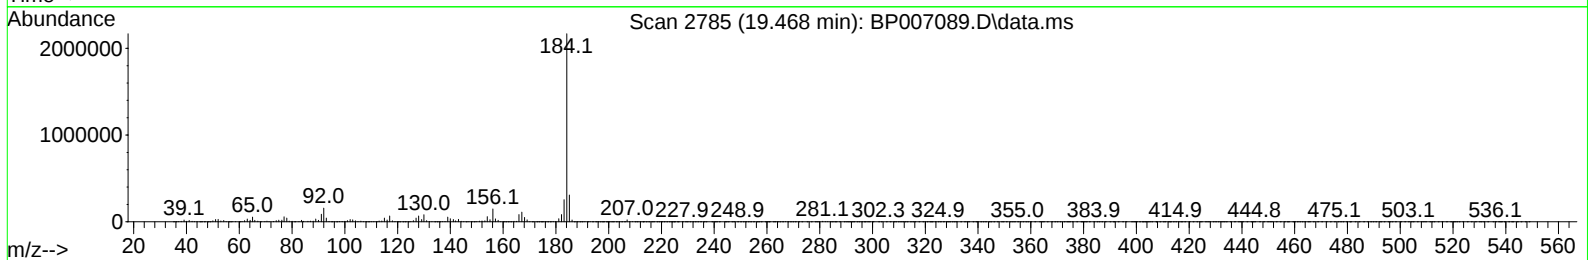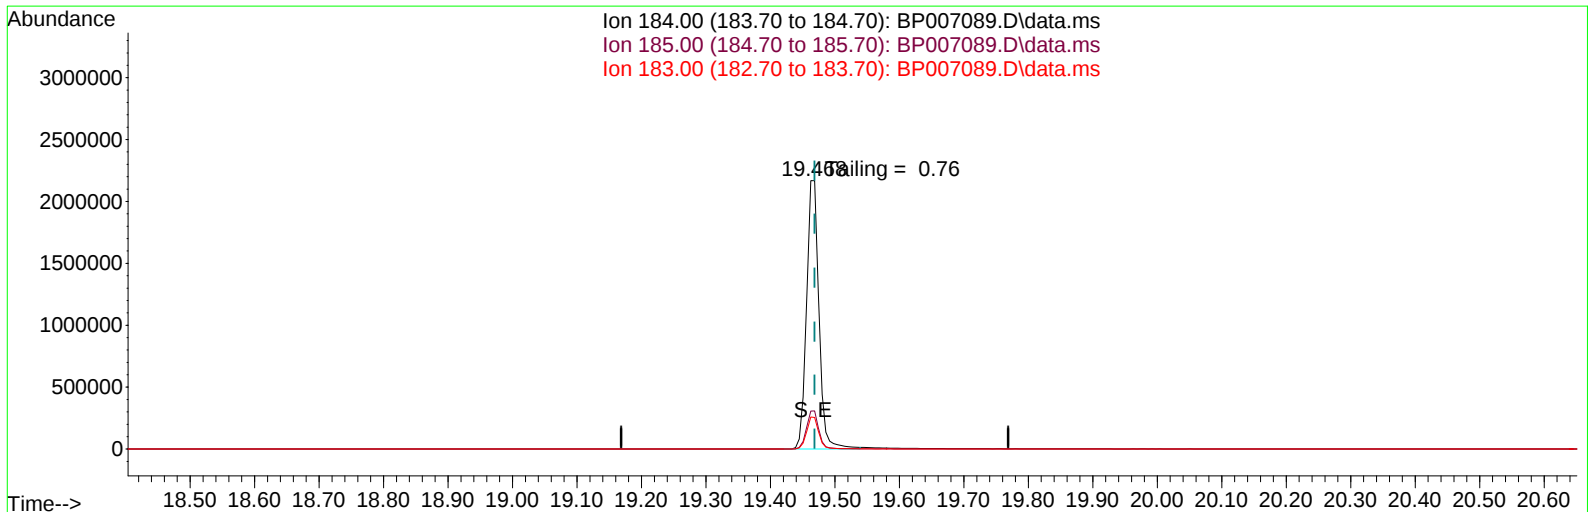

TIC: BP007089.D\data.ms

(77) Benzidine

19.468min (-0.000) 704682.65 ng

response 2945216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.23
183.00	11.90	11.78
0.00	0.00	0.00