
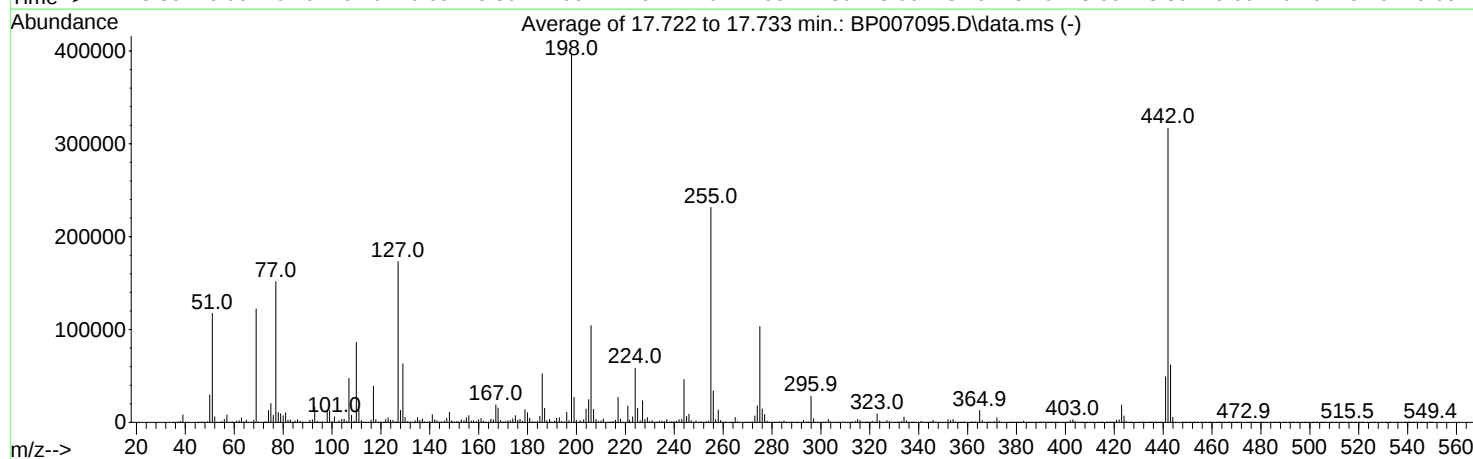


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007095.D
 Acq On : 22 Sep 2021 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 16:50:24 2021

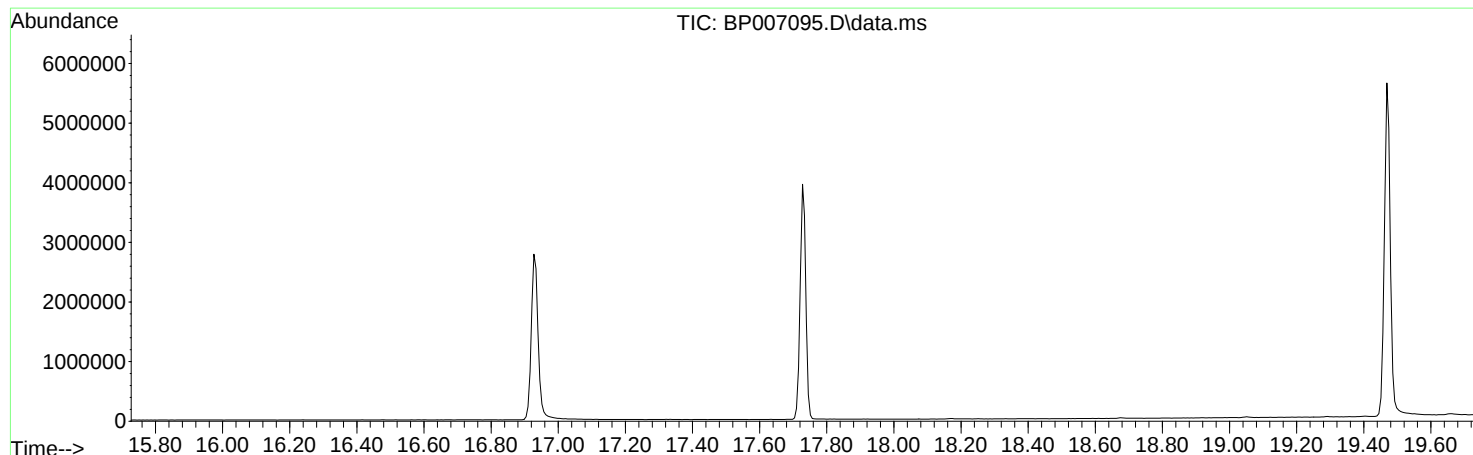

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	117311	PASS
68	69	0.00	2	1.8	2174	PASS
69	198	0.00	100	30.9	122268	PASS
70	69	0.00	2	0.5	578	PASS
127	198	10	80	43.7	173243	PASS
197	198	0.00	2	0.5	1852	PASS
198	198	100	100	100.0	396224	PASS
199	198	5	9	6.8	26835	PASS
275	198	10	60	26.1	103300	PASS
365	198	1	100	3.3	12923	PASS
441	198	0.01	100	12.4	49117	PASS
442	442	100	100	100.0	316854	PASS
443	442	15	24	19.5	61877	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2021	BNA_P	<u>BP007095.D</u>
Compound Name	Response	Retention Time
DDT	1428184	20.67
DDD	5183	20.24
DDE	1578	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6761	1434945	0.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
Data File : BP007095.D
Acq On : 22 Sep 2021 13:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 22 14:19:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 16:50:24 2021
Response via : Initial Calibration

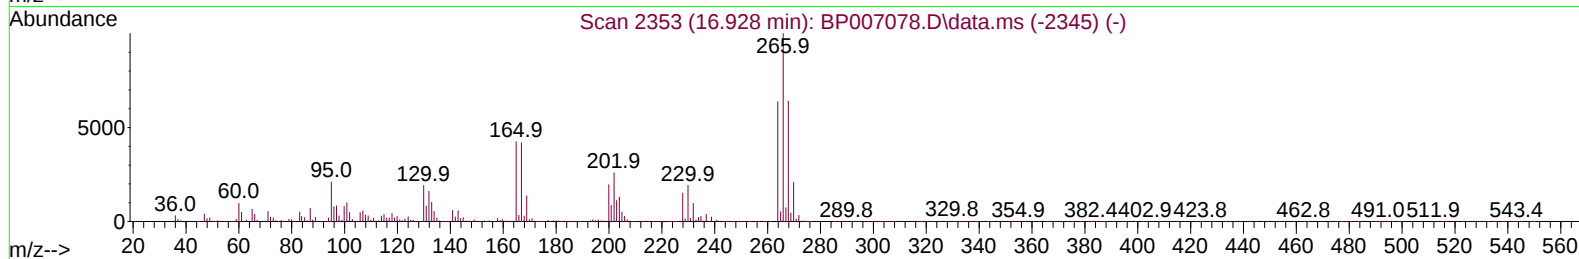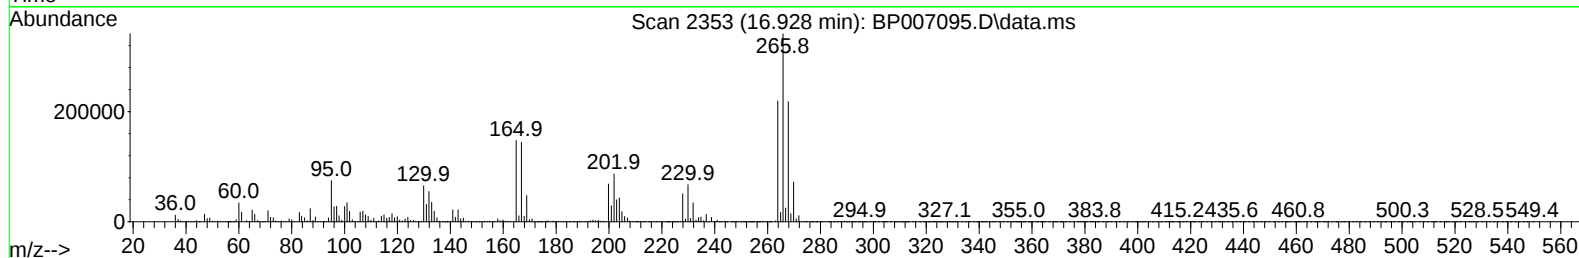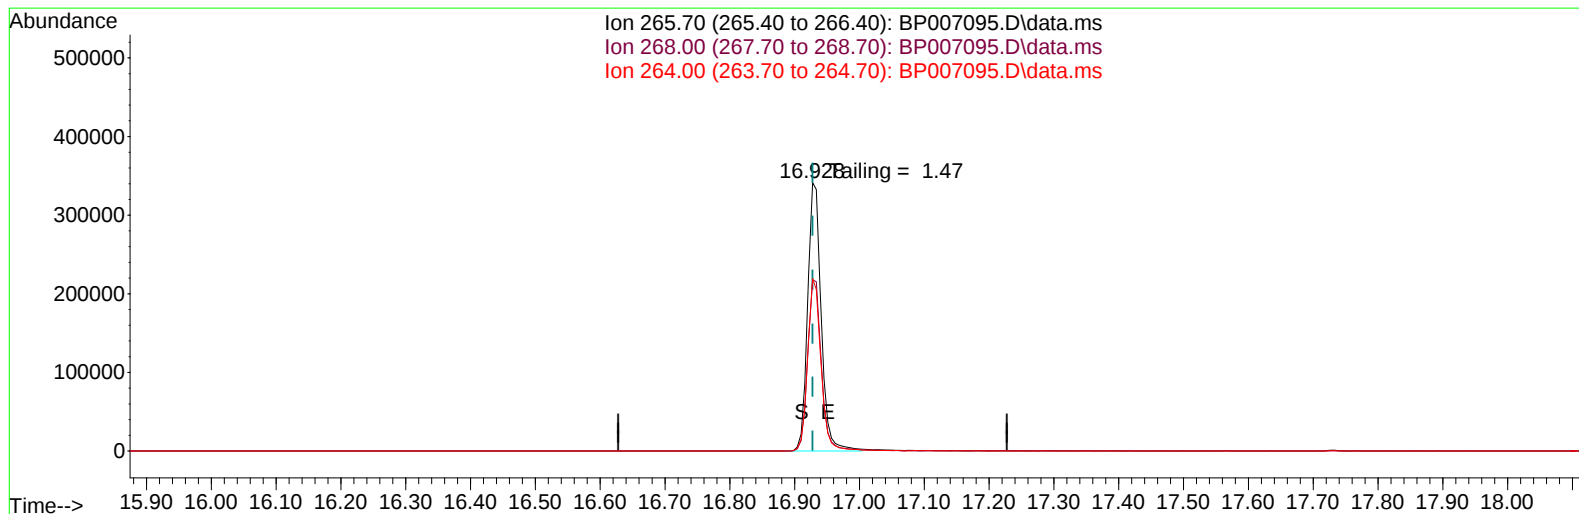

TIC: BP007095.D\data.ms

(70) Pentachlorophenol (C)

16.928min (-0.000) 67839.39 ng




response 501125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.80
264.00	62.90	64.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092221\
 Data File : BP007095.D
 Acq On : 22 Sep 2021 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 14:19:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 16:50:24 2021
 Response via : Initial Calibration

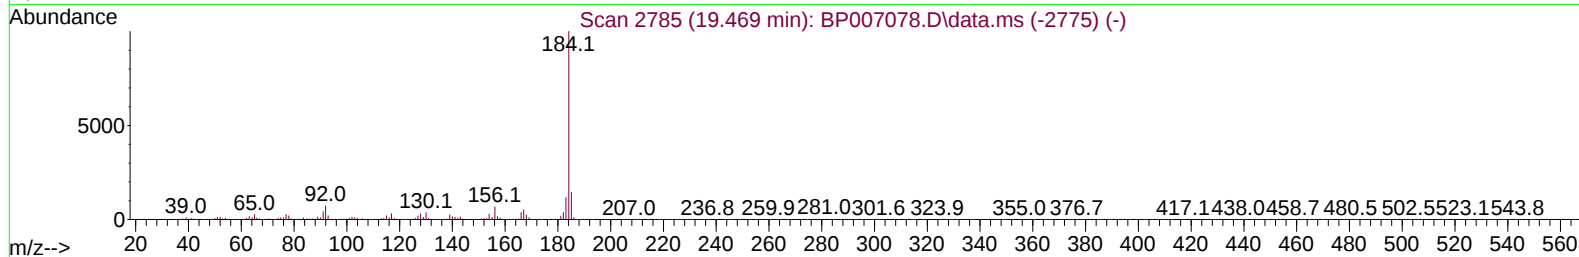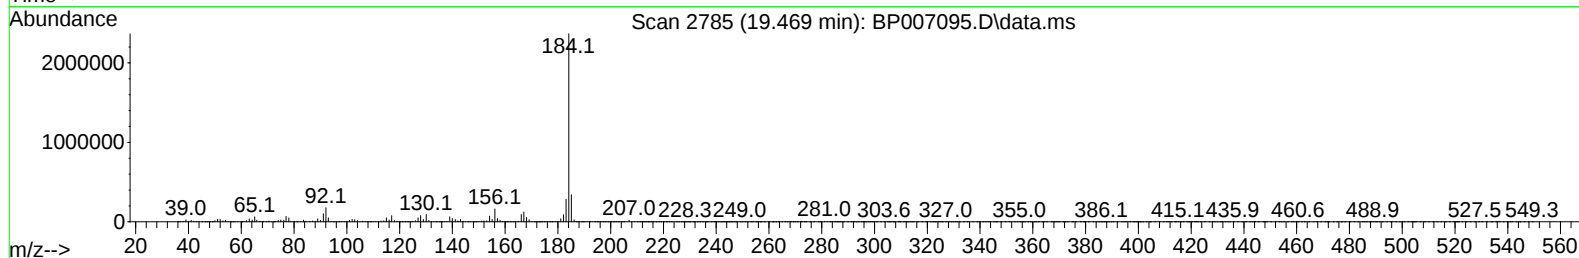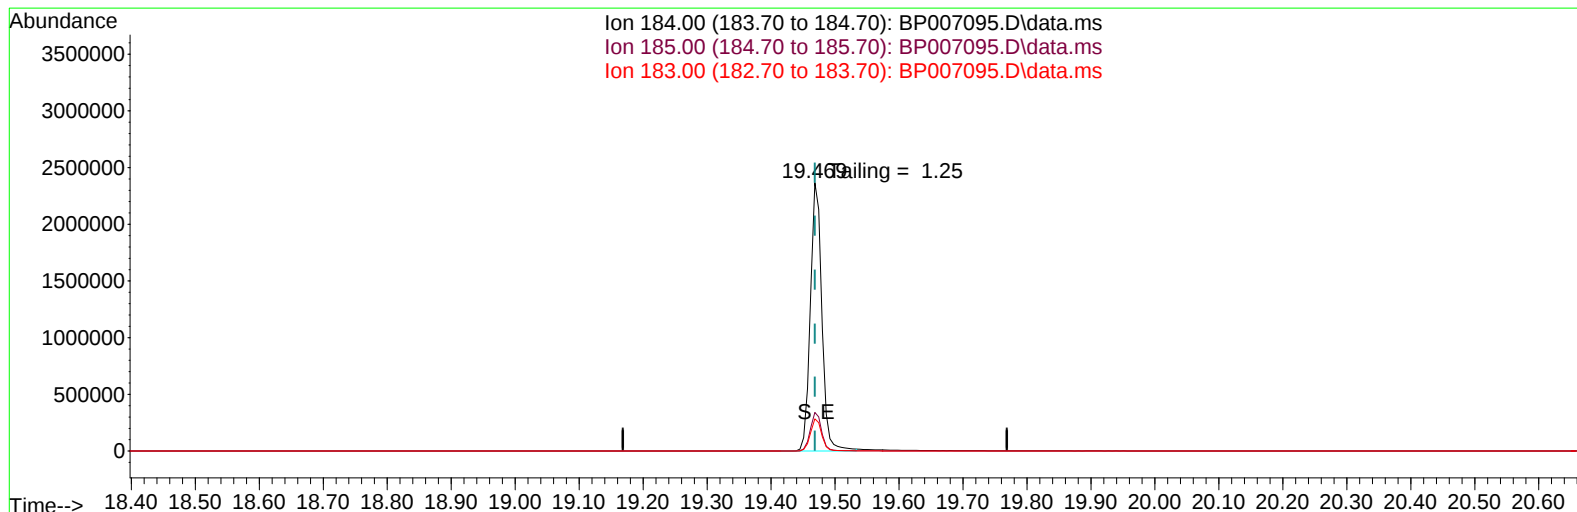

TIC: BP007095.D\data.ms

(77) Benzidine

19.469min (-0.000) 39704.98 ng

response 3034628

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.37
183.00	11.90	11.98
0.00	0.00	0.00