
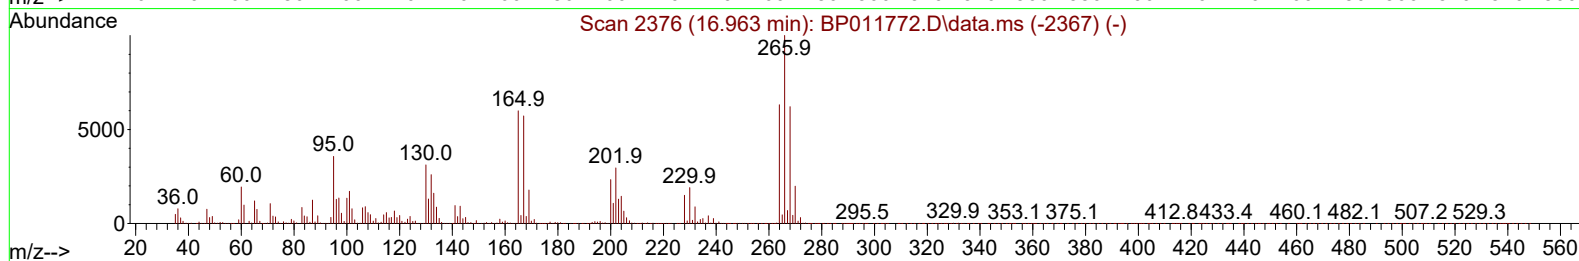
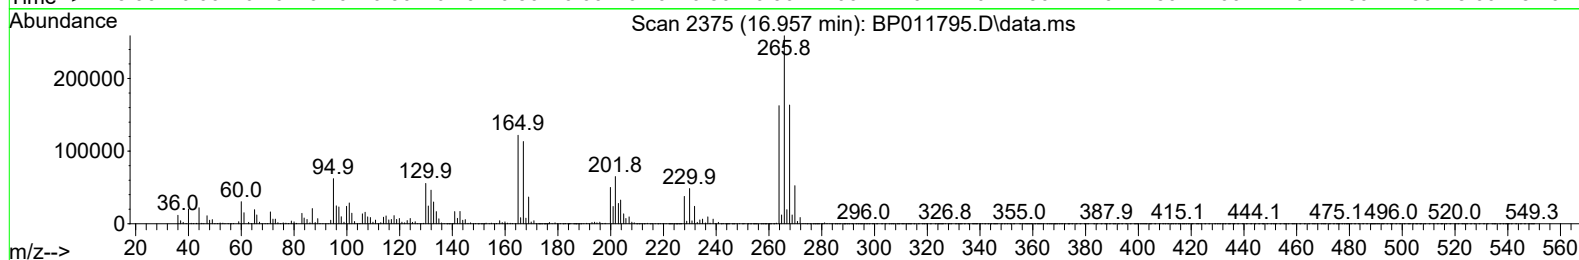


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
 Data File : BP011795.D
 Acq On : 26 Sep 2022 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 07:03:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

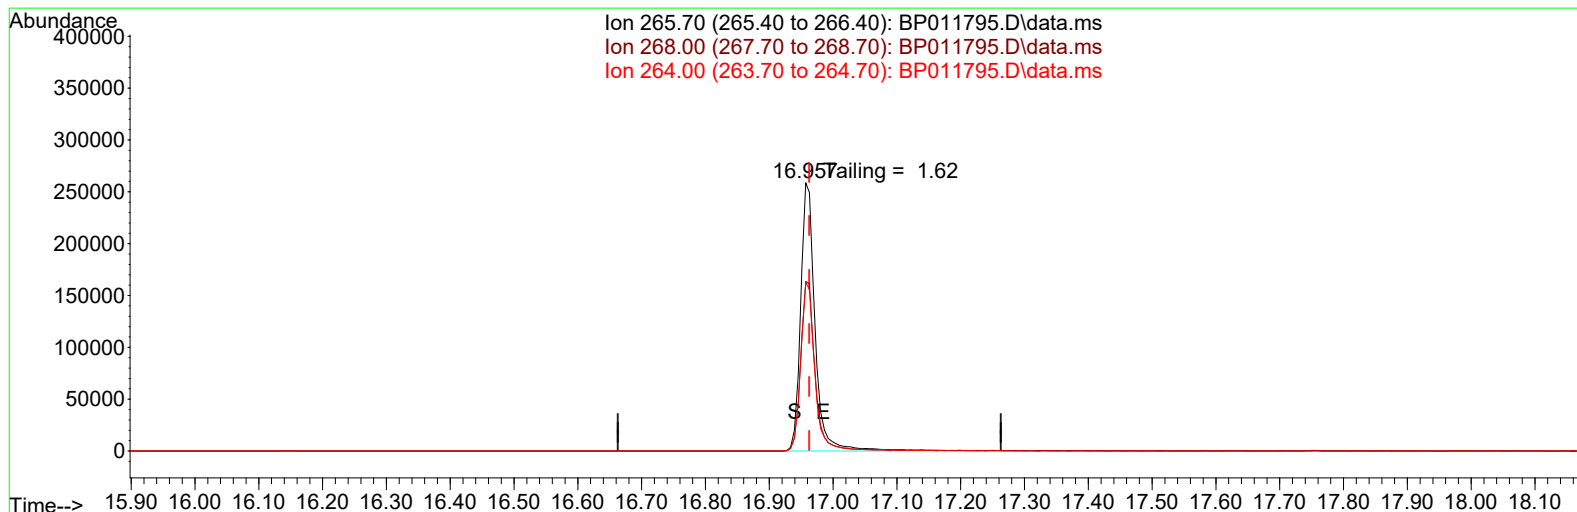

TIC: BP011795.D\data.ms

(70) Pentachlorophenol (C)




16.957min (-0.006) 2212835.06 ng

response 410932

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	63.19
264.00	63.20	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
 Data File : BP011795.D
 Acq On : 26 Sep 2022 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 07:03:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

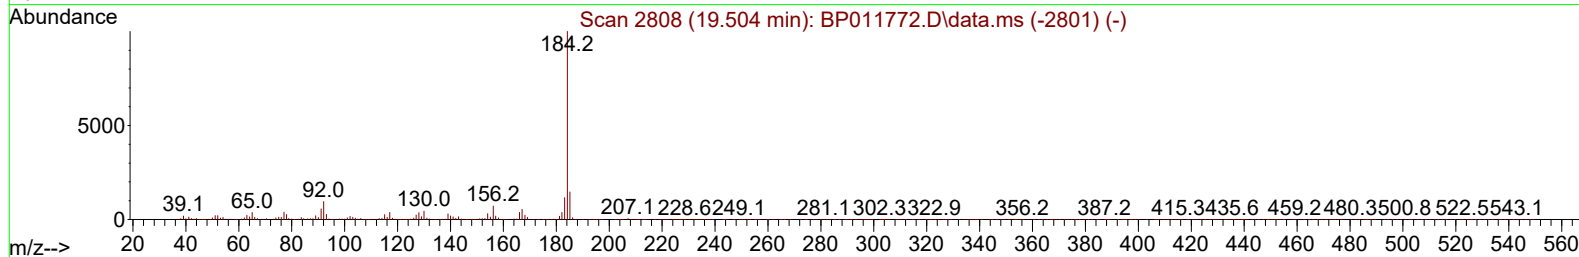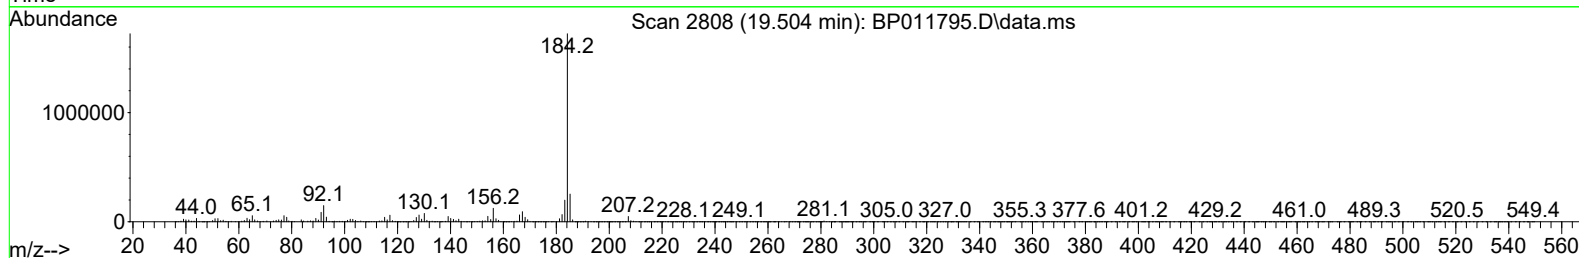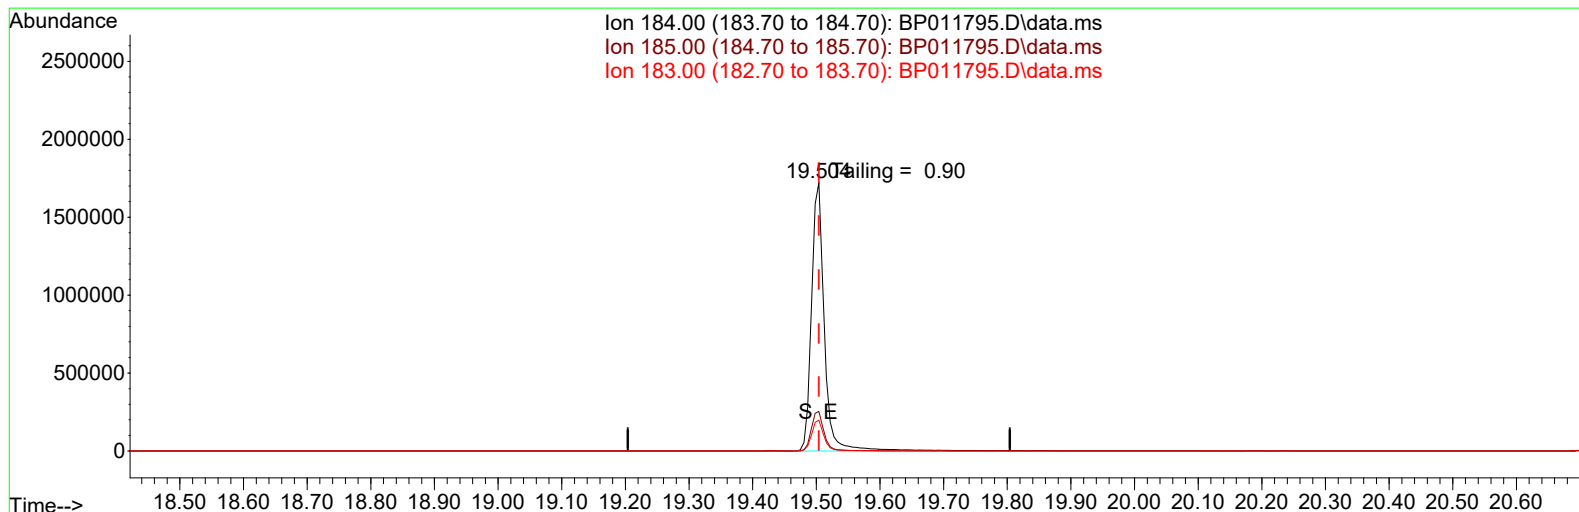

TIC: BP011795.D\data.ms

(77) Benzidine

19.504min (+ 0.000) 2698703.54 ng

response 2409321

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.75
183.00	11.60	11.50
0.00	0.00	0.00