

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
 Data File : BP011798.D
 Acq On : 26 Sep 2022 15:50
 Operator : CG/JU
 Sample : PB147874TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB147874TB

Quant Time: Sep 27 03:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 02:45:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	266954	20.000	ng	-0.01
21) Naphthalene-d8	10.722	136	1170414	20.000	ng	-0.01
39) Acenaphthene-d10	14.557	164	706353	20.000	ng	-0.01
64) Phenanthrene-d10	17.316	188	1499183	20.000	ng	0.00
76) Chrysene-d12	21.398	240	1337431	20.000	ng	0.00
86) Perylene-d12	23.845	264	1320497	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	2463571	161.922	ng	0.00
7) Phenol-d6	7.075	99	3256379	144.752	ng	0.00
23) Nitrobenzene-d5	9.081	82	1823638	81.553	ng	-0.01
42) 2,4,6-Tribromophenol	16.051	330	744426	156.517	ng	0.00
45) 2-Fluorobiphenyl	13.181	172	4092134	91.615	ng	-0.01
79) Terphenyl-d14	19.869	244	5908397	101.578	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
Data File : BP011798.D
Acq On : 26 Sep 2022 15:50
Operator : CG/JU
Sample : PB147874TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147874TB

Quant Time: Sep 27 03:19:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 02:45:14 2022
Response via : Initial Calibration




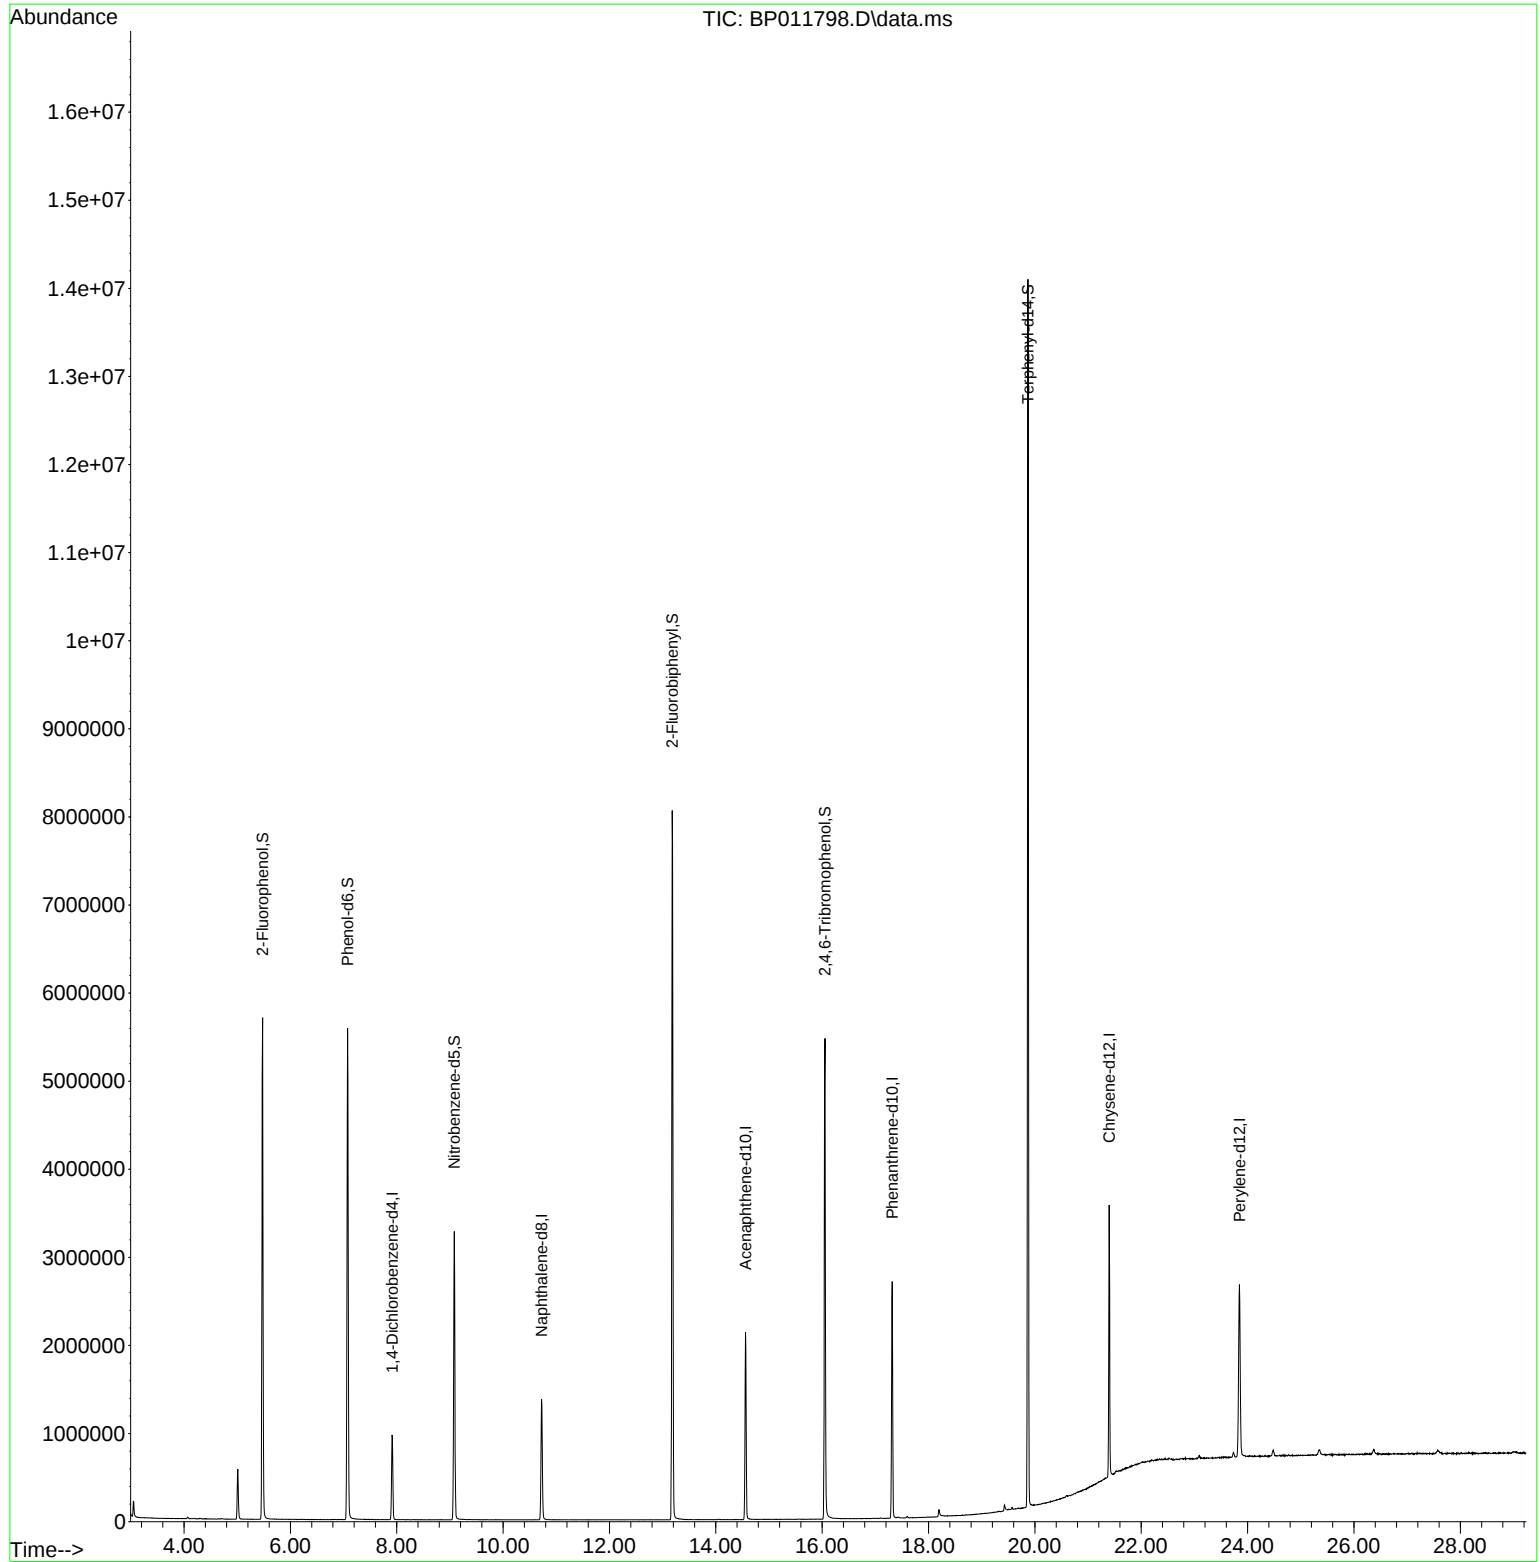


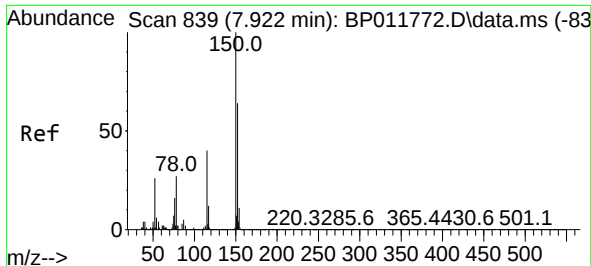

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.911 min Scan# 839
Delta R.T. -0.011 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50




Instrument :
BNA_P
ClientSampleId :
PB147874TB


Tgt Ion:152 Resp: 266954
Ion Ratio Lower Upper
152 100
150 160.7 124.2 186.4
115 61.1 50.0 75.0

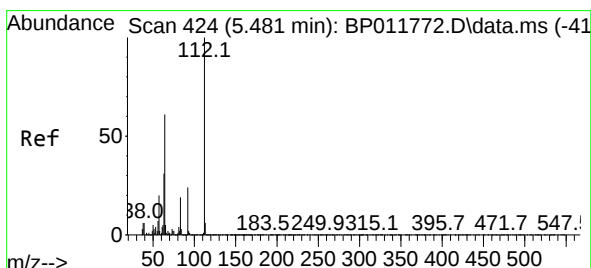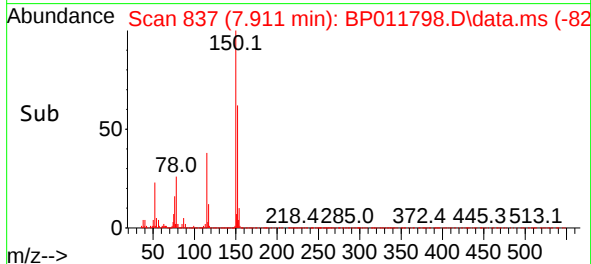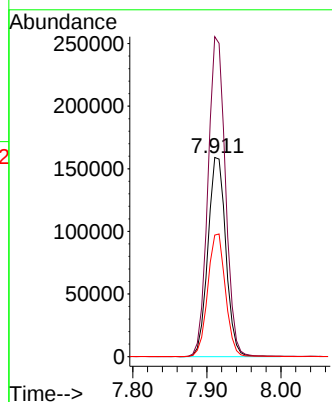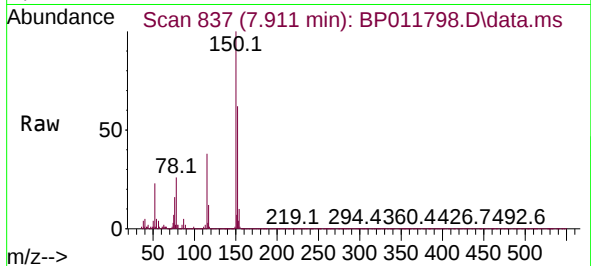

#5
2-Fluorophenol
Concen: 161.922 ng
RT: 5.475 min Scan# 423
Delta R.T. -0.006 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50

Tgt Ion:112 Resp: 2463571
Ion Ratio Lower Upper
112 100
64 59.9 49.2 73.8
63 30.5 25.2 37.8


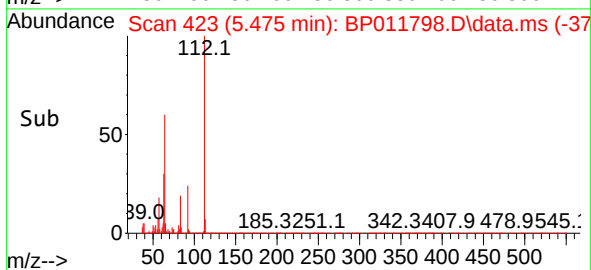
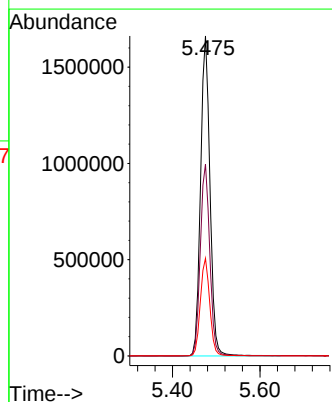
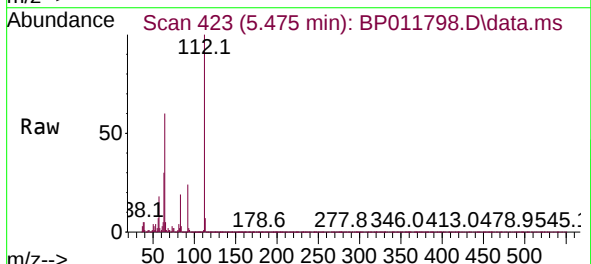


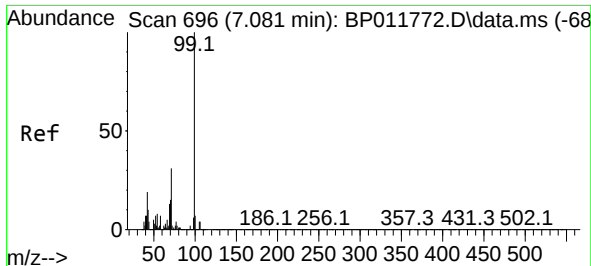

#7
Phenol-d6
Concen: 144.752 ng
RT: 7.075 min Scan# 69
Delta R.T. -0.006 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50




Instrument :
BNA_P
ClientSampleId :
PB147874TB


Tgt Ion: 99 Resp: 3256379
Ion Ratio Lower Upper
99 100
42 17.1 15.4 23.2
71 30.9 24.7 37.1

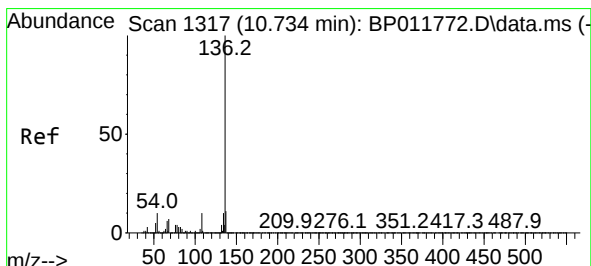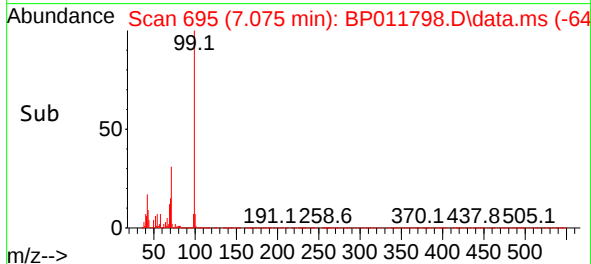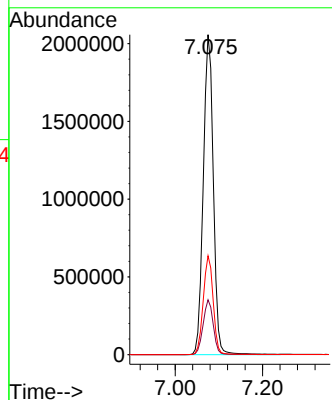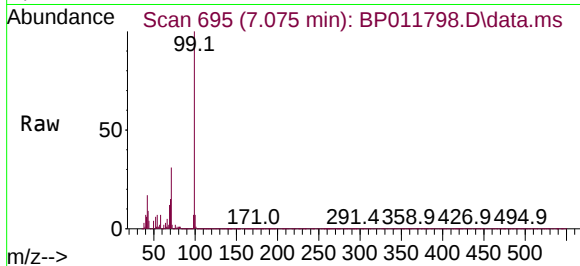

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.722 min Scan# 1315
Delta R.T. -0.012 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50

Tgt Ion: 136 Resp: 1170414
Ion Ratio Lower Upper
136 100
137 10.9 8.8 13.2
54 9.7 8.2 12.4
68 7.3 5.8 8.8


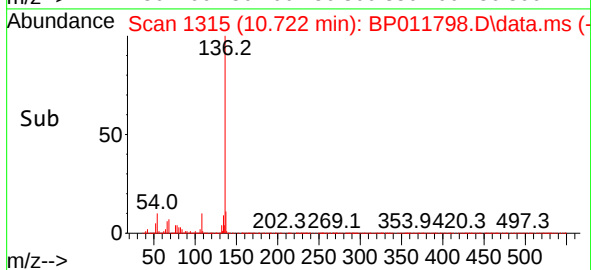
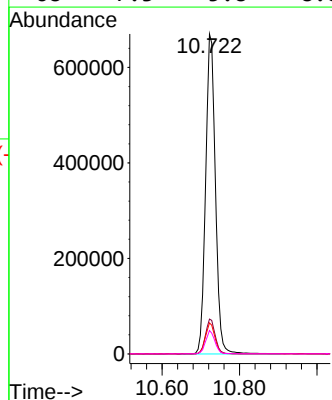
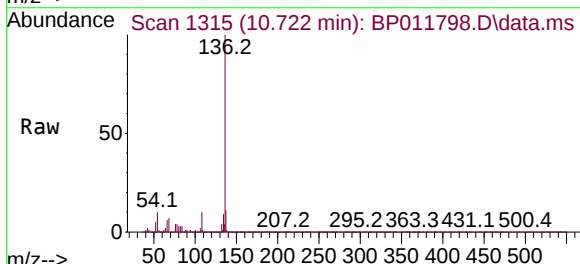


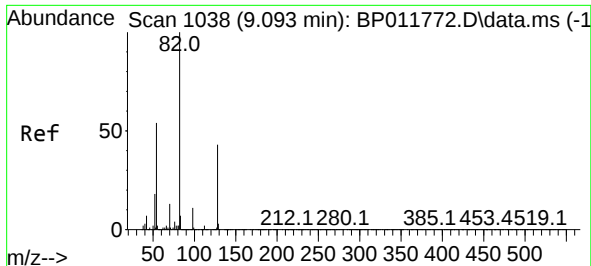

#23
Nitrobenzene-d5
Concen: 81.553 ng
RT: 9.081 min Scan# 10
Delta R.T. -0.012 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50




Instrument :
BNA_P
ClientSampleId :
PB147874TB


Tgt Ion: 82 Resp: 1823638
Ion Ratio Lower Upper
82 100
128 42.5 34.2 51.4
54 51.6 43.1 64.7

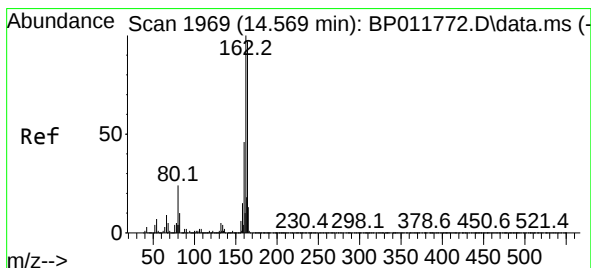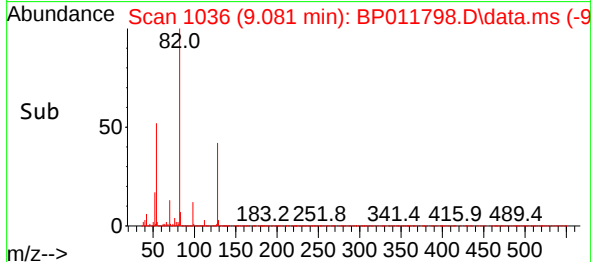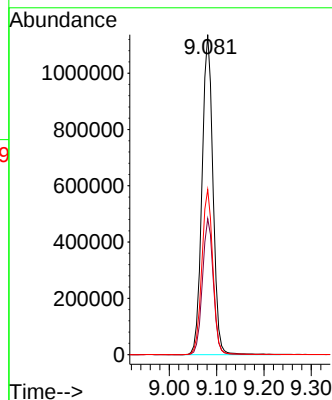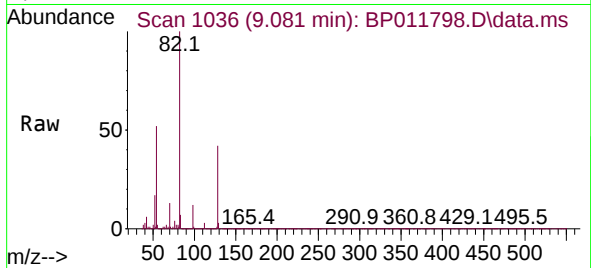

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.557 min Scan# 1967
Delta R.T. -0.012 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50

Tgt Ion:164 Resp: 706353
Ion Ratio Lower Upper
164 100
162 103.0 82.5 123.7
160 46.8 37.8 56.6


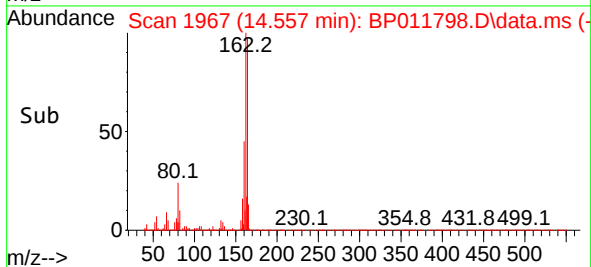
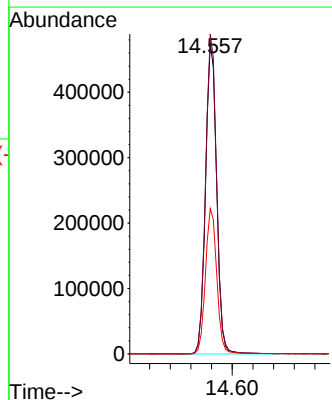
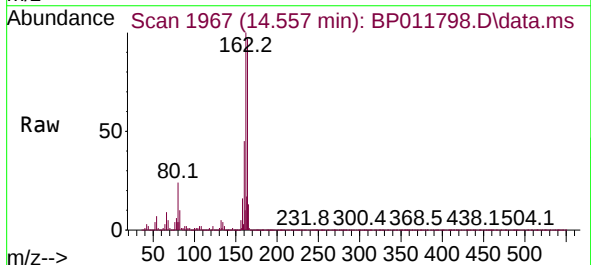


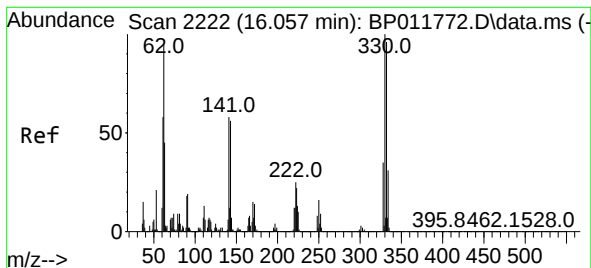

#42
 2,4,6-Tribromophenol
 Concen: 156.517 ng
 RT: 16.051 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP011798.D
 Acq: 26 Sep 2022 15:50




Instrument :
 BNA_P
 ClientSampleId :
 PB147874TB


Tgt Ion:330 Resp: 744426
 Ion Ratio Lower Upper
 330 100
 332 95.1 76.6 114.8
 141 55.6 48.7 73.1

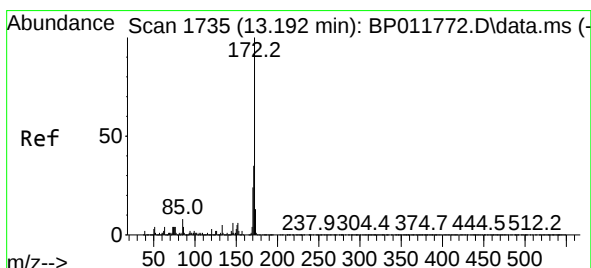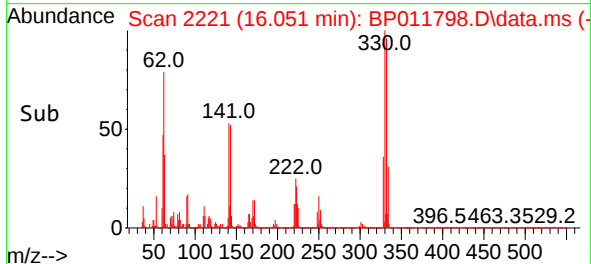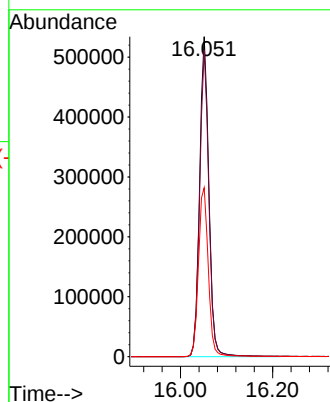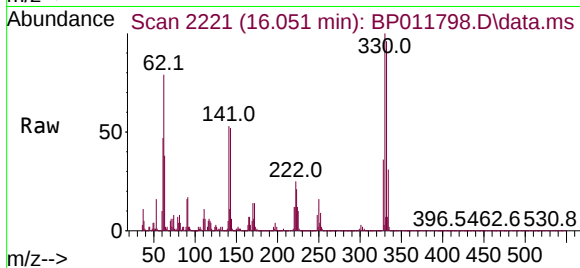

#45
 2-Fluorobiphenyl
 Concen: 91.615 ng
 RT: 13.181 min Scan# 1733
 Delta R.T. -0.012 min
 Lab File: BP011798.D
 Acq: 26 Sep 2022 15:50

Tgt Ion:172 Resp: 4092134
 Ion Ratio Lower Upper
 172 100
 171 35.6 27.9 41.9
 170 24.4 19.5 29.3


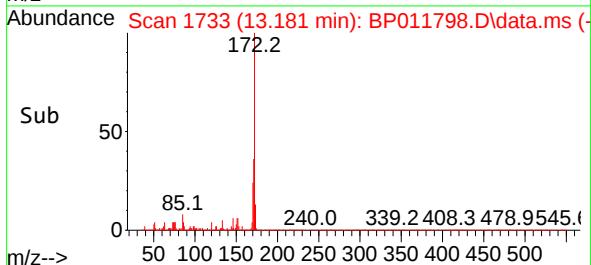
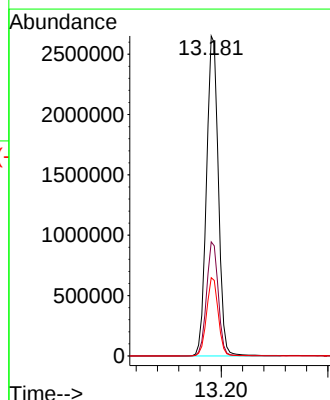
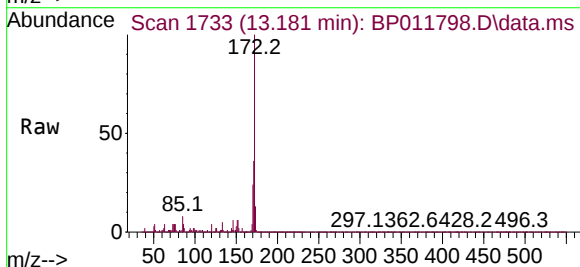


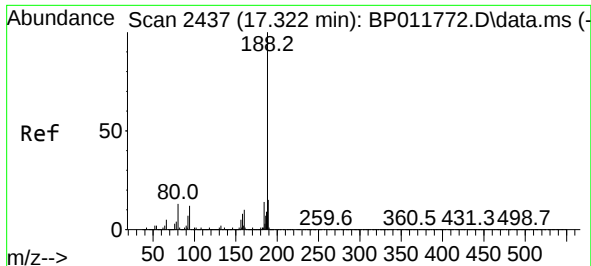

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.316 min Scan# 24
Delta R.T. -0.006 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50




Instrument :
BNA_P
ClientSampleId :
PB147874TB


Tgt Ion:188 Resp: 1499183
Ion Ratio Lower Upper
188 100
94 11.5 9.4 14.0
80 12.4 10.6 15.8

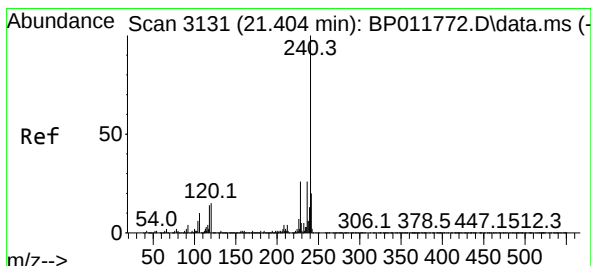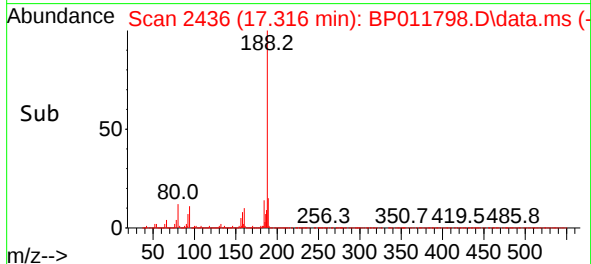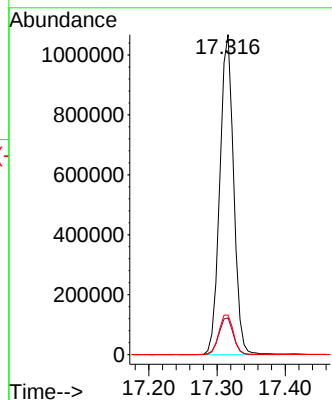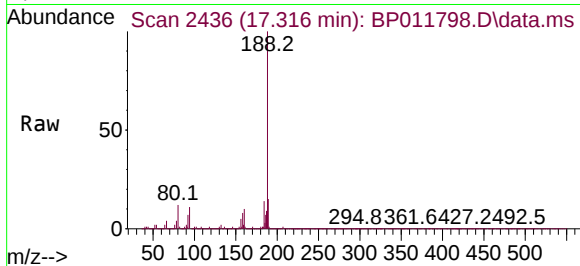

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.398 min Scan# 3130
Delta R.T. -0.006 min
Lab File: BP011798.D
Acq: 26 Sep 2022 15:50

Tgt Ion:240 Resp: 1337431
Ion Ratio Lower Upper
240 100
120 14.9 12.0 18.0
236 26.0 21.1 31.7

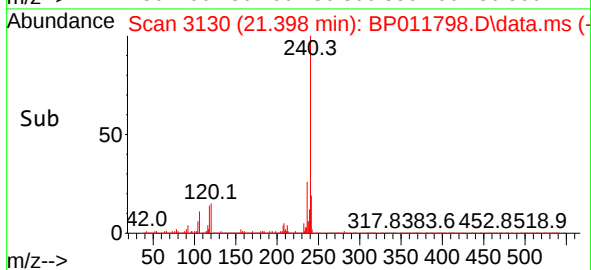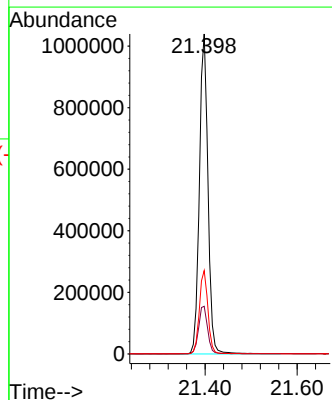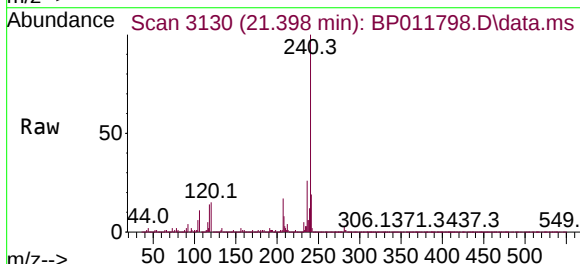

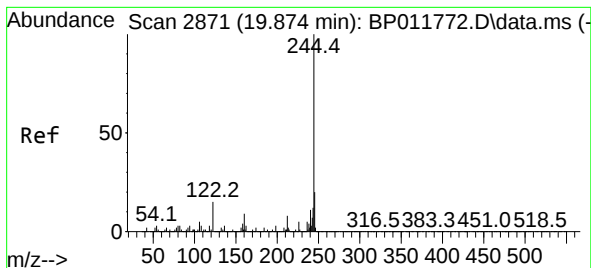

#79

Terphenyl-d14

Concen: 101.578 ng

RT: 19.869 min Scan# 2871

Delta R.T. -0.006 min

Lab File: BP011798.D

Acq: 26 Sep 2022 15:50

Instrument :

BNA_P

ClientSampleId :

PB147874TB





Tgt Ion:244 Resp: 5908397

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7

122 15.1 11.8 17.8

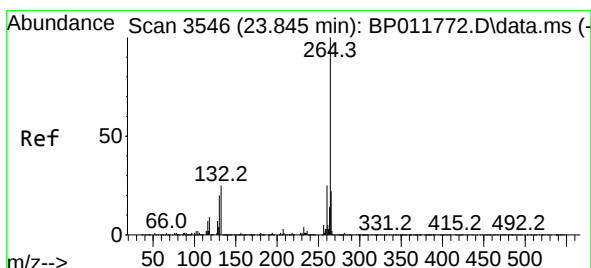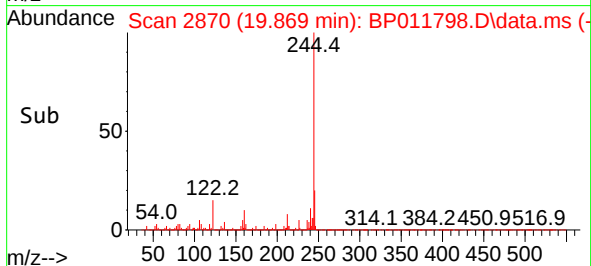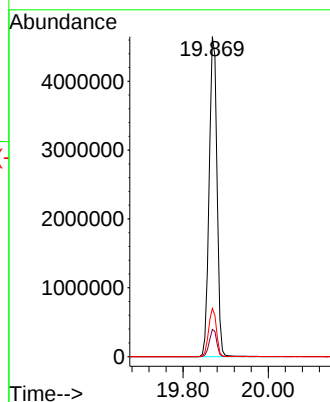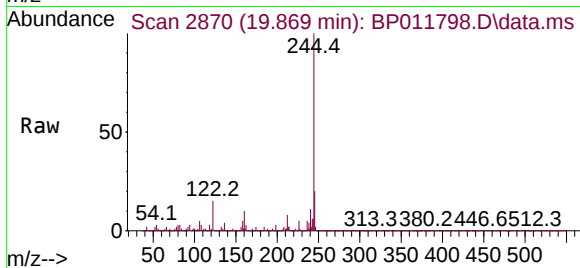

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.845 min Scan# 3546

Delta R.T. 0.000 min

Lab File: BP011798.D

Acq: 26 Sep 2022 15:50

Tgt Ion:264 Resp: 1320497

Ion Ratio Lower Upper

264 100

260 24.6 19.7 29.5

265 22.4 17.8 26.8

