
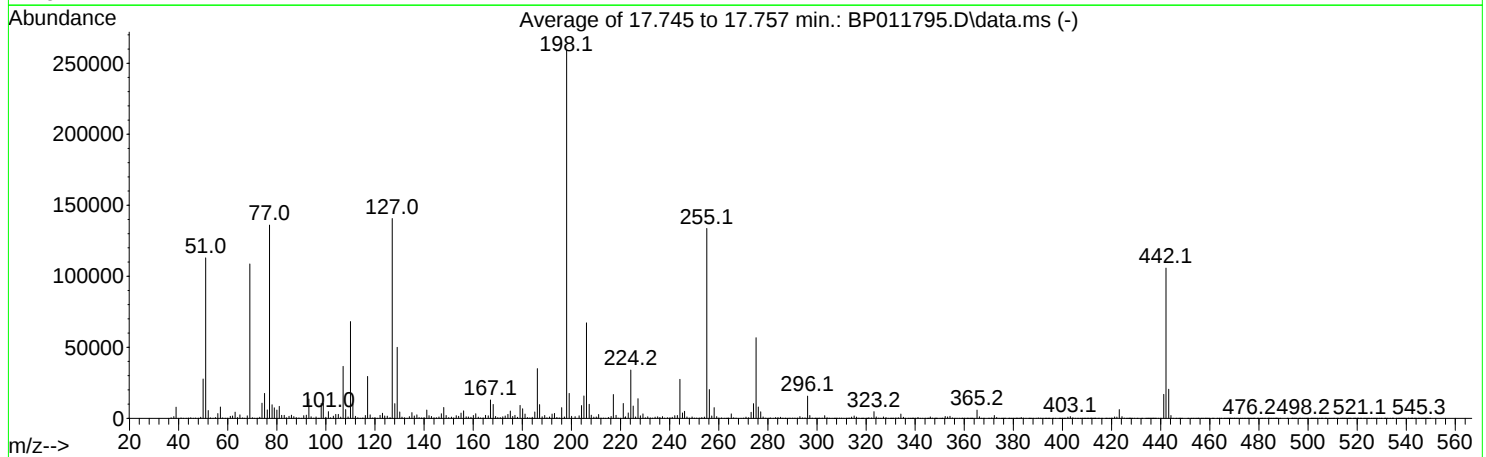


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
 Data File : BP011795.D
 Acq On : 26 Sep 2022 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 22 02:45:14 2022

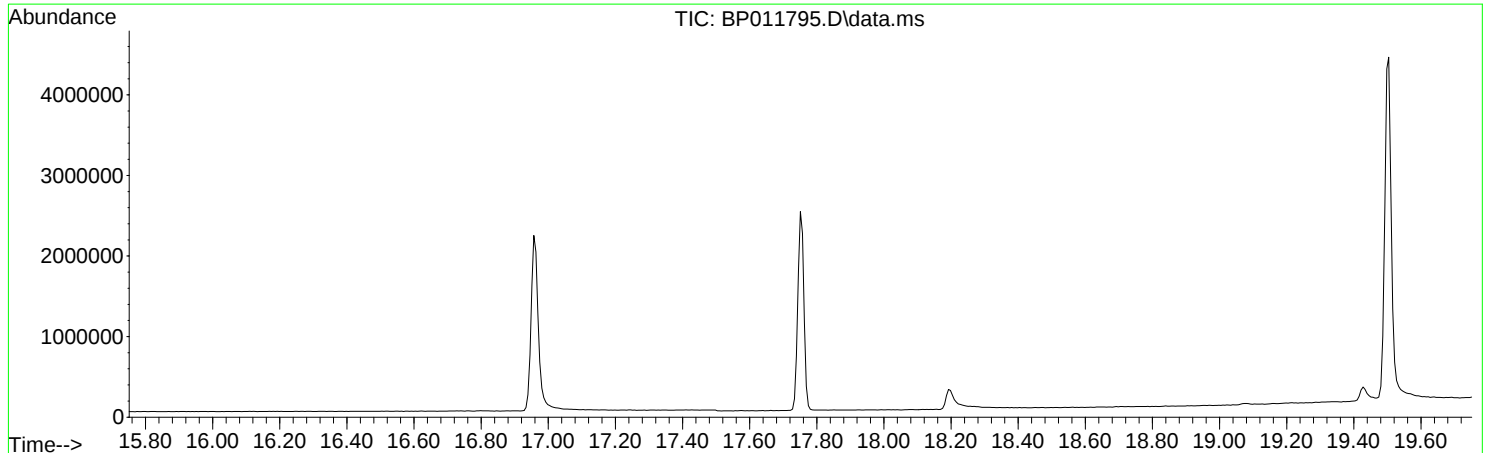




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	112922	PASS
68	69	0.00	2	1.6	1706	PASS
69	198	0.00	100	42.0	108687	PASS
70	69	0.00	2	0.4	402	PASS
127	198	10	80	54.3	140694	PASS
197	198	0.00	2	0.4	954	PASS
198	198	100	100	100.0	259028	PASS
199	198	5	9	6.8	17565	PASS
275	198	10	60	21.9	56717	PASS
365	198	1	100	2.3	5836	PASS
441	198	0.01	100	6.5	16838	PASS
442	442	100	100	100.0	105796	PASS
443	442	15	24	19.3	20428	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
Data File : BP011795.D
Acq On : 26 Sep 2022 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 27 07:03:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 02:45:14 2022
Response via : Initial Calibration

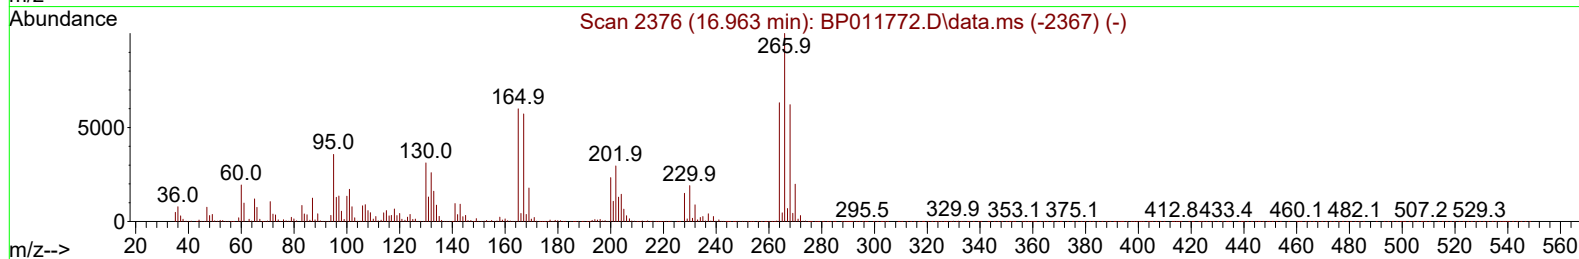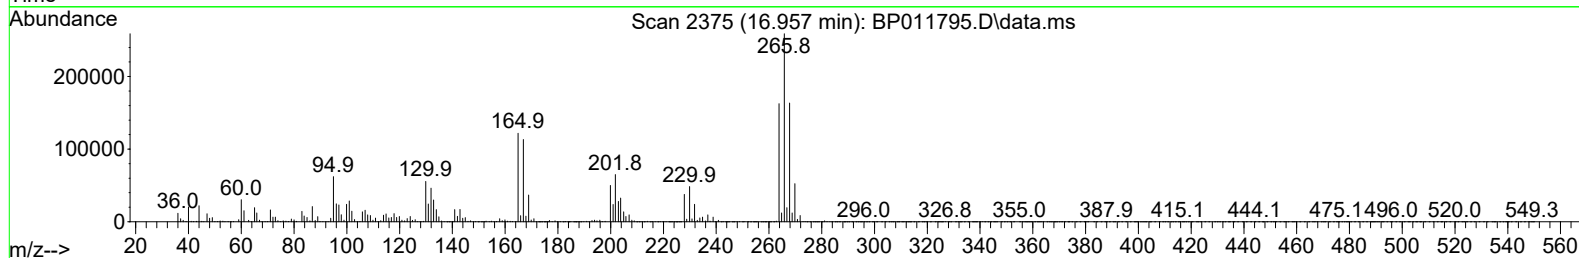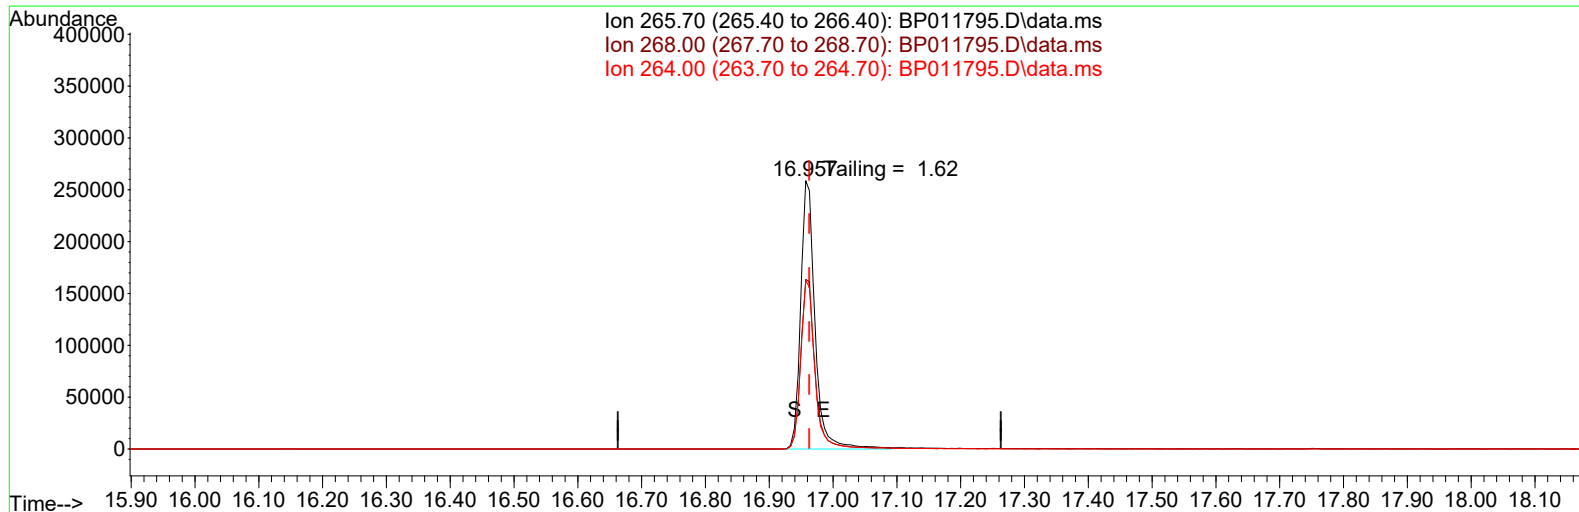

TIC: BP011795.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.006) 2212835.06 ng




response 410932

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	63.19
264.00	63.20	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092622\
Data File : BP011795.D
Acq On : 26 Sep 2022 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 27 07:03:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 02:45:14 2022
Response via : Initial Calibration

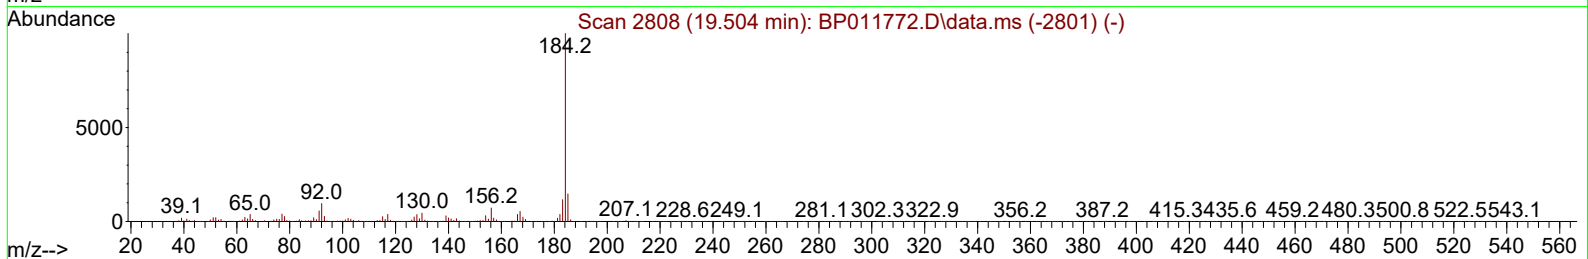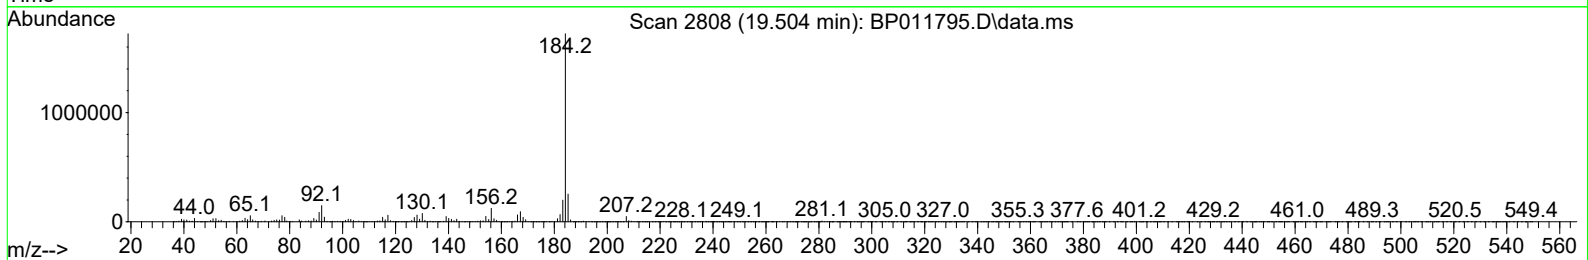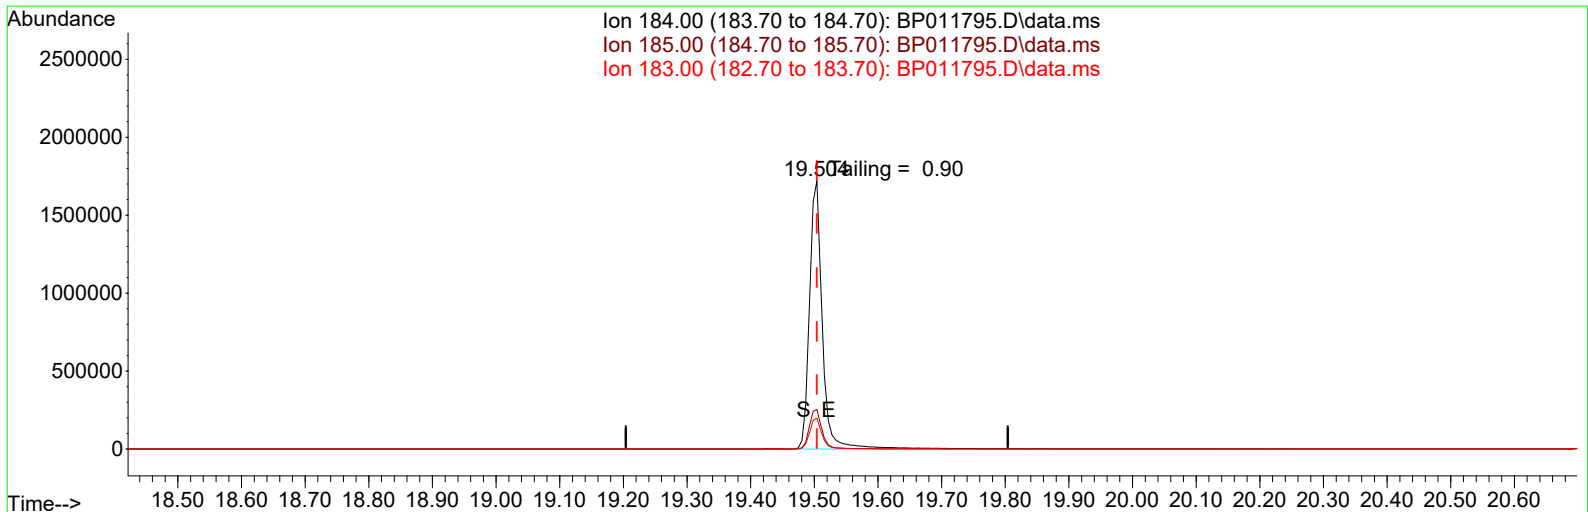

TIC: BP011795.D\data.ms

(77) Benzidine

19.504min (+ 0.000) 2698703.54 ng

response 2409321

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.75
183.00	11.60	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2022	BNA_P	<u>BP011795.D</u>
Compound Name	Response	Retention Time
DDT	936967	20.704
DDD	11546	20.269
DDE	2643	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14189	951156	1.49

Instrument :
BNA_P
ClientSampleId :
DFTPP