
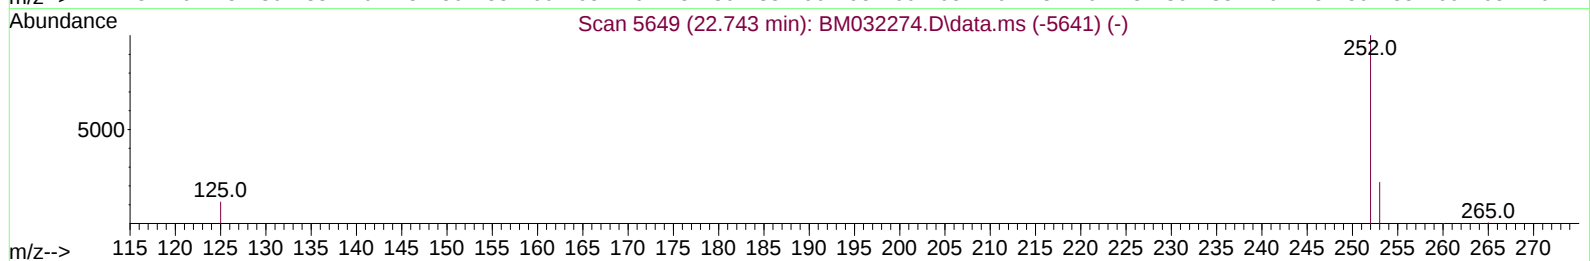
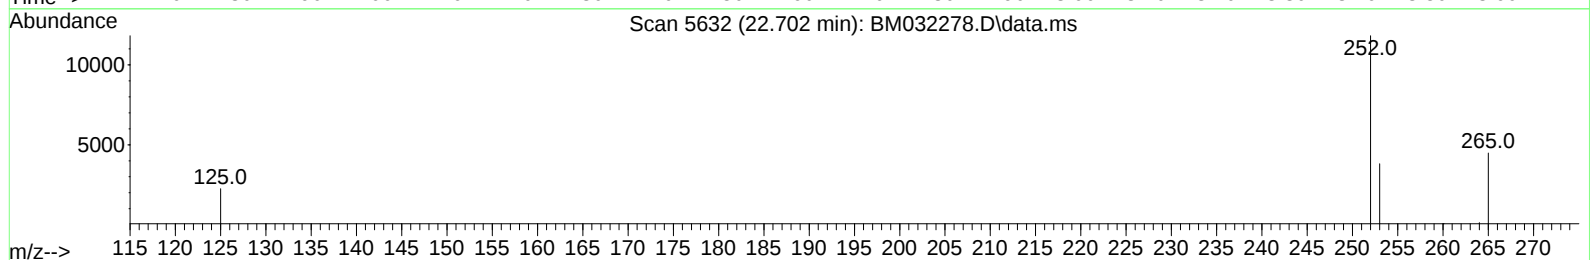


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032278.D
Acq On : 29 Sep 2021 18:49
Operator : CG/JU
Sample : PB139218BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Sep 30 01:04:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

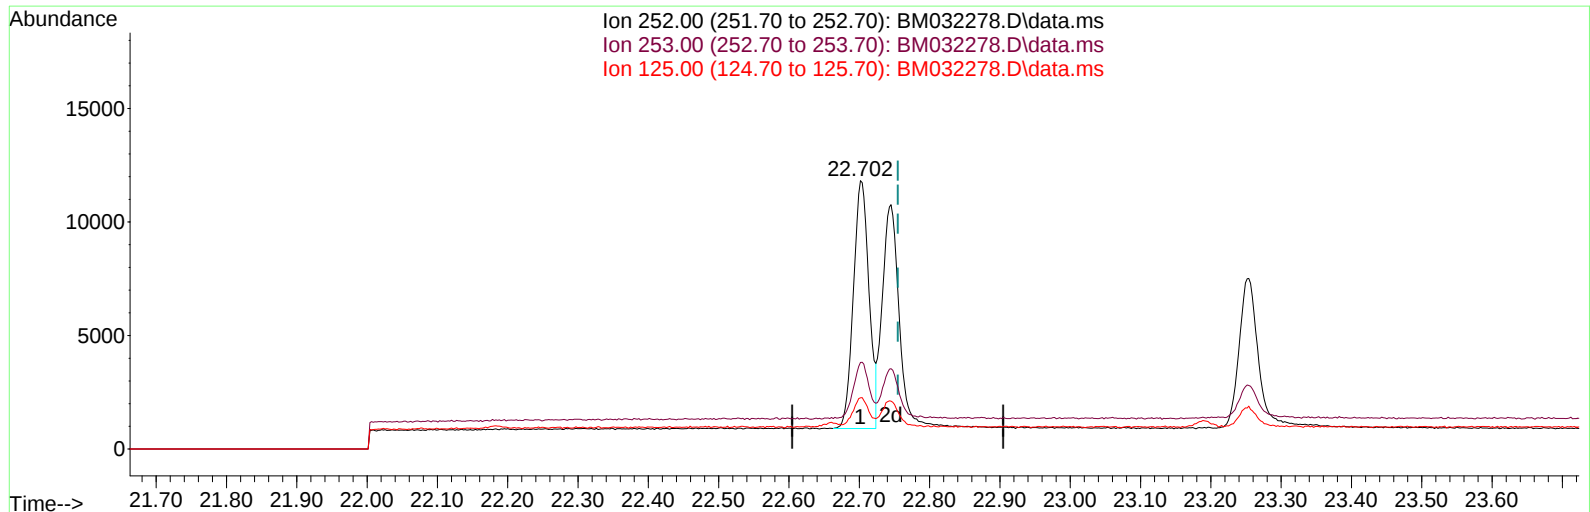

TIC: BM032278.D\data.ms

(25) Benzo(k)fluoranthene

22.702min (-0.053) 0.38 ng/u1

response 16865

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	32.29
125.00	16.10	19.07
0.00	0.00	0.00