

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007236.D
 Acq On : 28 Sep 2021 18:11
 Operator : CG/JU
 Sample : M3927-23
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-06

Quant Time: Sep 29 04:18:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	208525	20.000	ng	-0.01
21) Naphthalene-d8	10.681	136	812931	20.000	ng	#-0.01
39) Acenaphthene-d10	14.516	164	516742	20.000	ng	-0.01
64) Phenanthrene-d10	17.263	188	1089119	20.000	ng	#-0.01
76) Chrysene-d12	21.351	240	1050659	20.000	ng	0.00
86) Perylene-d12	23.763	264	1134466	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.452	112	1066780	85.636	ng	-0.01
7) Phenol-d6	7.052	99	1369074	80.412	ng	-0.01
23) Nitrobenzene-d5	9.040	82	824191	59.043	ng	-0.02
42) 2,4,6-Tribromophenol	16.004	330	684398	102.160	ng	-0.01
45) 2-Fluorobiphenyl	13.140	172	2159424	59.868	ng	-0.01
79) Terphenyl-d14	19.822	244	3412213	62.234	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007236.D
Acq On : 28 Sep 2021 18:11
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Time: Sep 29 04:18:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 23 11:17:25 2021
Response via : Initial Calibration




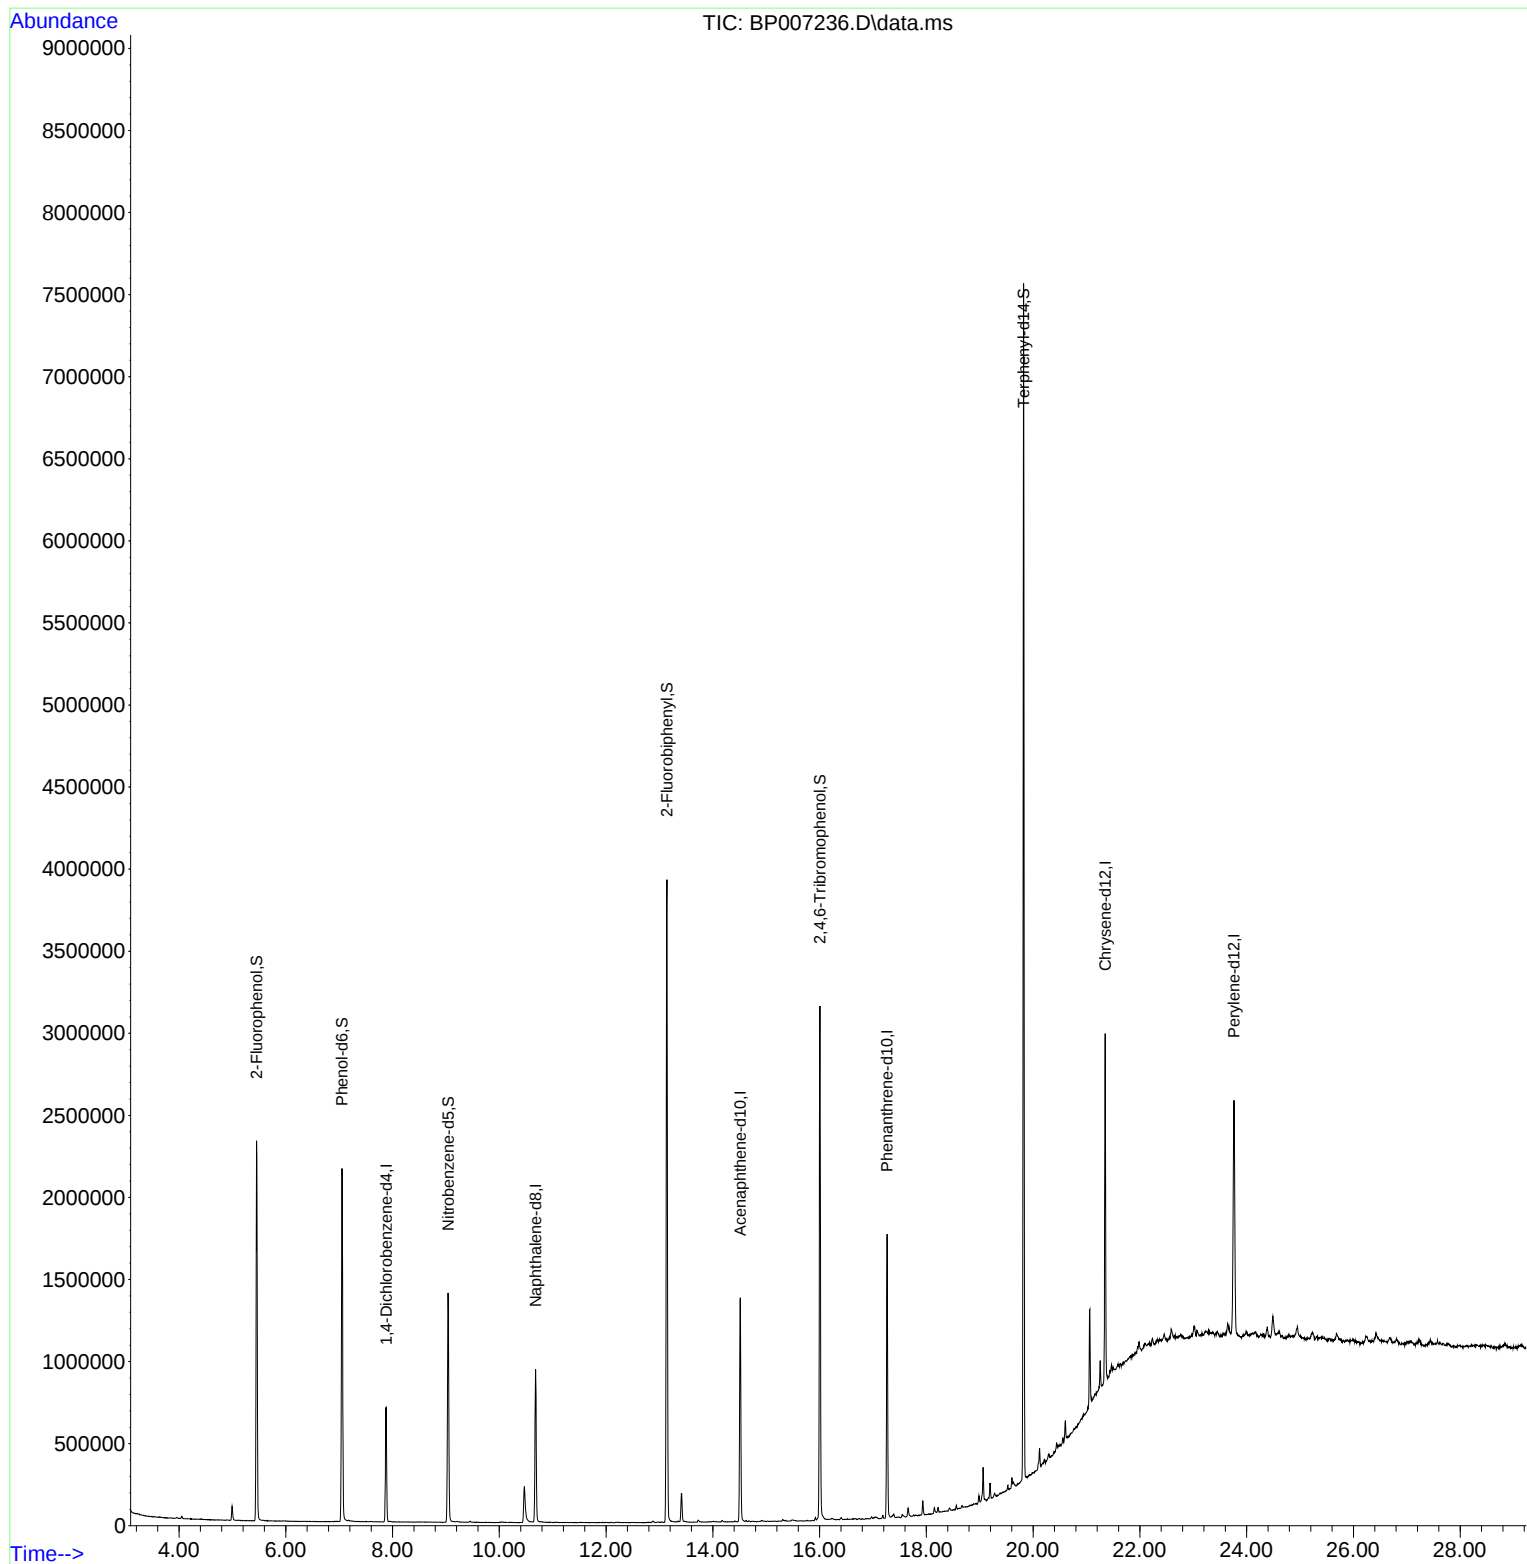




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.881 min Scan# 815
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11




Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06


Tgt Ion:152 Resp: 208525
Ion Ratio Lower Upper
152 100
150 150.7 125.6 188.4
115 54.9 48.5 72.7

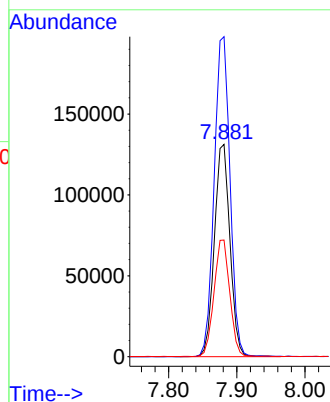

#5
2-Fluorophenol
Concen: 85.636 ng
RT: 5.452 min Scan# 402
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Tgt Ion:112 Resp: 1066780
Ion Ratio Lower Upper
112 100
64 52.9 41.4 62.2
63 27.4 23.8 35.8


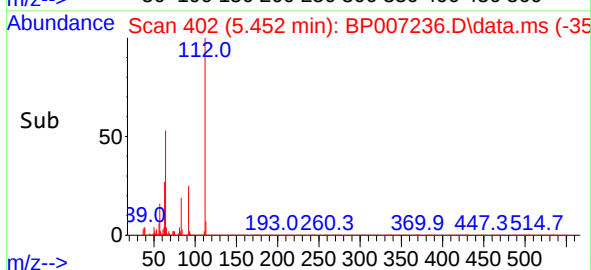
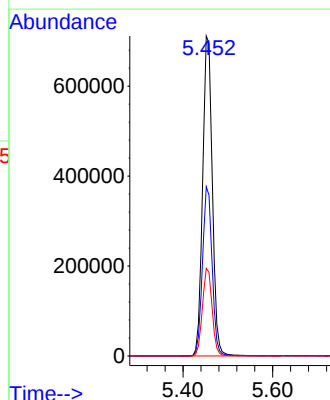





#7
Phenol-d6
Concen: 80.412 ng
RT: 7.052 min Scan# 674
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11




Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06


Tgt Ion: 99 Resp: 1369074
Ion Ratio Lower Upper
99 100
42 14.4 13.4 20.0
71 32.6 30.6 46.0

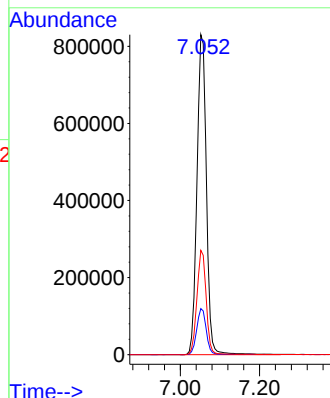

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.681 min Scan# 1291
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Tgt Ion: 136 Resp: 812931
Ion Ratio Lower Upper
136 100
137 10.6 8.6 12.8
54 6.9 4.6 6.8#
68 5.6 3.6 5.4#

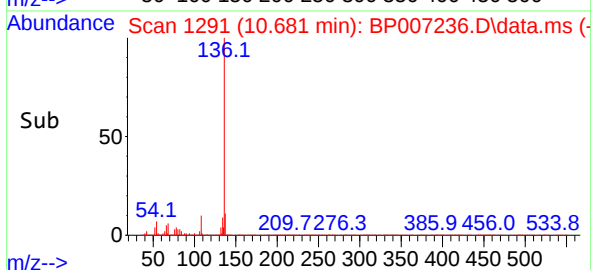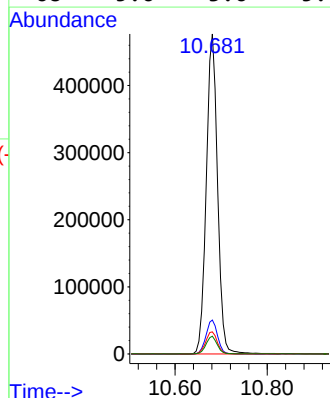



#23

Nitrobenzene-d5

Concen: 59.043 ng

RT: 9.040 min Scan# 1012

Delta R.T. -0.018 min

Lab File: BP007236.D

Acq: 28 Sep 2021 18:11

Tgt Ion: 82 Resp: 824191





Ion	Ratio	Lower	Upper
82	100		
128	47.5	35.7	53.5
54	45.4	35.0	52.4

Instrument :

BNA_P

ClientSampleId :

WOOSPK-BACKFILL-06

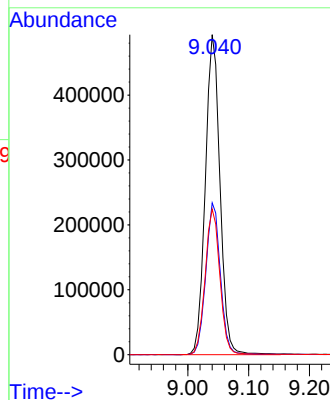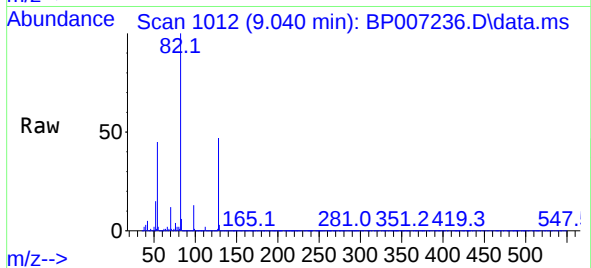

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.516 min Scan# 1943




Delta R.T. -0.012 min


Lab File: BP007236.D

Acq: 28 Sep 2021 18:11

Tgt Ion: 164 Resp: 516742

Ion	Ratio	Lower	Upper
164	100		
162	99.0	80.2	120.2
160	43.9	34.5	51.7


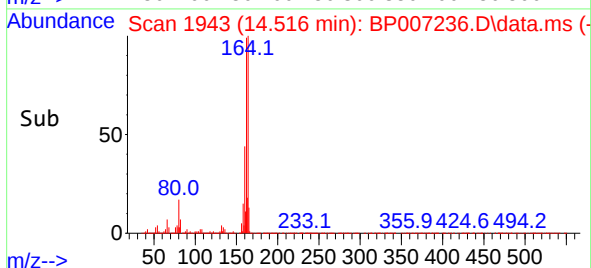
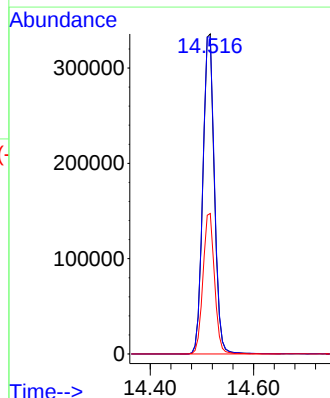





#42
2,4,6-Tribromophenol
Concen: 102.160 ng
RT: 16.004 min Scan# 2196
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11




Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06


Tgt Ion:330 Resp: 684398
Ion Ratio Lower Upper
330 100
332 96.3 77.8 116.8
141 27.5 25.4 38.2

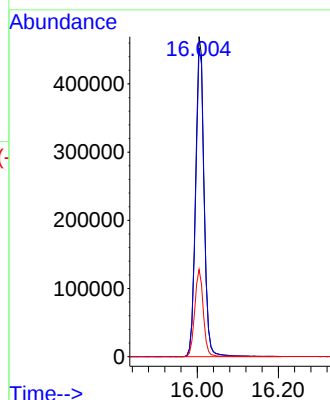

#45
2-Fluorobiphenyl
Concen: 59.868 ng
RT: 13.140 min Scan# 1709
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Tgt Ion:172 Resp: 2159424
Ion Ratio Lower Upper
172 100
171 35.5 27.9 41.9
170 23.4 18.6 27.8


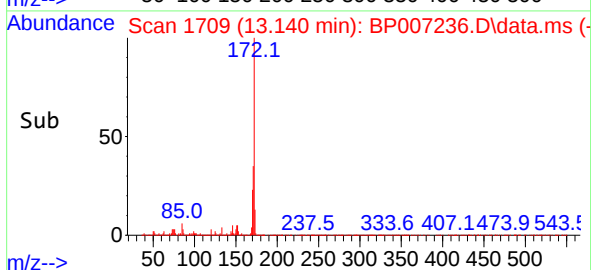
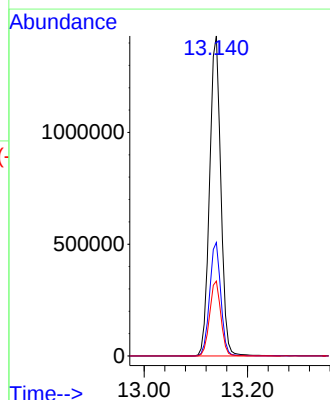





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.263 min Scan# 2410
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11




Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06


Tgt Ion:188 Resp: 1089119
Ion Ratio Lower Upper
188 100
94 8.4 5.6 8.4#
80 9.2 6.3 9.5

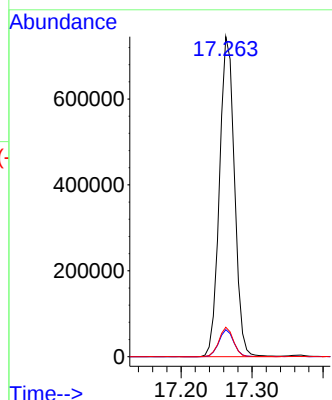

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.351 min Scan# 3105
Delta R.T. -0.006 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Tgt Ion:240 Resp: 1050659
Ion Ratio Lower Upper
240 100
120 9.0 6.5 9.7
236 25.6 20.6 31.0


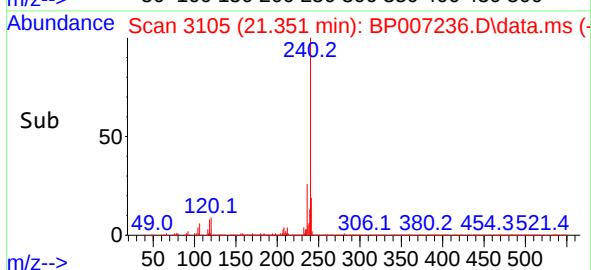
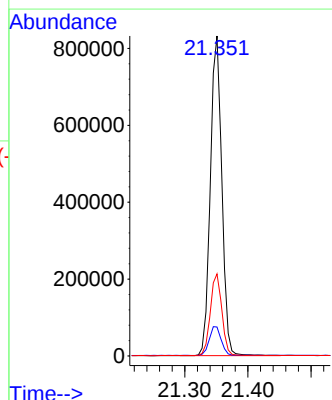





#79
Terphenyl-d14
Concen: 62.234 ng
RT: 19.822 min Scan# 2845
Delta R.T. -0.012 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Tgt Ion:244 Resp: 3412213
Ion Ratio Lower Upper
244 100
212 6.9 6.0 9.0
122 8.8 7.1 10.7

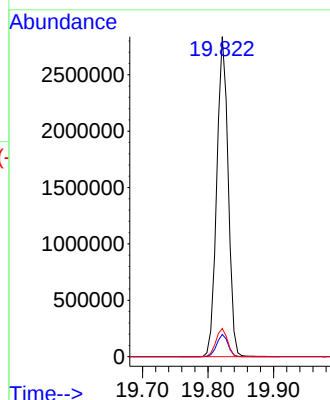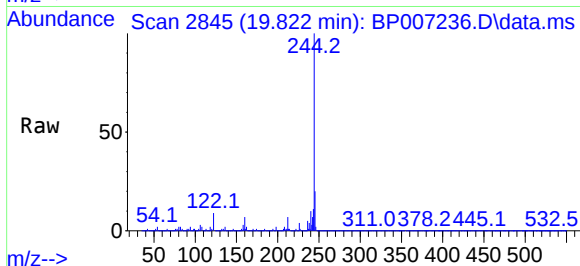

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.763 min Scan# 3515
Delta R.T. -0.006 min
Lab File: BP007236.D
Acq: 28 Sep 2021 18:11

Tgt Ion:264 Resp: 1134466
Ion Ratio Lower Upper
264 100
260 23.9 18.6 28.0
265 21.8 17.6 26.4

