

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007224.D
 Acq On : 28 Sep 2021 10:57
 Operator : CG/JU
 Sample : PB139369BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139369BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	419	rBV	2756673	4084340	41.58%	9.697%
2	7.064	668	676	692	rBV	2405960	3969775	40.41%	9.425%
3	7.881	808	815	825	rBV	557226	864088	8.80%	2.051%
4	9.046	1004	1013	1029	rBV	1566852	2608471	26.55%	6.193%
5	10.687	1284	1292	1303	rBV	678727	1174737	11.96%	2.789%
6	13.146	1702	1710	1727	rBV	4212350	6519824	66.37%	15.479%
7	14.522	1934	1944	1959	rBV	1081029	1630347	16.60%	3.871%
8	16.010	2190	2197	2219	rBV	3432983	5303014	53.98%	12.590%
9	17.269	2405	2411	2425	rBV	1311418	1971883	20.07%	4.682%
10	19.828	2841	2846	2852	rBV	8169069	9823463	100.00%	23.323%
11	21.357	3102	3106	3113	rBV	1553944	1962471	19.98%	4.659%
12	23.774	3512	3517	3528	rVB2	1066634	2207538	22.47%	5.241%




Sum of corrected areas: 42119951

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007224.D
Acq On : 28 Sep 2021 10:57
Operator : CG/JU
Sample : PB139369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

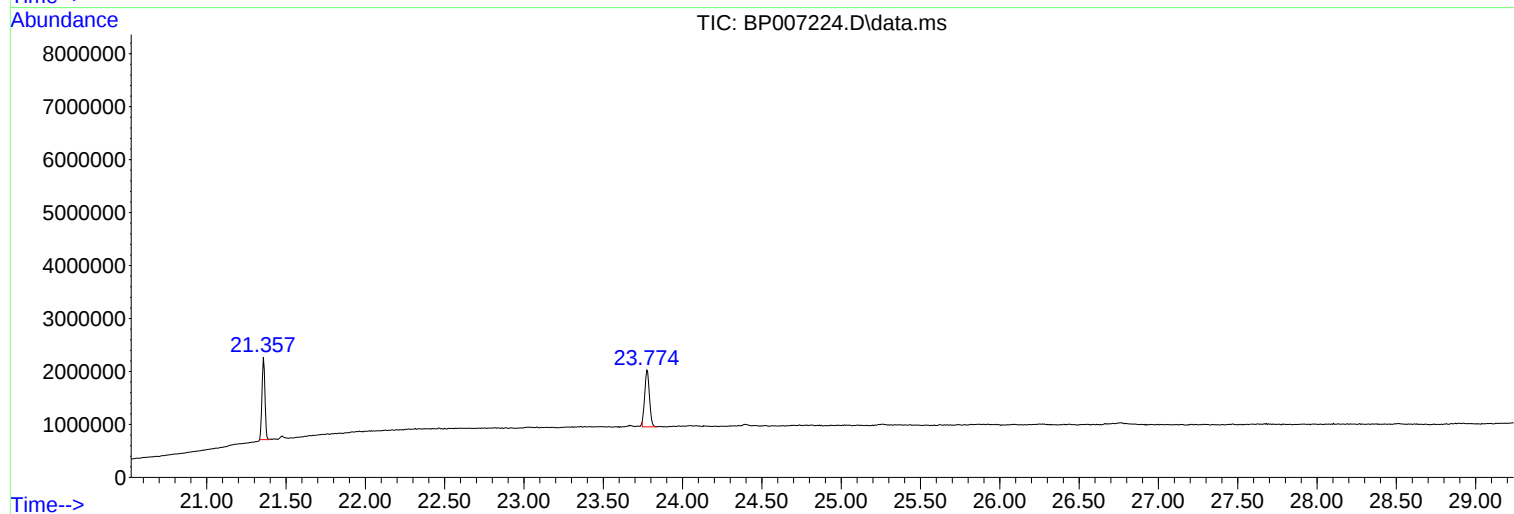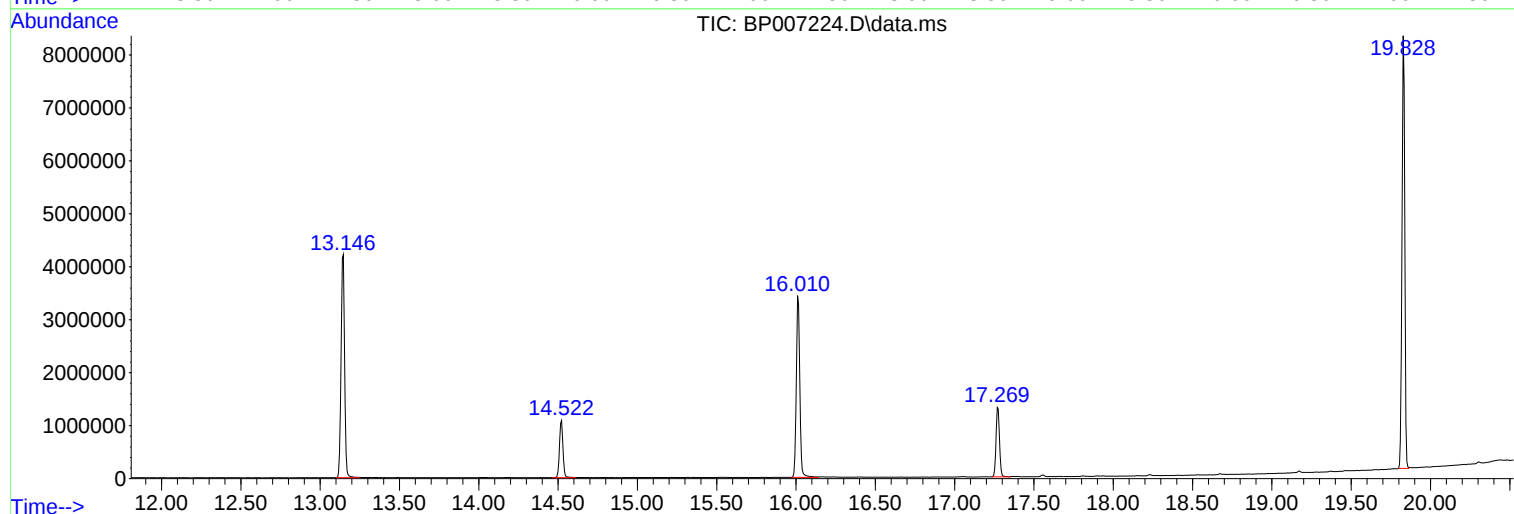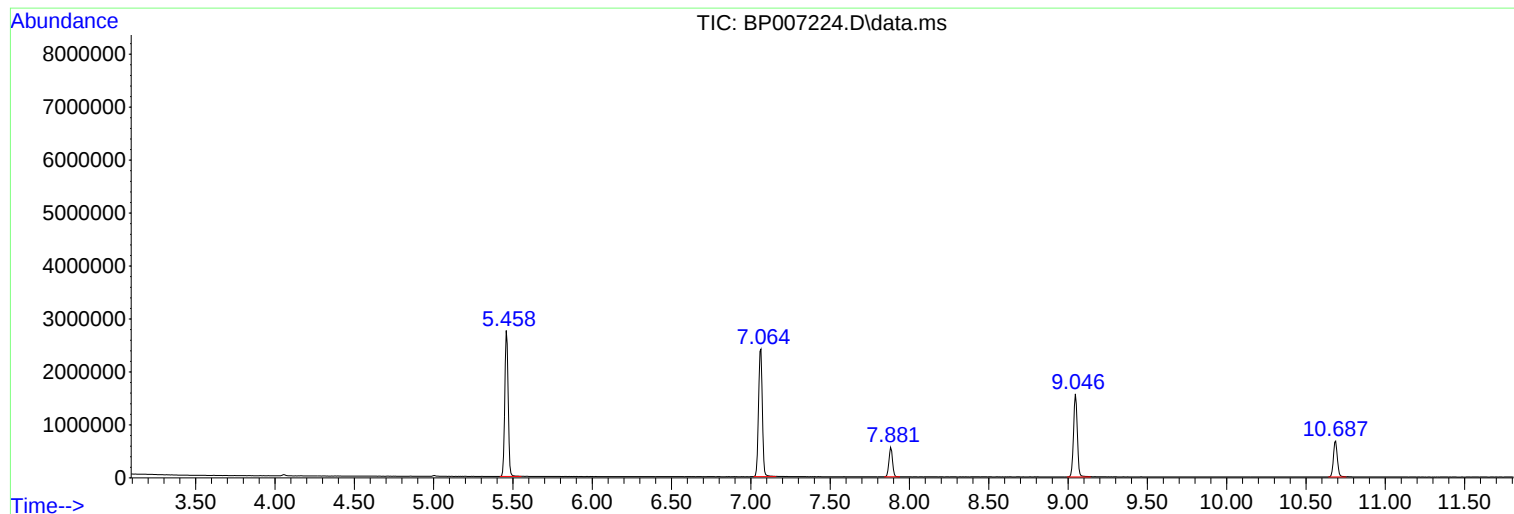

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007224.D
Acq On : 28 Sep 2021 10:57
Operator : CG/JU
Sample : PB139369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007224.D
Acq On : 28 Sep 2021 10:57
Operator : CG/JU
Sample : PB139369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139369BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------