

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007225.D
 Acq On : 28 Sep 2021 11:31
 Operator : CG/JU
 Sample : PB139420BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139420BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	397	403	423	rVB	2710398	4072424	41.22%	9.614%
2	7.063	668	676	696	rBV	2434095	3996396	40.45%	9.434%
3	7.881	808	815	824	rBV	557634	865620	8.76%	2.043%
4	9.045	1005	1013	1025	rBV	1543571	2604177	26.36%	6.148%
5	10.686	1282	1292	1304	rBV	680659	1182755	11.97%	2.792%
6	13.145	1702	1710	1732	rBV	4246370	6564531	66.44%	15.497%
7	14.522	1936	1944	1963	rBV	1033470	1640407	16.60%	3.872%
8	16.010	2190	2197	2215	rBV	3492217	5296065	53.60%	12.502%
9	17.268	2404	2411	2424	rBV	1332779	1998797	20.23%	4.719%
10	19.827	2841	2846	2852	rBV	8328271	9880446	100.00%	23.325%
11	21.356	3102	3106	3112	rBV	1630407	2006804	20.31%	4.737%
12	23.774	3511	3517	3527	rVB2	1089392	2252158	22.79%	5.317%




Sum of corrected areas: 42360580

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007225.D
Acq On : 28 Sep 2021 11:31
Operator : CG/JU
Sample : PB139420BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139420BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

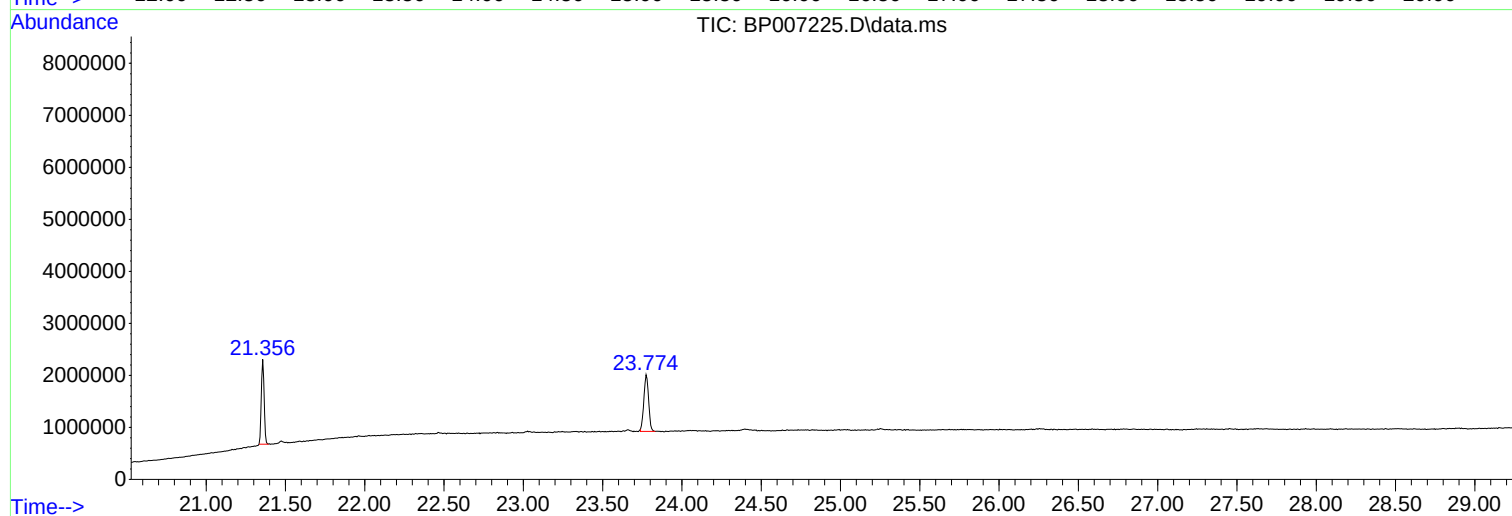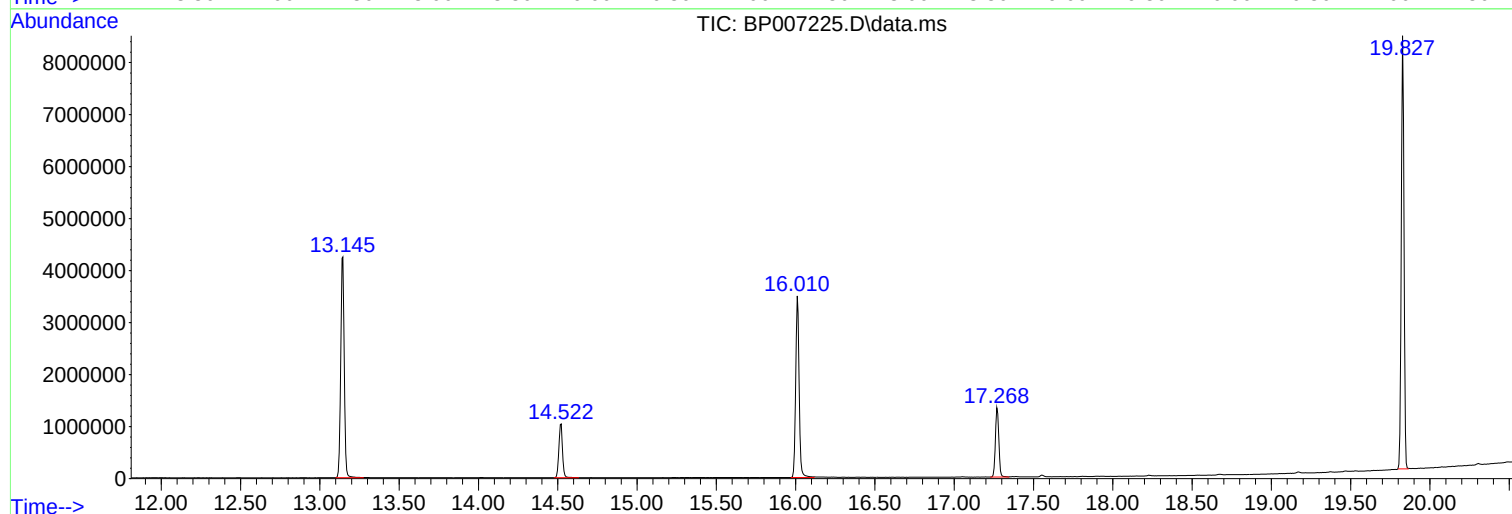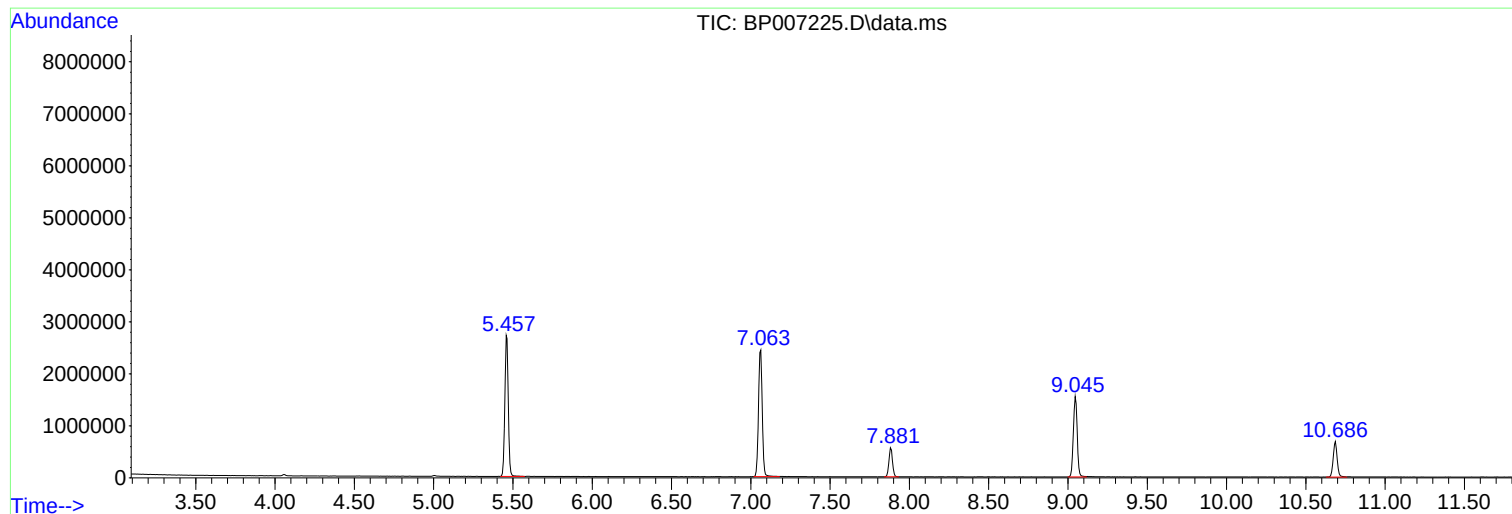

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007225.D
Acq On : 28 Sep 2021 11:31
Operator : CG/JU
Sample : PB139420BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139420BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007225.D
Acq On : 28 Sep 2021 11:31
Operator : CG/JU
Sample : PB139420BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139420BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------