

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007233.D
 Acq On : 28 Sep 2021 16:28
 Operator : CG/JU
 Sample : M3927-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	396	403	415	rBV	2346858	3460194	40.48%	8.404%
2	7.057	667	675	691	rBV	2170069	3514279	41.12%	8.536%
3	7.881	808	815	822	rBV	617593	968668	11.33%	2.353%
4	9.046	1005	1013	1031	rBV	1323764	2281055	26.69%	5.540%
5	10.463	1247	1254	1272	rBV	415760	898344	10.51%	2.182%
6	10.681	1284	1291	1303	rBV	813633	1373004	16.06%	3.335%
7	13.139	1701	1709	1723	rBV	3864384	5801652	67.88%	14.092%
8	14.516	1936	1943	1959	rBV	1225959	1882627	22.03%	4.573%
9	16.004	2190	2196	2219	rVB	3054445	4474646	52.35%	10.868%
10	17.263	2404	2410	2422	rBV	1501490	2240455	26.21%	5.442%
11	17.933	2520	2524	2530	rVB	76476	93507	1.09%	0.227%
12	19.821	2840	2845	2850	rBV	6868257	8547127	100.00%	20.760%
13	21.063	3053	3056	3060	rVB	353650	389786	4.56%	0.947%
14	21.351	3100	3105	3116	rBV	1918672	2543713	29.76%	6.178%
15	23.762	3509	3515	3523	rVB2	1319862	2702035	31.61%	6.563%




Sum of corrected areas: 41171092

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007233.D
Acq On : 28 Sep 2021 16:28
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

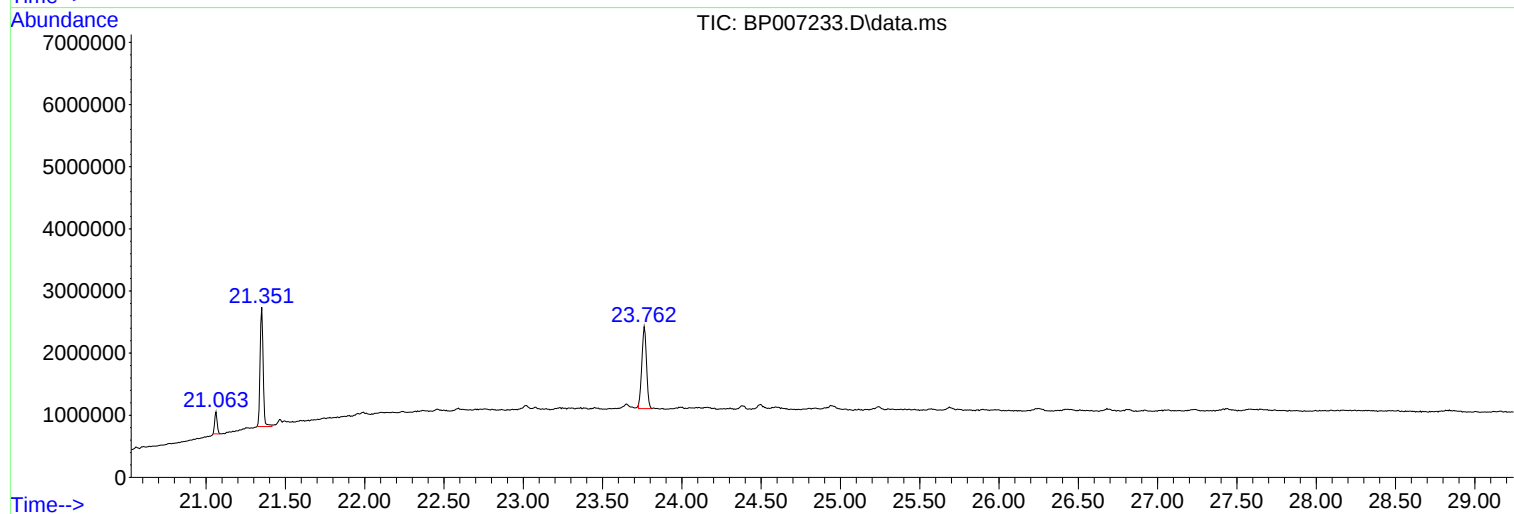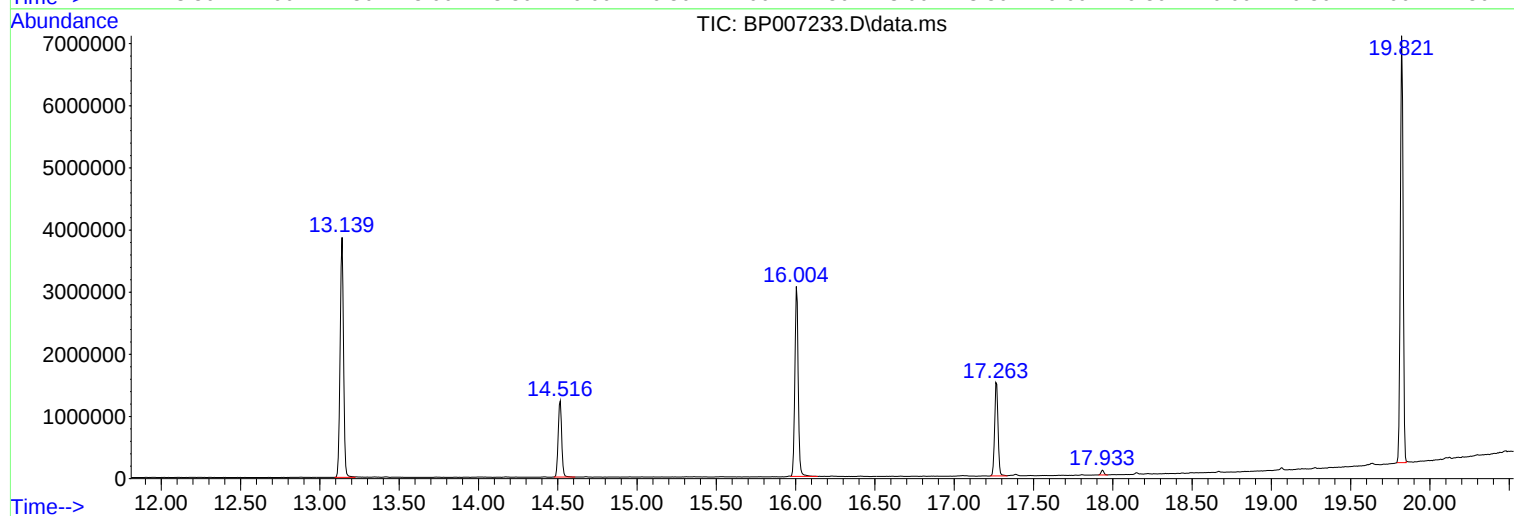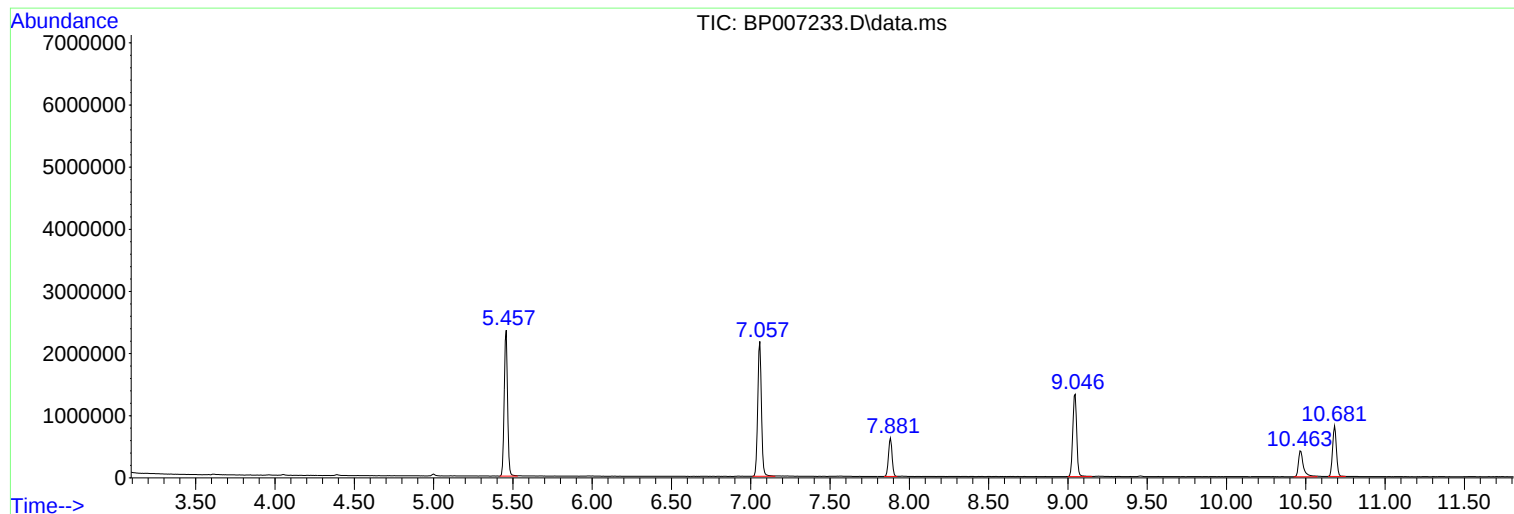

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007233.D
Acq On : 28 Sep 2021 16:28
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007233.D
Acq On : 28 Sep 2021 16:28
Operator : CG/JU
Sample : M3927-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------