

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007234.D
 Acq On : 28 Sep 2021 17:03
 Operator : CG/JU
 Sample : M3927-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	396	402	417	rBV	2348481	3525681	40.36%	8.342%
2	7.052	667	674	690	rBV	2146093	3564777	40.81%	8.434%
3	7.881	807	815	822	rBV	643809	1025086	11.74%	2.425%
4	9.040	1004	1012	1029	rBV	1362548	2323230	26.60%	5.497%
5	10.463	1246	1254	1275	rBV	422291	910877	10.43%	2.155%
6	10.681	1283	1291	1300	rBV	853963	1446051	16.56%	3.421%
7	13.140	1701	1709	1724	rBV	3873667	5902573	67.58%	13.966%
8	14.516	1935	1943	1957	rBV	1251054	1979935	22.67%	4.685%
9	16.004	2190	2196	2214	rBV	3093666	4542704	52.01%	10.748%
10	17.263	2404	2410	2423	rBV	1585759	2370035	27.13%	5.608%
11	17.934	2520	2524	2529	rBV	86910	105376	1.21%	0.249%
12	19.822	2840	2845	2850	rBV	7431992	8734631	100.00%	20.666%
13	21.057	3052	3055	3062	rBV	374928	487711	5.58%	1.154%
14	21.351	3100	3105	3110	rBV	1973495	2563782	29.35%	6.066%
15	23.763	3509	3515	3523	rVB2	1382005	2782263	31.85%	6.583%




Sum of corrected areas: 42264712

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007234.D
Acq On : 28 Sep 2021 17:03
Operator : CG/JU
Sample : M3927-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

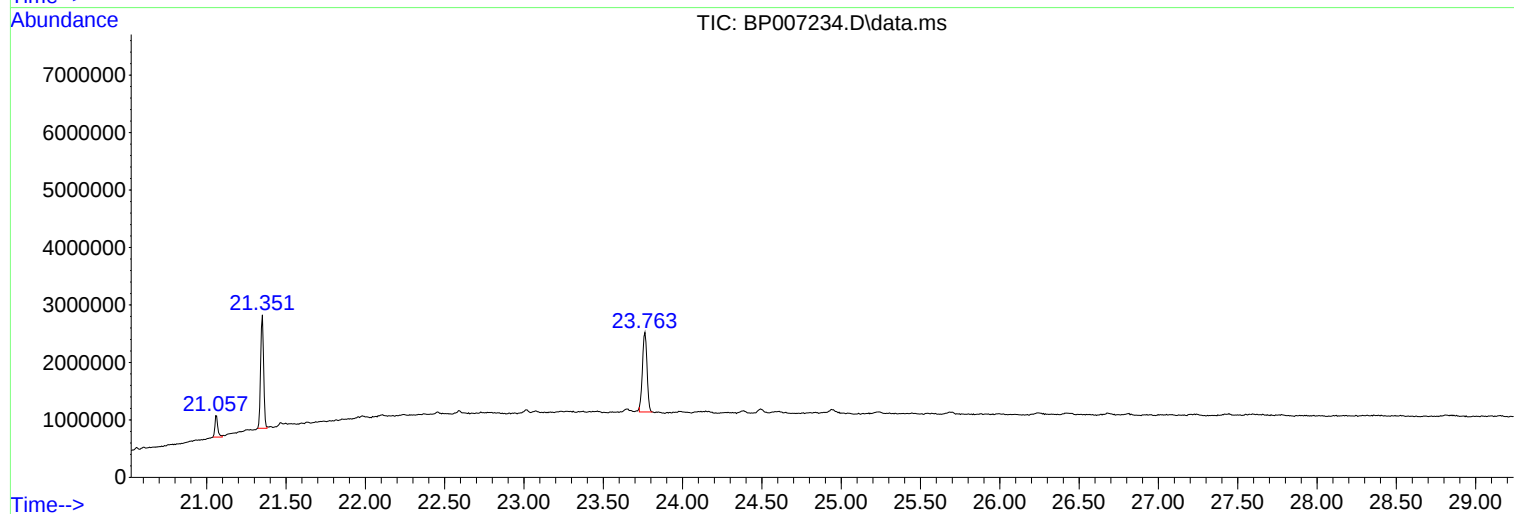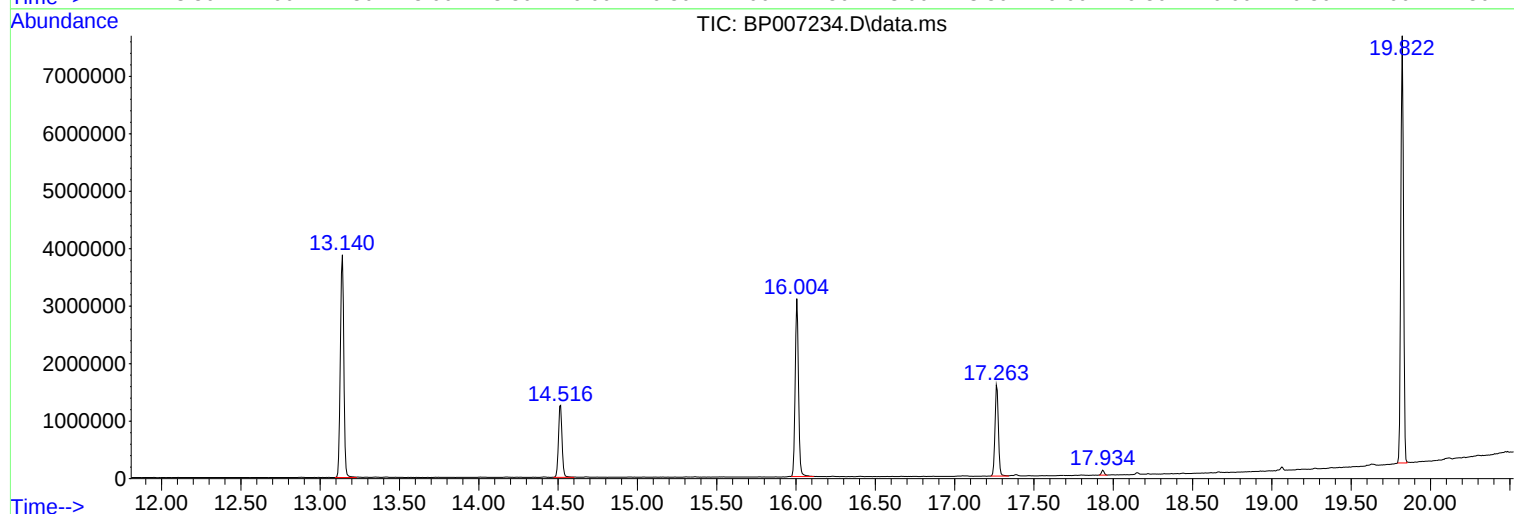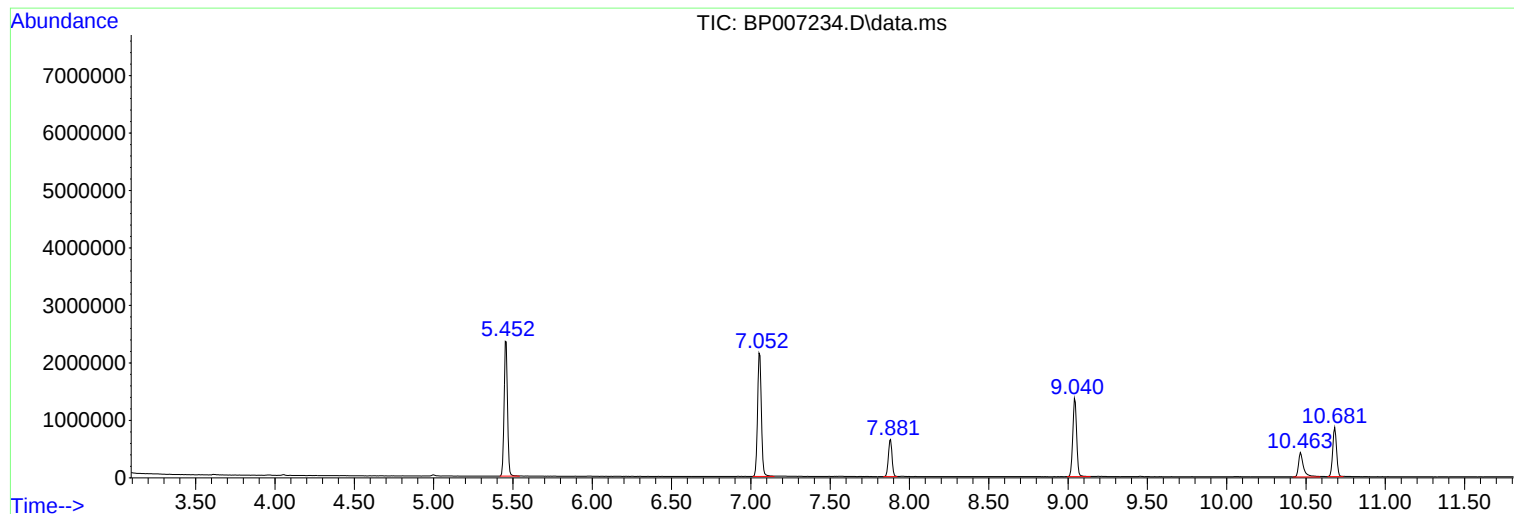

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007234.D
Acq On : 28 Sep 2021 17:03
Operator : CG/JU
Sample : M3927-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007234.D
Acq On : 28 Sep 2021 17:03
Operator : CG/JU
Sample : M3927-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
