

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007236.D
 Acq On : 28 Sep 2021 18:11
 Operator : CG/JU
 Sample : M3927-23
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WOOSPK-BACKFILL-06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	320	324	333	rVB	85121	119997	1.37%	0.273%
2	5.452	396	402	418	rBV	2313946	3441773	39.42%	7.827%
3	7.052	667	674	693	rBV	2150638	3593506	41.15%	8.172%
4	7.881	807	815	823	rBV	698011	1128908	12.93%	2.567%
5	9.040	1004	1012	1034	rBV	1396819	2353608	26.95%	5.353%
6	10.469	1247	1255	1274	rBV	219158	512895	5.87%	1.166%
7	10.681	1283	1291	1302	rBV	929555	1583703	18.14%	3.602%
8	13.140	1701	1709	1727	rBV	3914843	5964965	68.31%	13.566%
9	13.410	1749	1755	1763	rBV	171512	275920	3.16%	0.628%
10	14.516	1935	1943	1956	rBV	1362115	2151812	24.64%	4.894%
11	16.004	2185	2196	2215	rBV	3130985	4626744	52.99%	10.522%
12	17.263	2404	2410	2422	rBV	1729162	2555040	29.26%	5.811%
13	17.934	2520	2524	2530	rVB	86483	104327	1.19%	0.237%
14	19.063	2713	2716	2720	rVB	194519	205924	2.36%	0.468%
15	19.192	2735	2738	2742	rBV	91603	100529	1.15%	0.229%
16	19.822	2840	2845	2851	rBV	7277326	8731740	100.00%	19.858%
17	20.122	2893	2896	2900	rVB	111164	120703	1.38%	0.275%
18	21.063	3052	3056	3061	rBV	584863	753356	8.63%	1.713%
19	21.351	3100	3105	3112	rBV	2115392	2707166	31.00%	6.157%
20	23.763	3509	3515	3523	rVB2	1423390	2938262	33.65%	6.682%




Sum of corrected areas: 43970878

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007236.D
Acq On : 28 Sep 2021 18:11
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

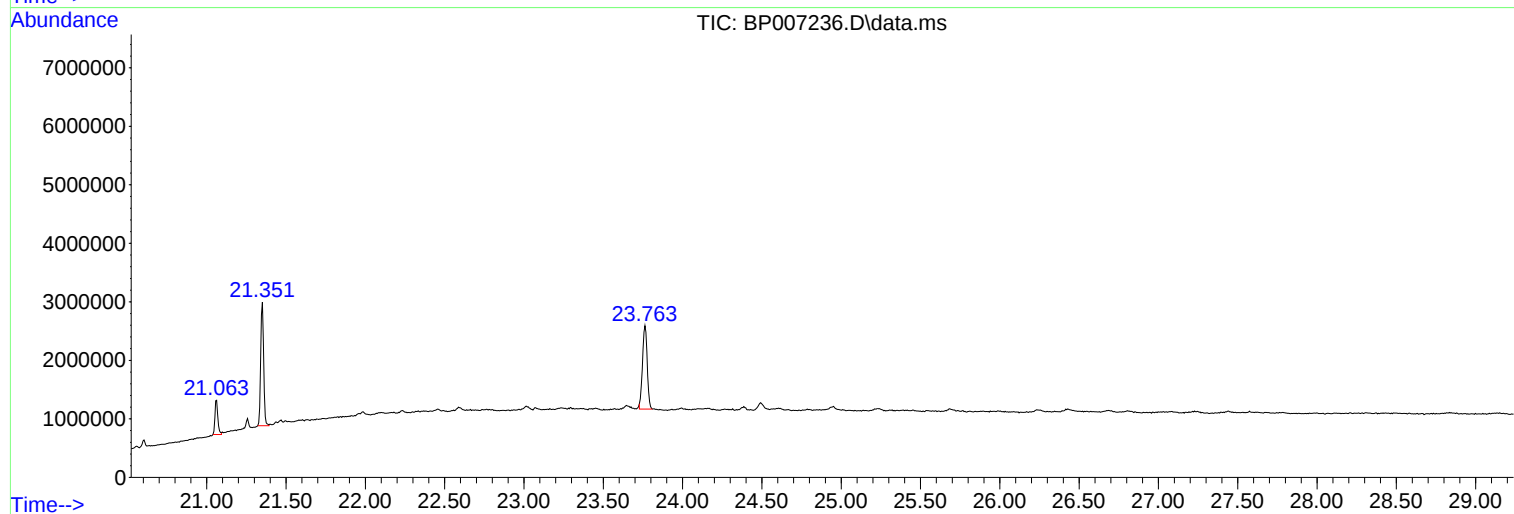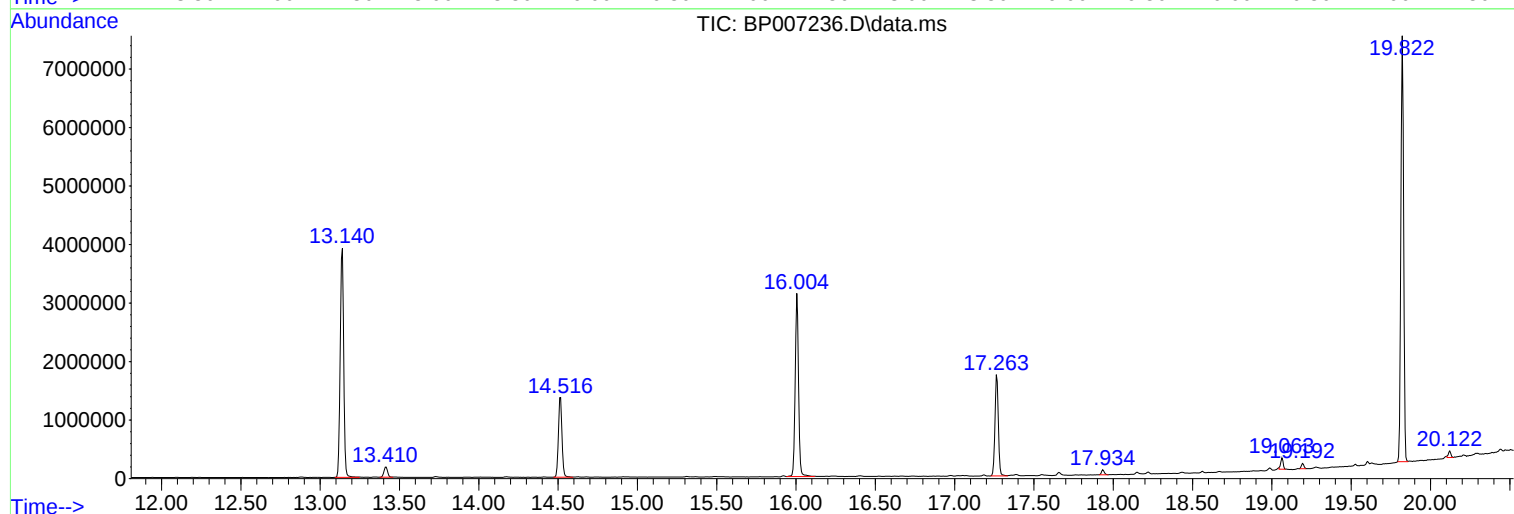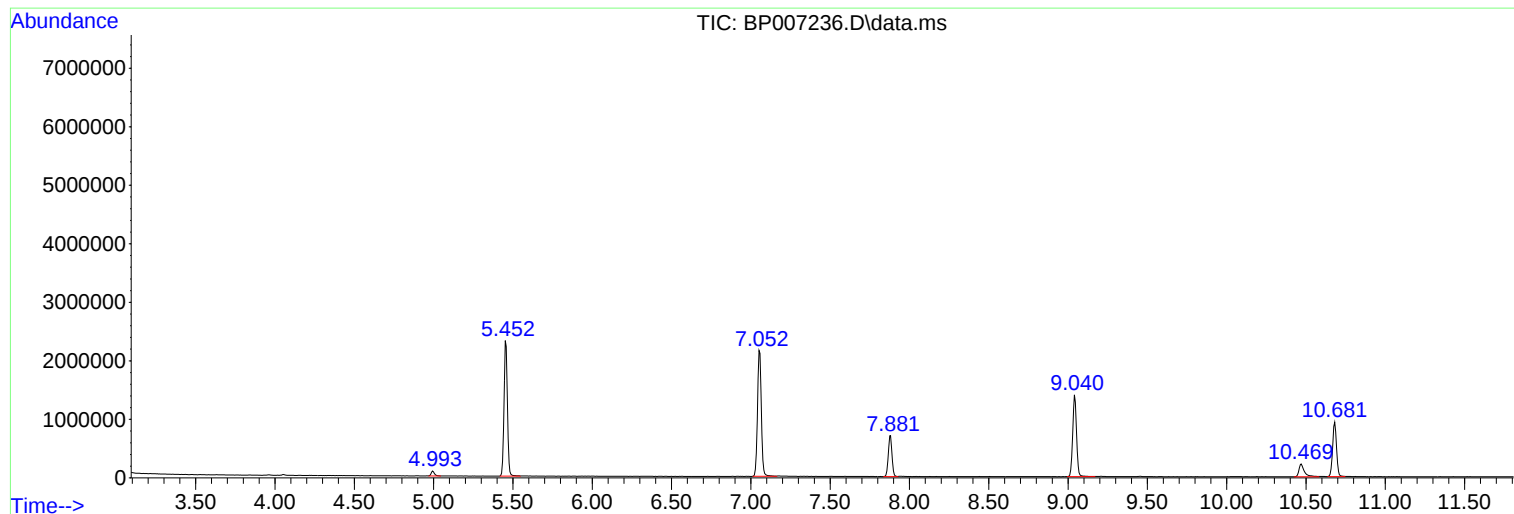

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007236.D
Acq On : 28 Sep 2021 18:11
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
Data File : BP007236.D
Acq On : 28 Sep 2021 18:11
Operator : CG/JU
Sample : M3927-23
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WOOSPK-BACKFILL-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------