


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007222.D
 Acq On : 28 Sep 2021 09:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 29 14:45:49 2021

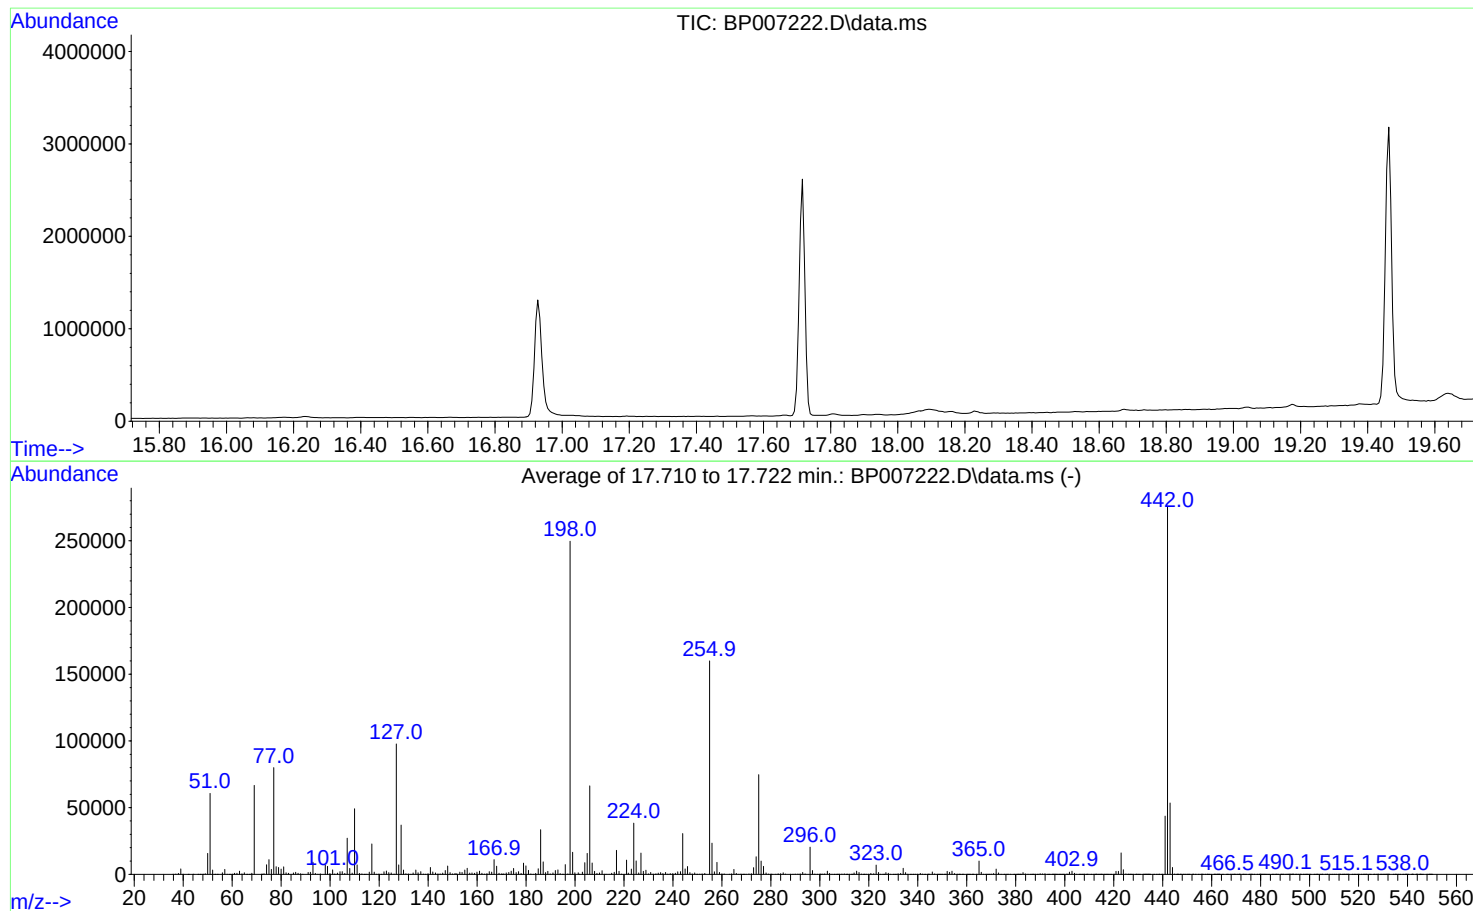




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	60727	PASS
68	69	0.00	2	1.3	889	PASS
69	198	0.00	100	26.7	66707	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.1	97723	PASS
197	198	0.00	2	0.1	371	PASS
198	198	100	100	100.0	249704	PASS
199	198	5	9	6.6	16585	PASS
275	198	10	60	29.9	74736	PASS
365	198	1	100	4.0	9912	PASS
441	198	0.01	100	17.5	43651	PASS
442	442	100	100	100.0	275722	PASS
443	442	15	24	19.4	53539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007222.D
 Acq On : 28 Sep 2021 09:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 10:39:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

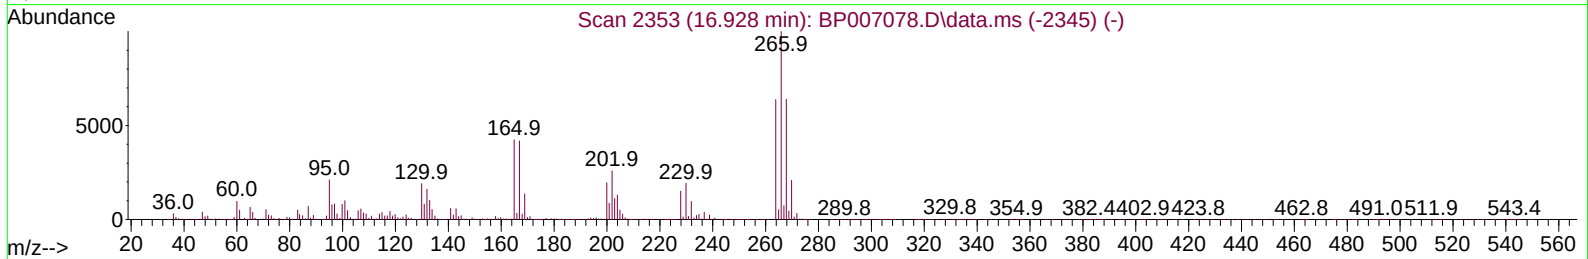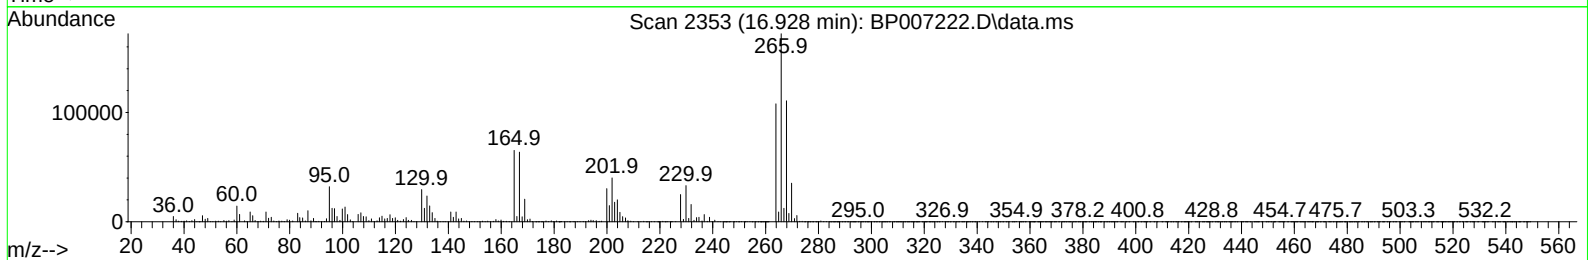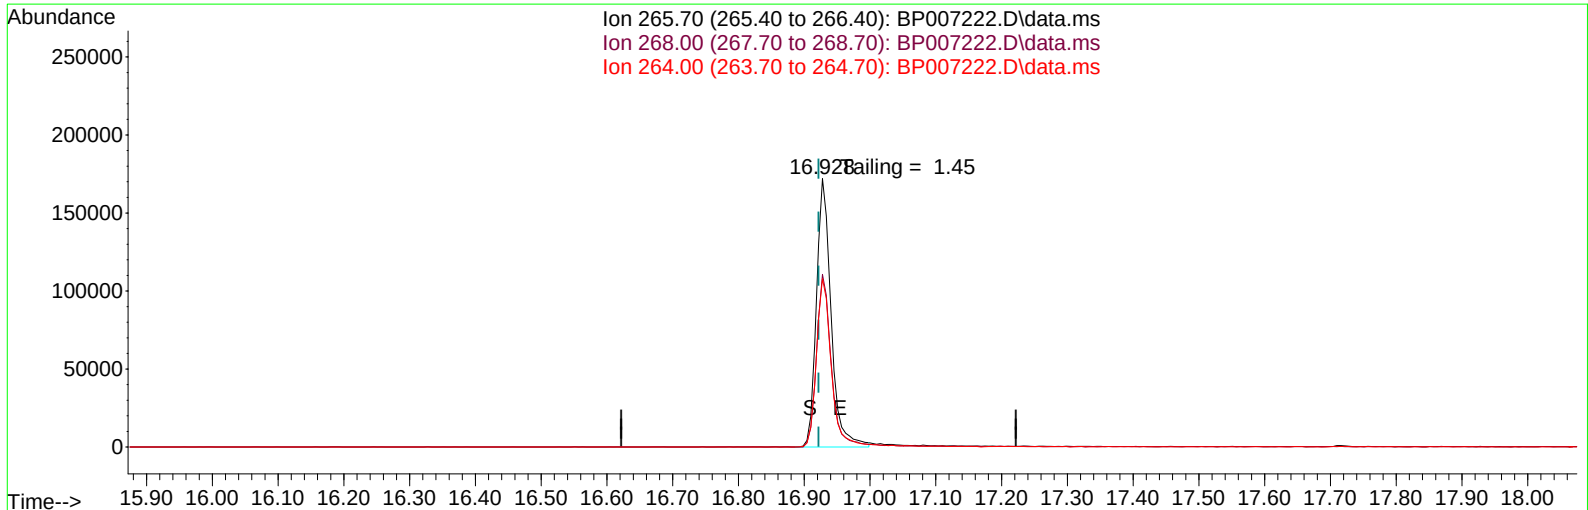

TIC: BP007222.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.006) 886527.43 ng




response 273419

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.36
264.00	62.90	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092821\
 Data File : BP007222.D
 Acq On : 28 Sep 2021 09:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 10:39:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 23 11:17:25 2021
 Response via : Initial Calibration

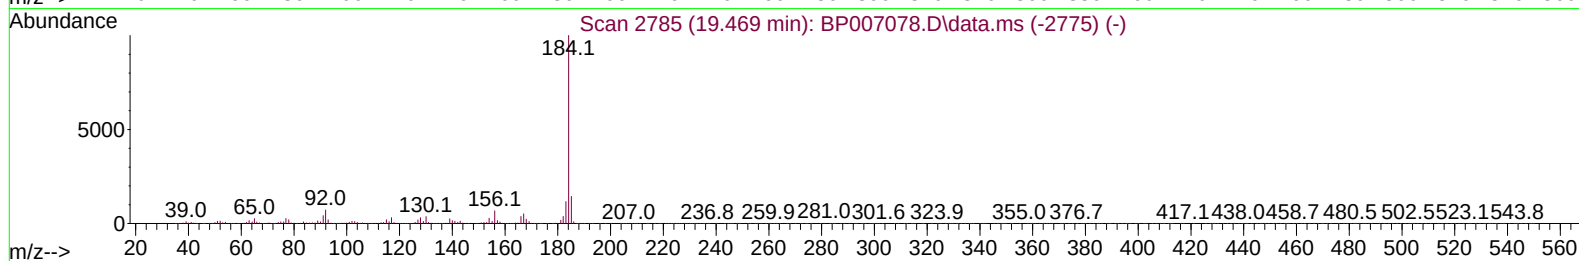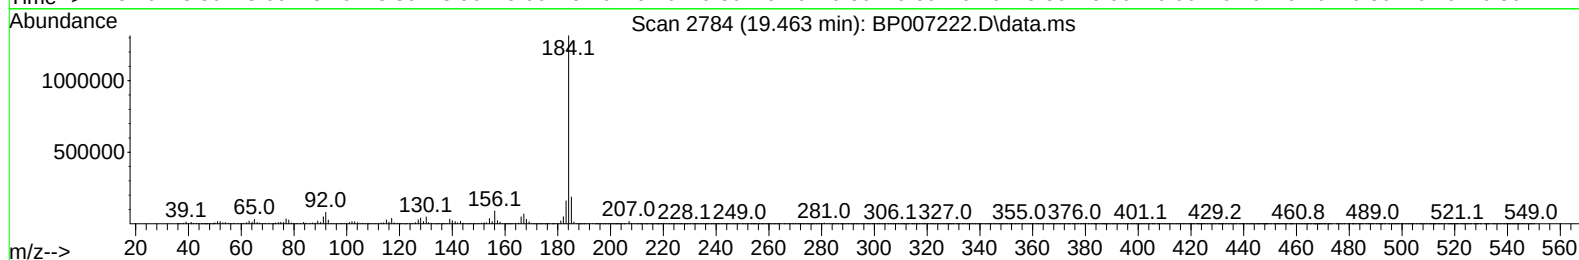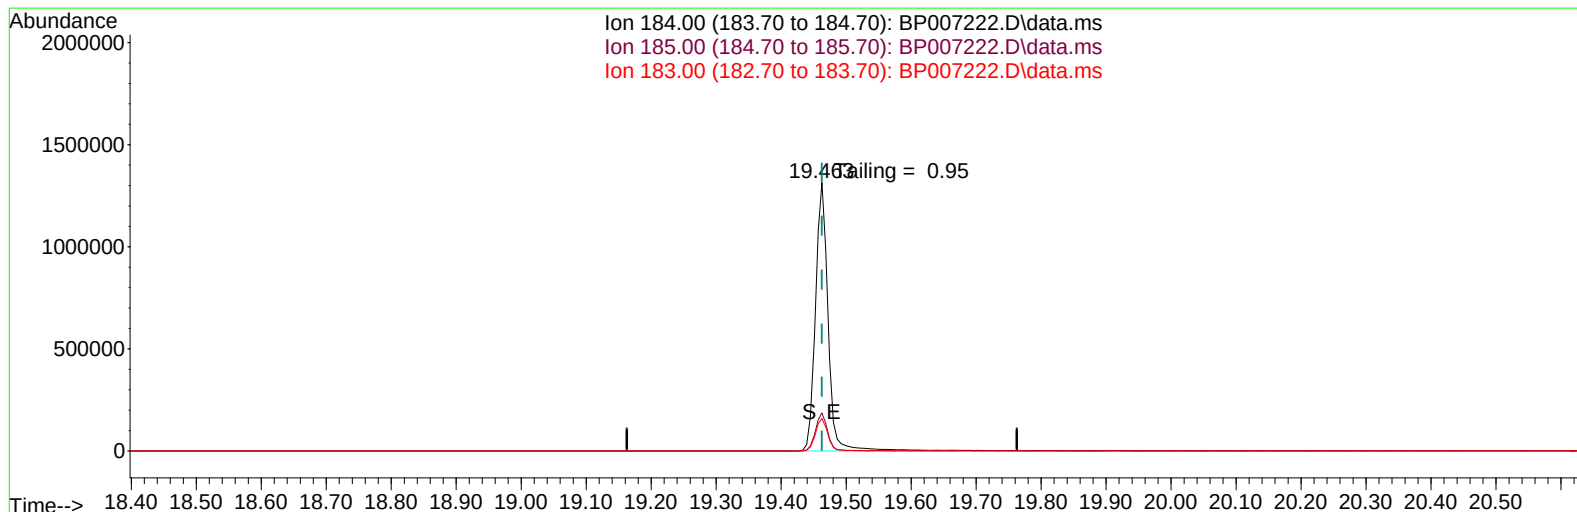

TIC: BP007222.D\data.ms

(77) Benzidine

19.463min (-0.000) 292217.74 ng

response 1778101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.19
183.00	11.90	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2021	BNA_P	<u>BP007222.D</u>
Compound Name	Response	Retention Time
DDT	895087	20.66
DDD	14069	20.23
DDE	1829	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15898	910985	1.75

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP