
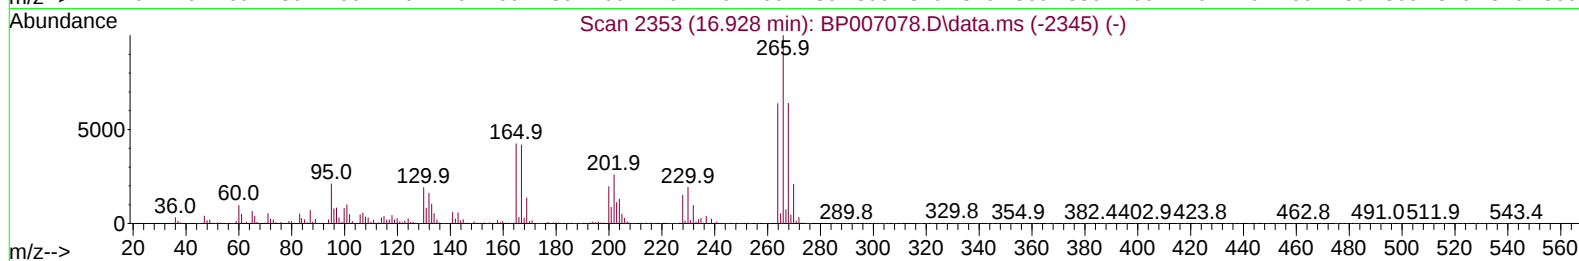
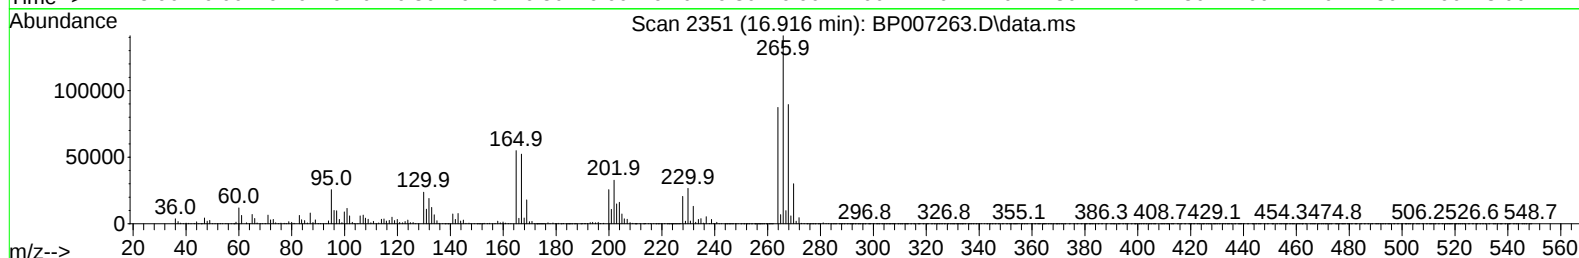


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
 Data File : BP007263.D
 Acq On : 30 Sep 2021 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 11:48:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration

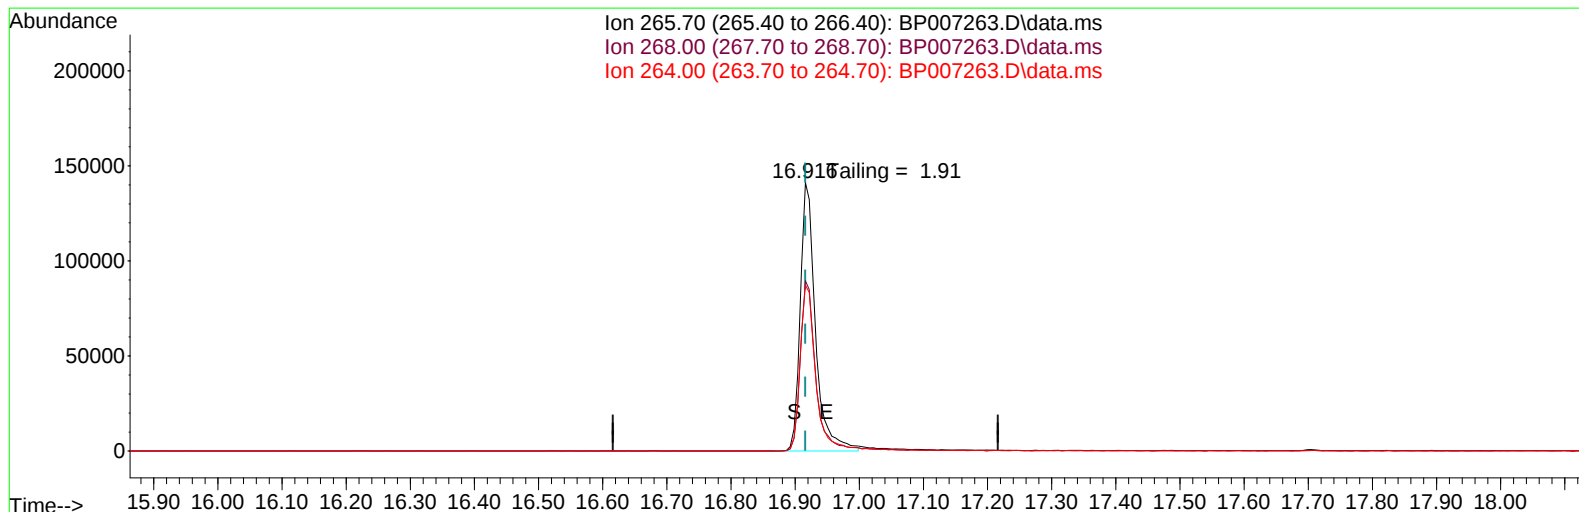

TIC: BP007263.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.000) 145339.91 ng

response 240525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.42
264.00	62.90	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
 Data File : BP007263.D
 Acq On : 30 Sep 2021 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 11:48:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration

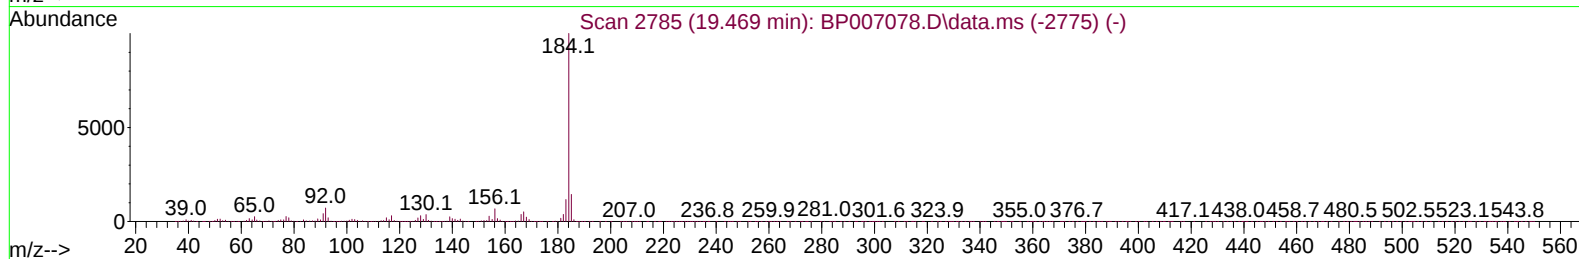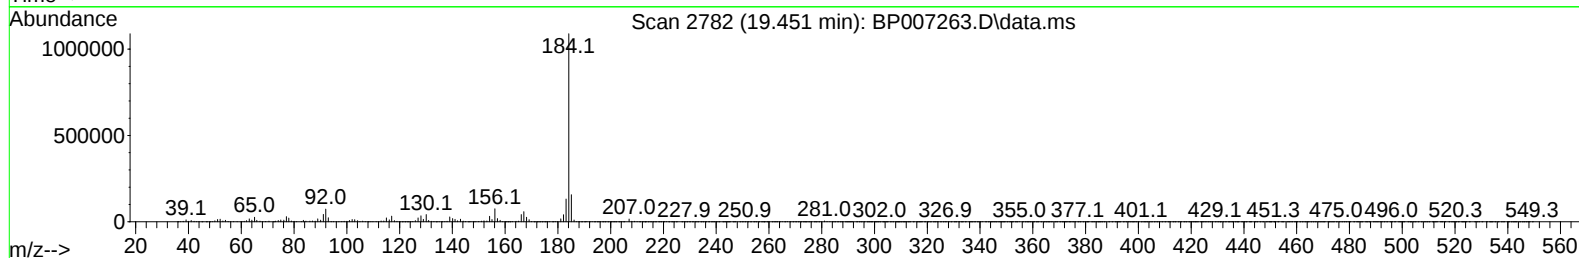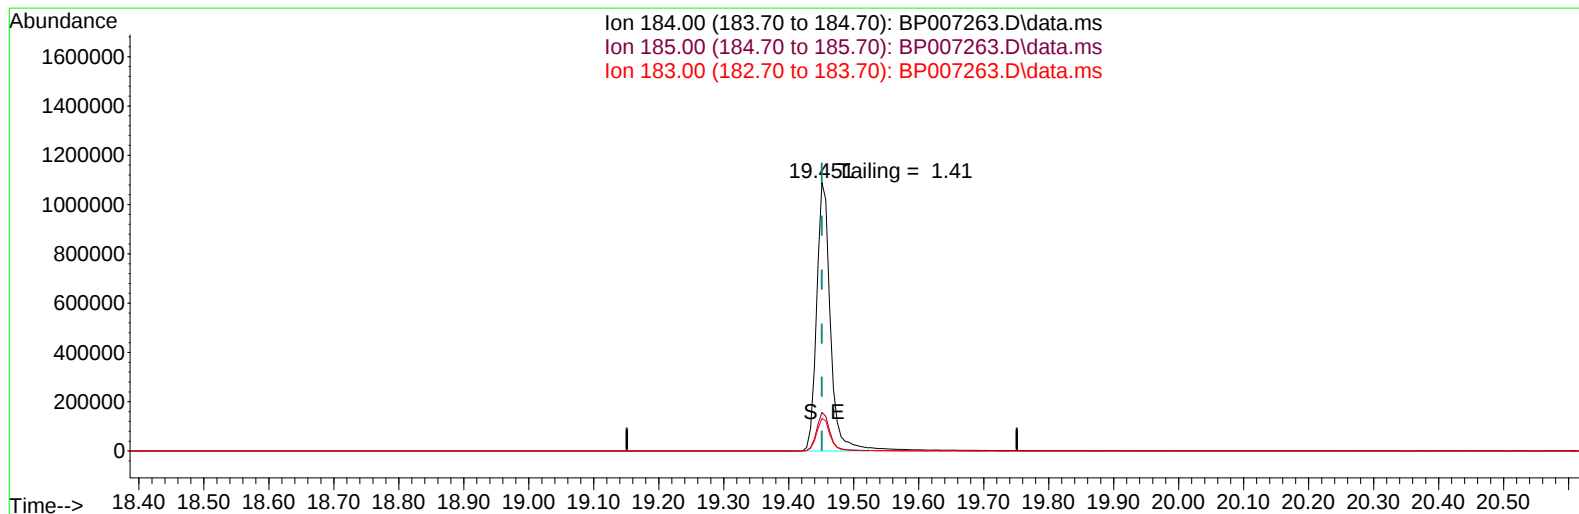

TIC: BP007263.D\data.ms

(77) Benzidine**19.451min (+ 0.000) 271427.21 ng****response 1634911**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.40
183.00	11.90	12.11
0.00	0.00	0.00