

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
 Data File : BP007265.D
 Acq On : 30 Sep 2021 11:41
 Operator : CG/JU
 Sample : PB139463BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139463BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	396	402	414	rBV	2285285	3457069	36.37%	8.584%
2	7.052	667	674	694	rBV	2383008	3934847	41.40%	9.770%
3	7.875	807	814	822	rBV	538078	870749	9.16%	2.162%
4	9.040	1003	1012	1028	rBV	1356812	2391630	25.16%	5.938%
5	10.675	1283	1290	1305	rBV	568139	1041855	10.96%	2.587%
6	13.134	1700	1708	1731	rBV	4453301	6880242	72.39%	17.084%
7	14.510	1932	1942	1961	rBV	887326	1433174	15.08%	3.559%
8	16.004	2187	2196	2226	rBV	2842791	4634432	48.76%	11.507%
9	17.263	2403	2410	2423	rBV	1174059	1787842	18.81%	4.439%
10	19.822	2839	2845	2856	rBV	7866592	9504845	100.00%	23.601%
11	21.351	3100	3105	3113	rBV	1576874	2119979	22.30%	5.264%
12	23.763	3509	3515	3527	rVB2	1058208	2216776	23.32%	5.504%




Sum of corrected areas: 40273440

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
Data File : BP007265.D
Acq On : 30 Sep 2021 11:41
Operator : CG/JU
Sample : PB139463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139463BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

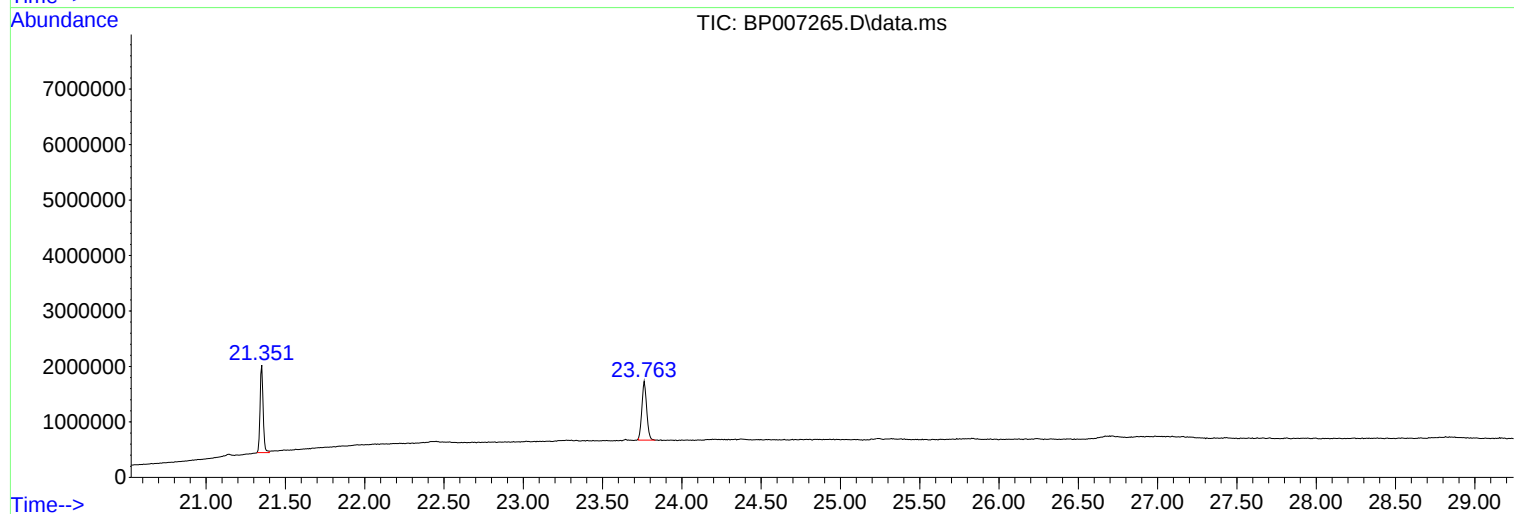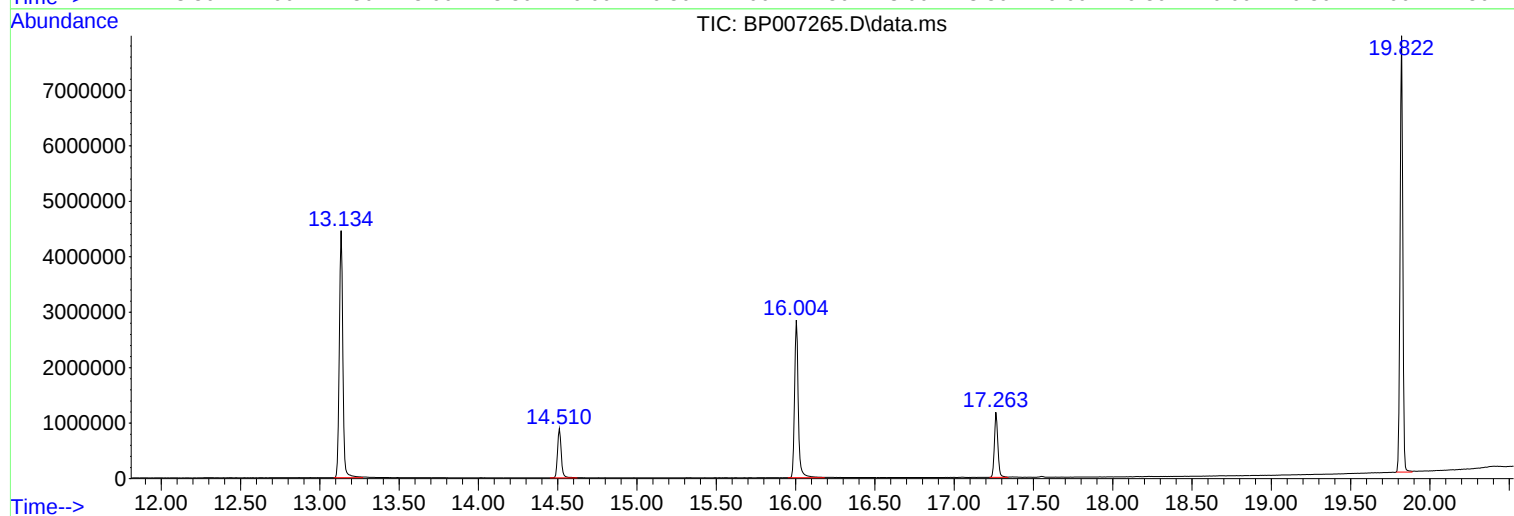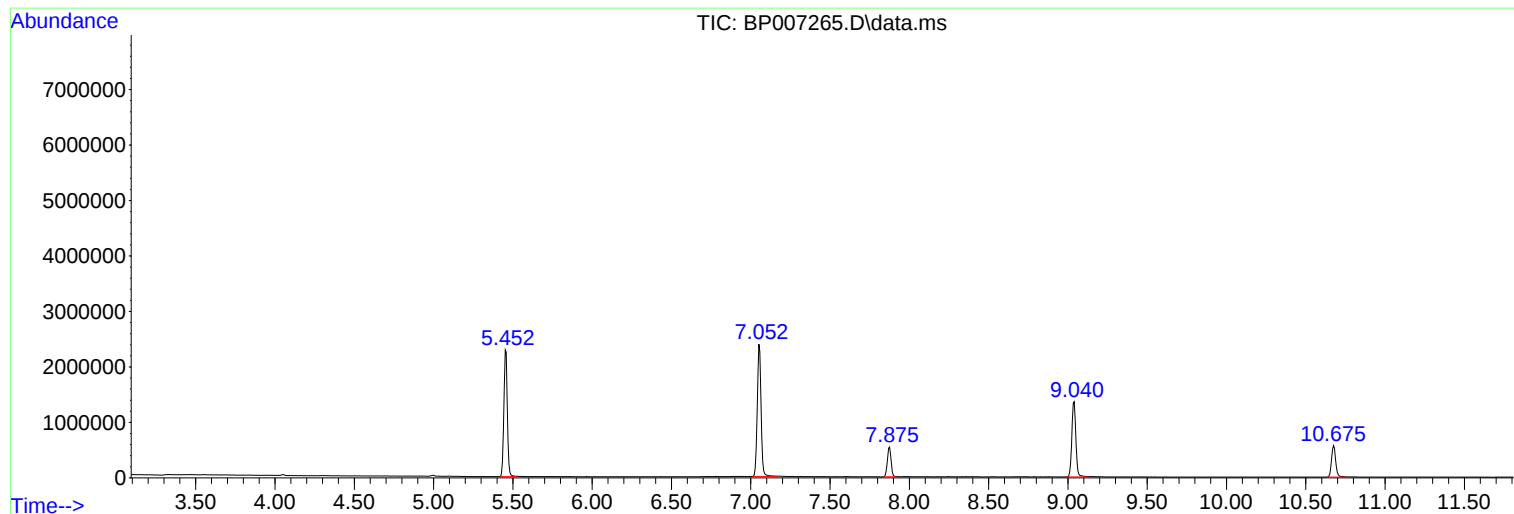

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
Data File : BP007265.D
Acq On : 30 Sep 2021 11:41
Operator : CG/JU
Sample : PB139463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139463BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
Data File : BP007265.D
Acq On : 30 Sep 2021 11:41
Operator : CG/JU
Sample : PB139463BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139463BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------