
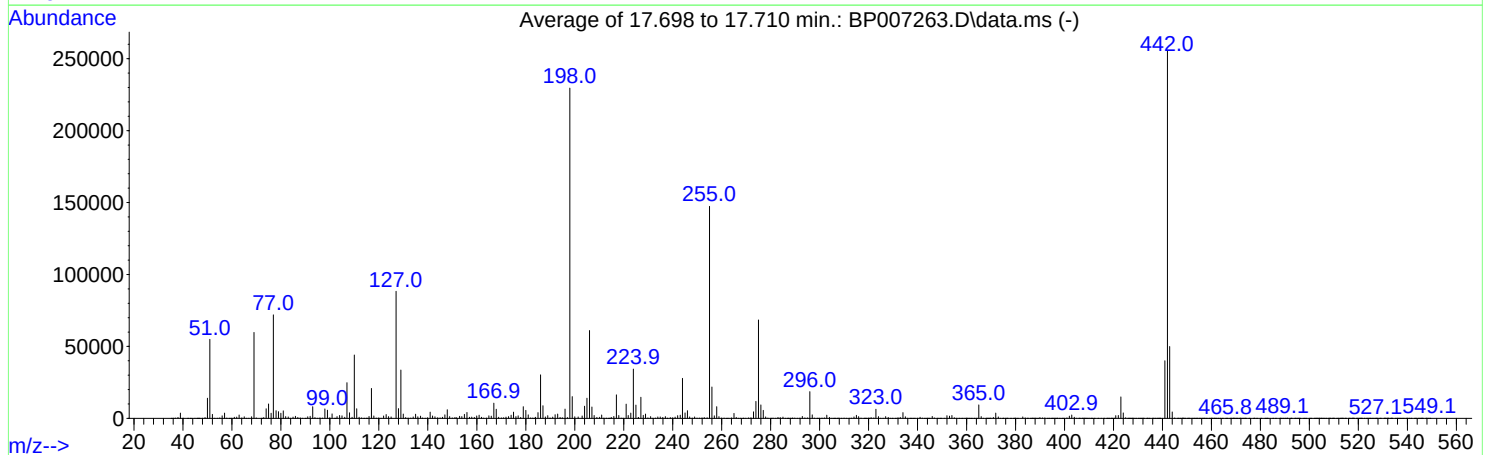


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
 Data File : BP007263.D
 Acq On : 30 Sep 2021 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

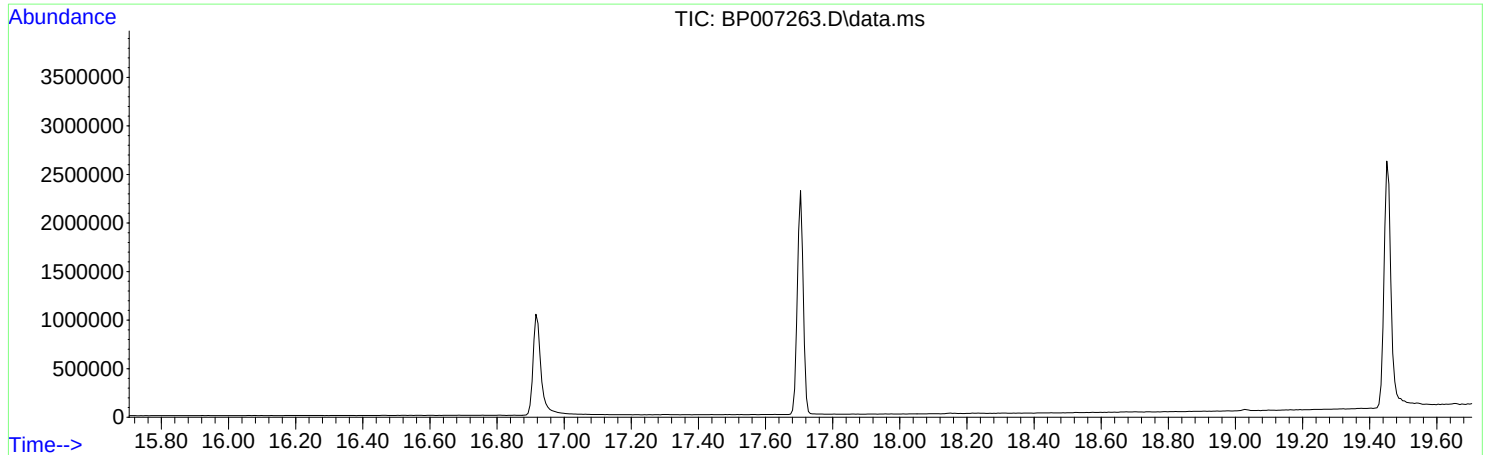




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	54931	PASS
68	69	0.00	2	1.8	1086	PASS
69	198	0.00	100	26.0	59739	PASS
70	69	0.00	2	0.7	390	PASS
127	198	10	80	38.5	88279	PASS
197	198	0.00	2	0.3	610	PASS
198	198	100	100	100.0	229553	PASS
199	198	5	9	6.6	15107	PASS
275	198	10	60	29.8	68406	PASS
365	198	1	100	4.1	9399	PASS
441	198	0.01	100	17.4	40045	PASS
442	442	100	100	100.0	255680	PASS
443	442	15	24	19.5	49930	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
Data File : BP007263.D
Acq On : 30 Sep 2021 10:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 30 11:48:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 29 14:45:49 2021
Response via : Initial Calibration

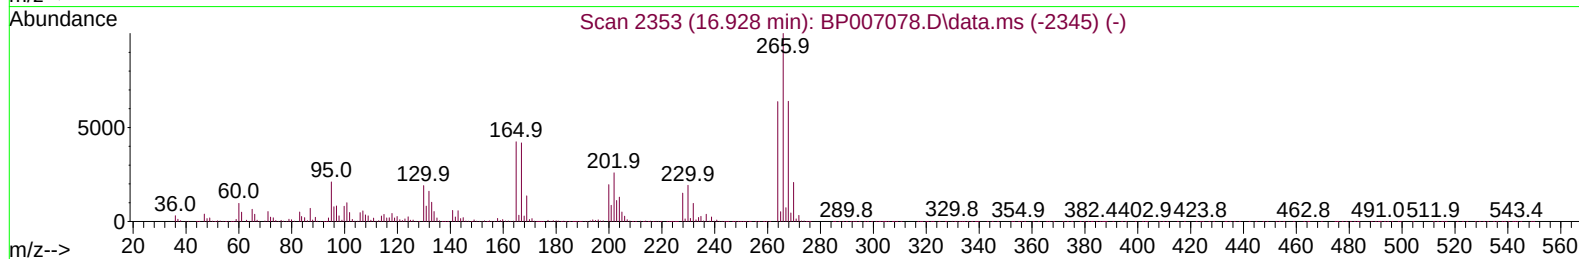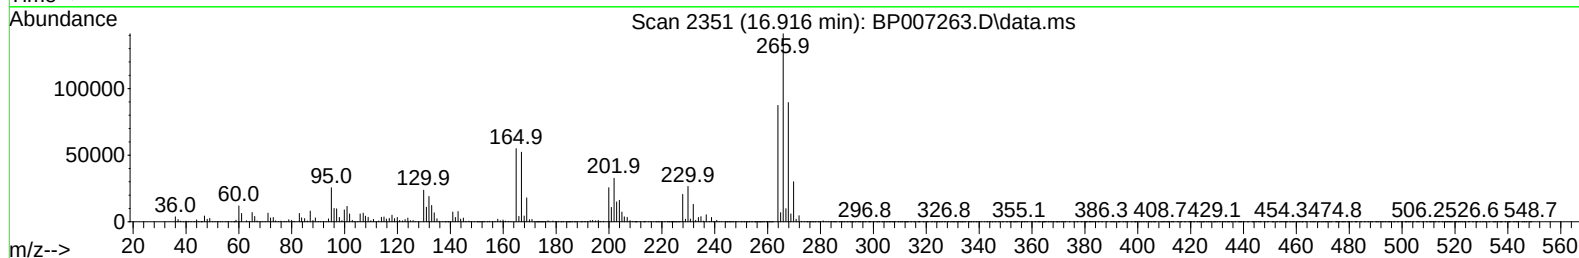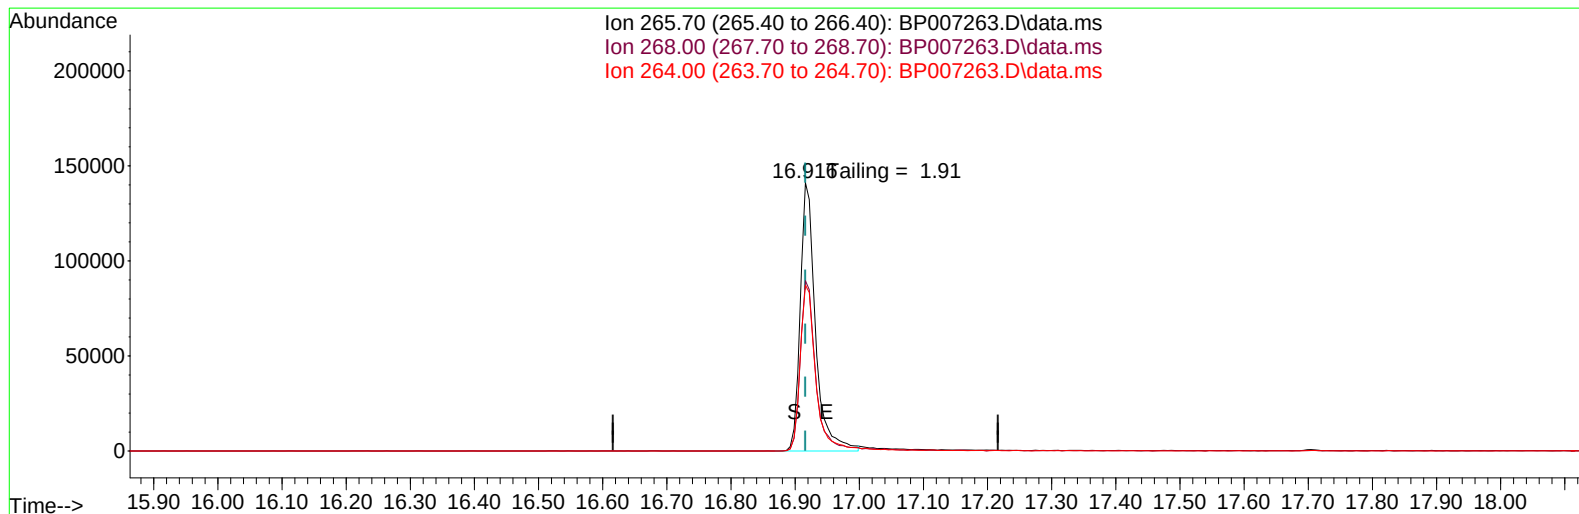

TIC: BP007263.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.000) 145339.91 ng




response 240525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.42
264.00	62.90	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093021\
 Data File : BP007263.D
 Acq On : 30 Sep 2021 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 11:48:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration

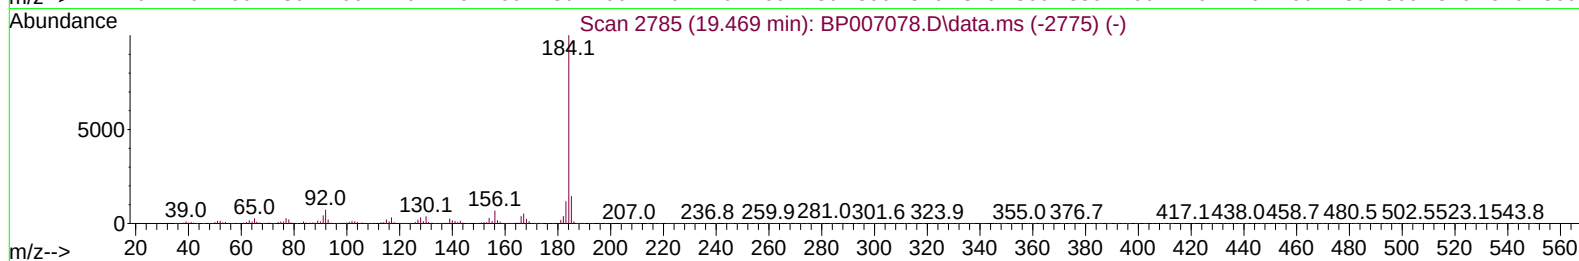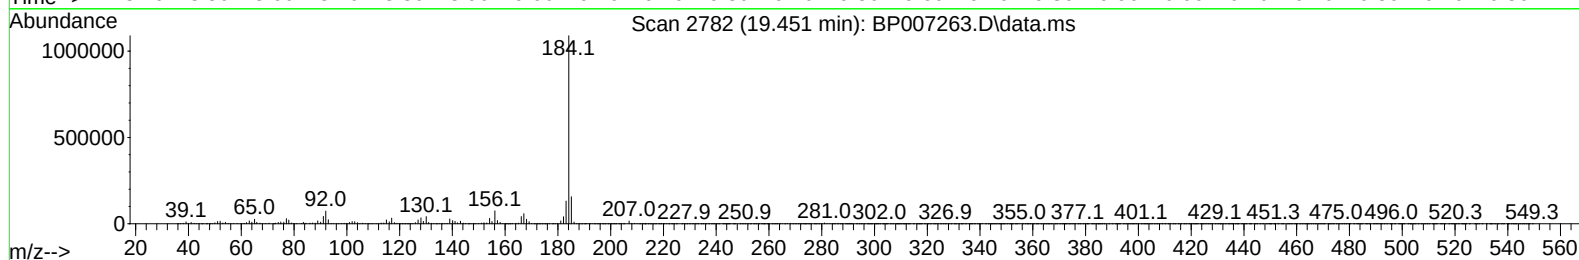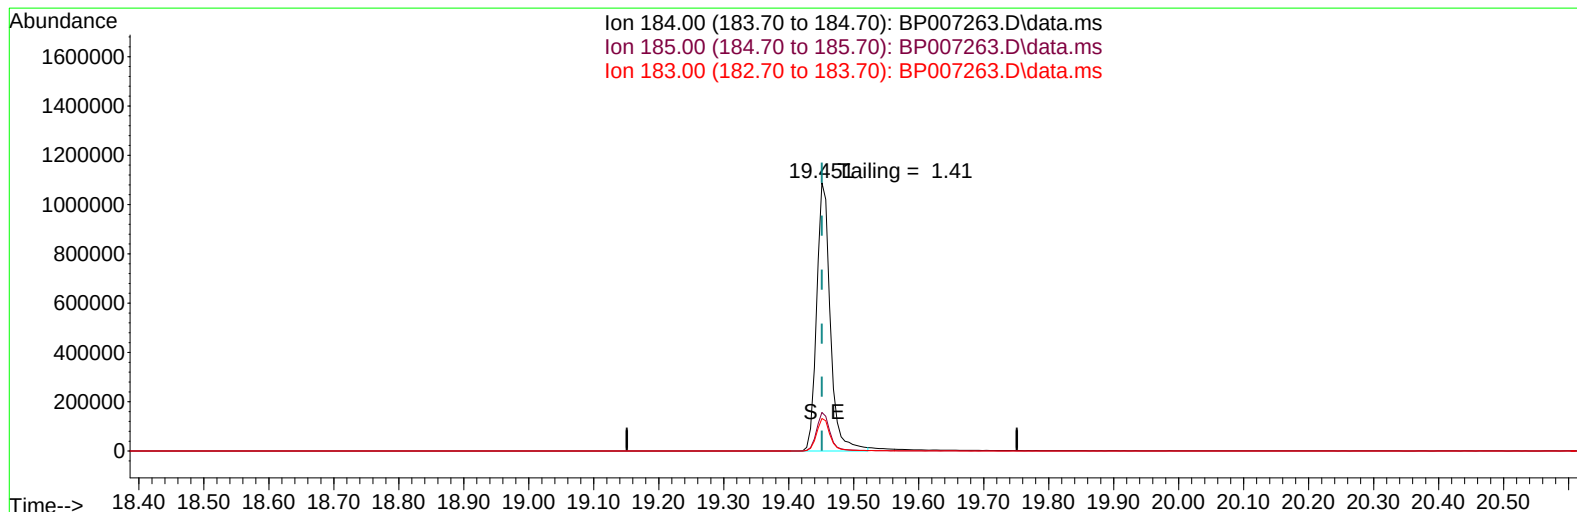

TIC: BP007263.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 271427.21 ng

response 1634911

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.40
183.00	11.90	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2021	BNA_P	BP007263.D
Compound Name	Response	Retention Time
DDT	929219	20.65
DDD	14831	20.22
DDE	1391	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16222	945441	1.72

Instrument :
BNA_P
ClientSampleId :
DFTPP