
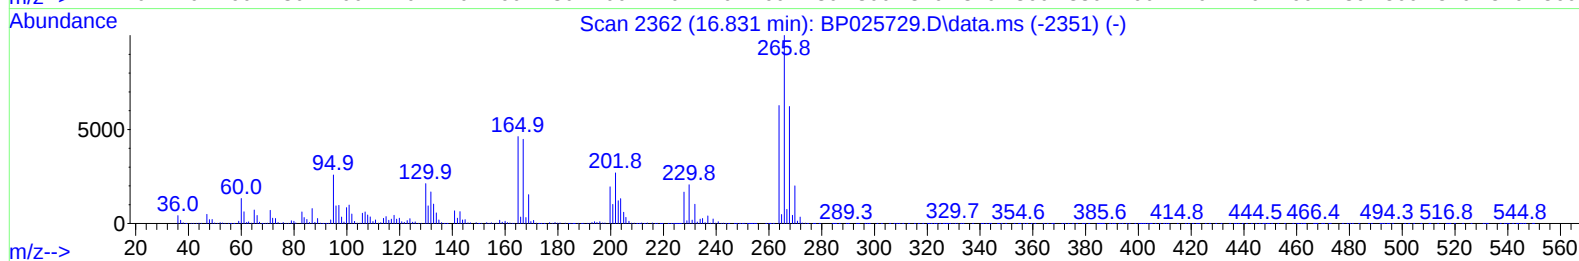
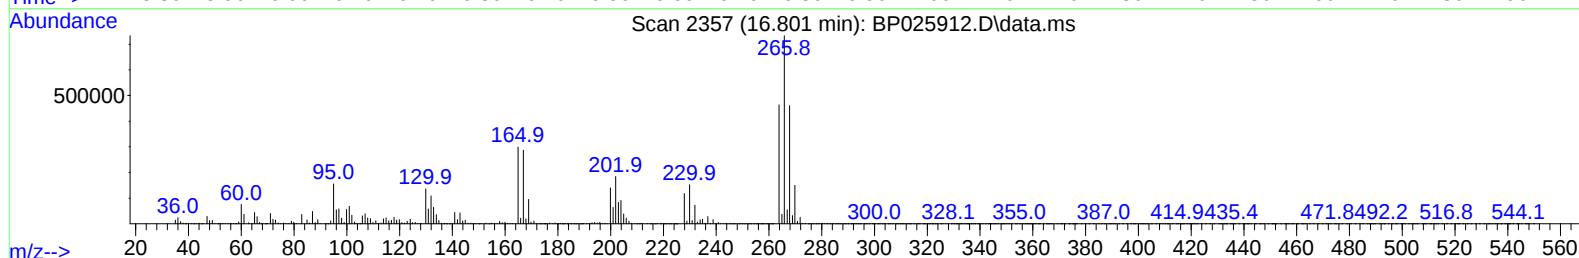


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100325\
Data File : BP025912.D
Acq On : 03 Oct 2025 13:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 13:46:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

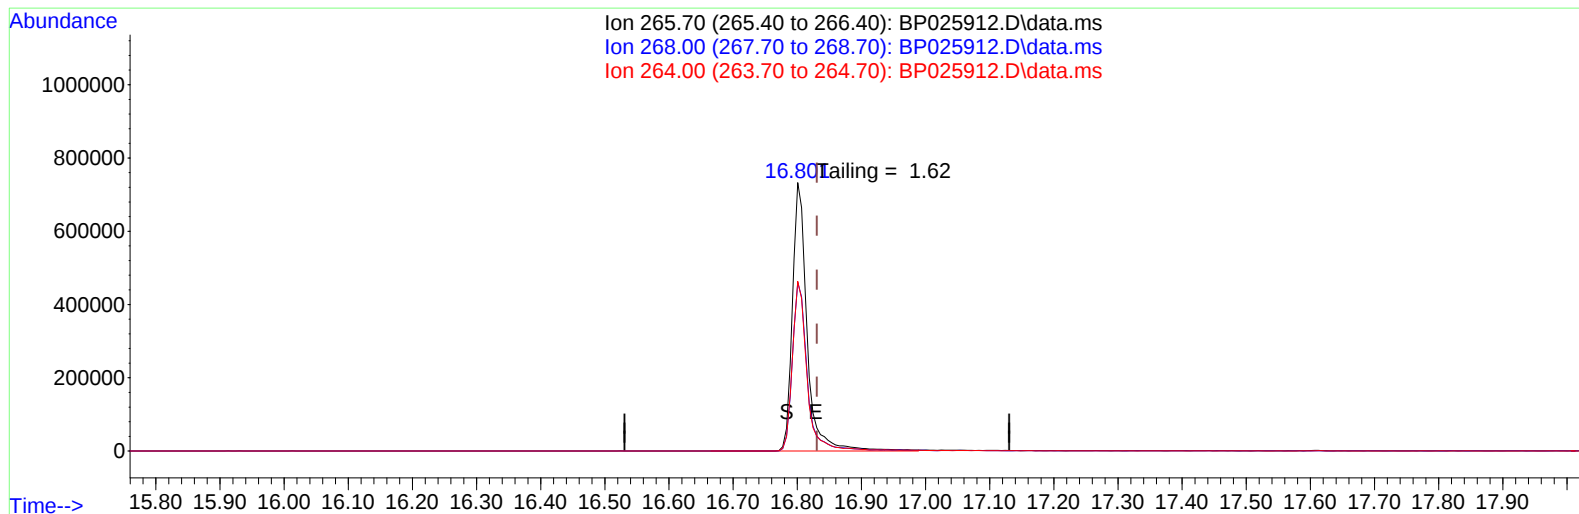

TIC: BP025912.D\data.ms

(70) Pentachlorophenol (C)




16.801min (-0.030) 3092542.18 ng

response 1175251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.80
264.00	62.70	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100325\
Data File : BP025912.D
Acq On : 03 Oct 2025 13:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 13:46:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

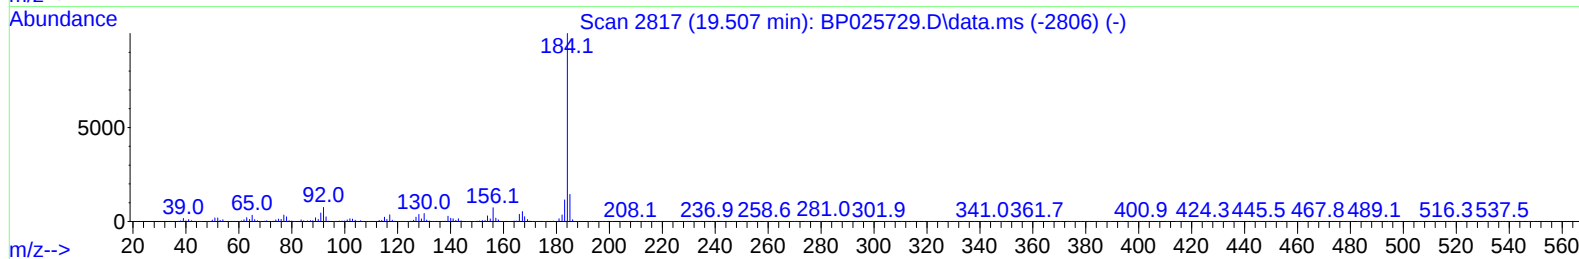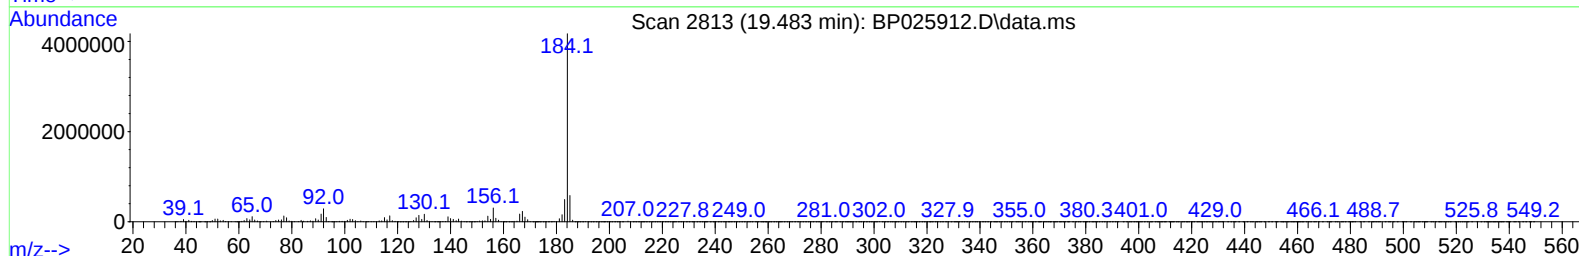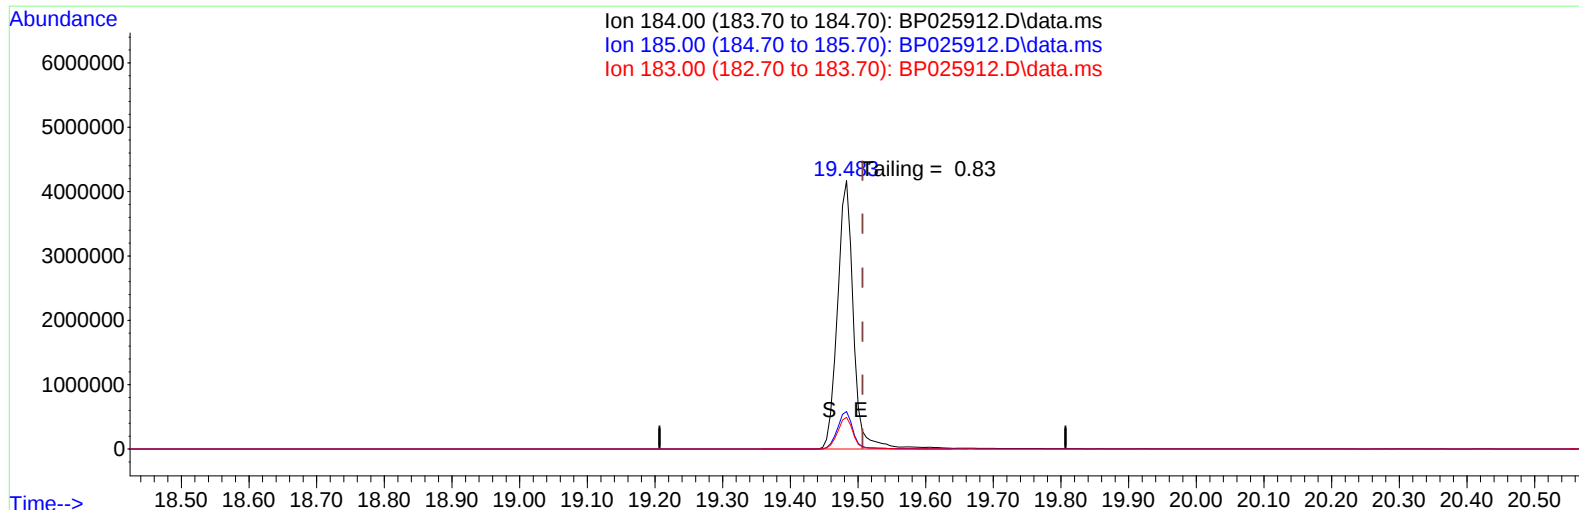

TIC: BP025912.D\data.ms

(77) Benzidine**19.483min (-0.024) 856514.67 ng****response 6735512**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	11.50	11.80
0.00	0.00	0.00