
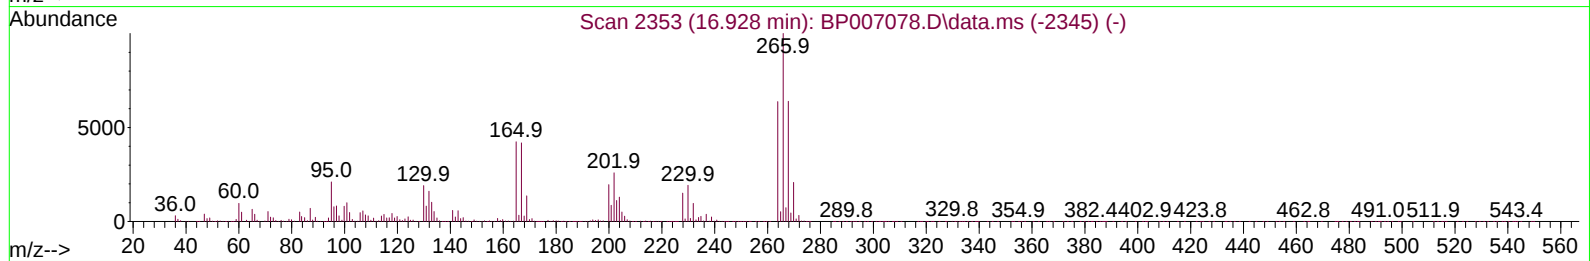
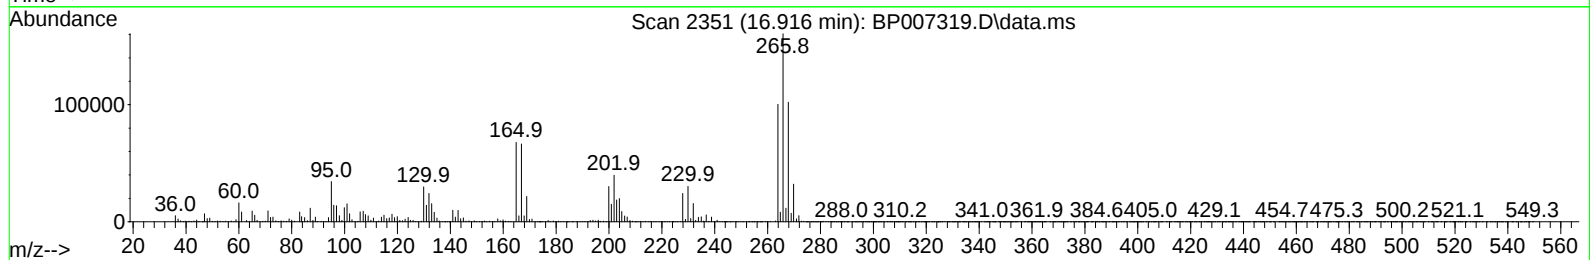


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007319.D
 Acq On : 05 Oct 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:35:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

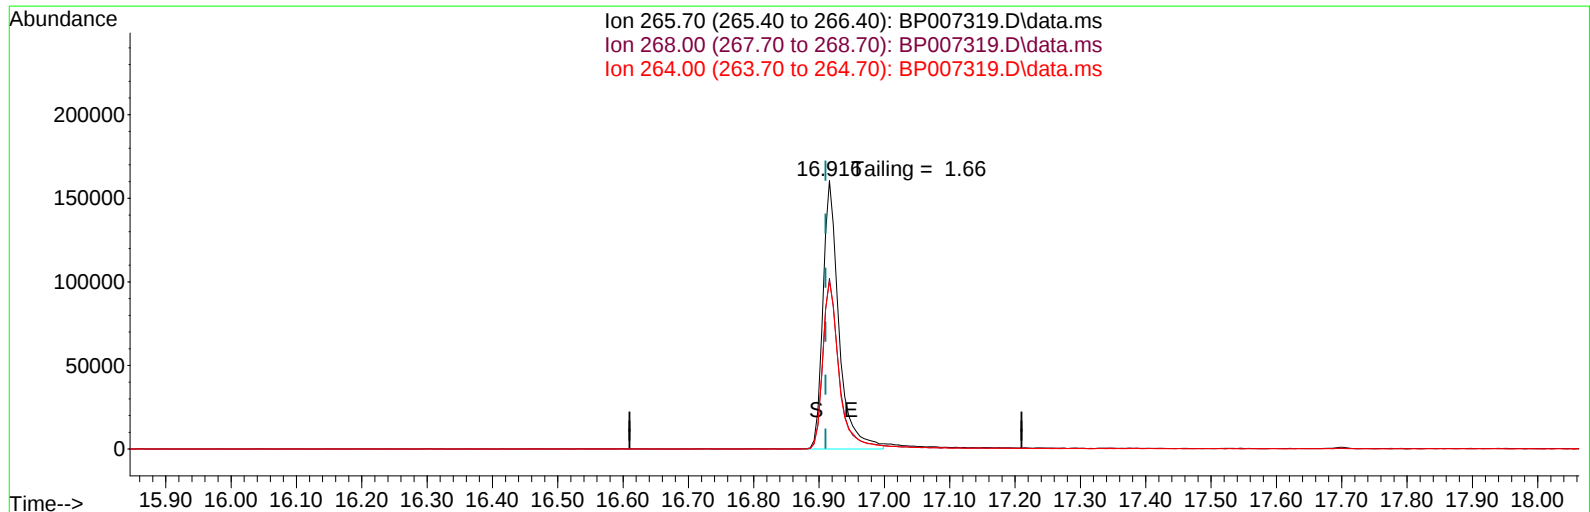

TIC: BP007319.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.006) 221716.85 ng

response 281863

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.54
264.00	62.90	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007319.D
 Acq On : 05 Oct 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:35:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

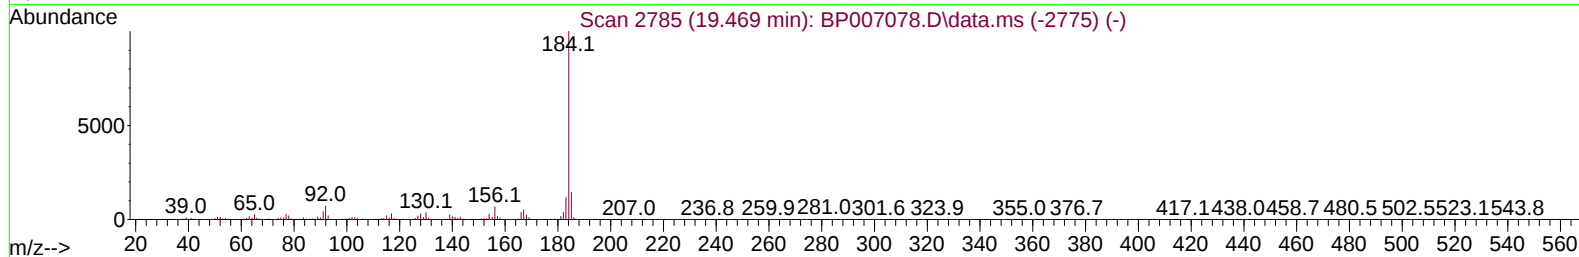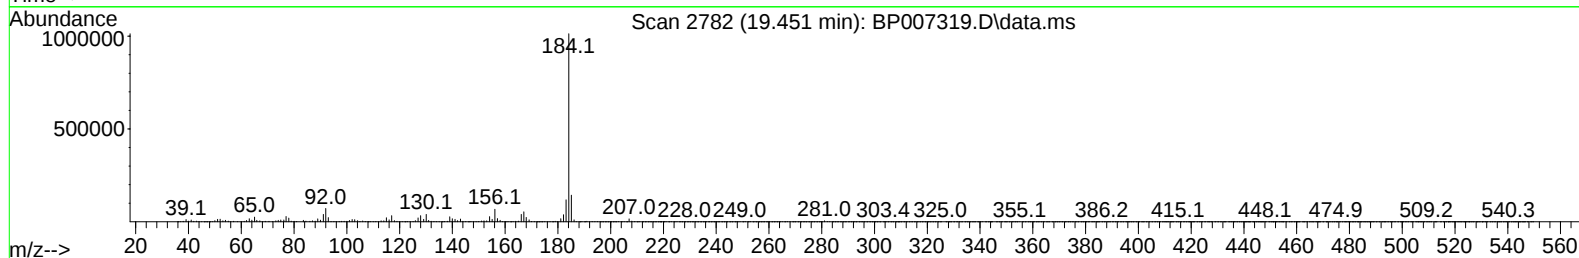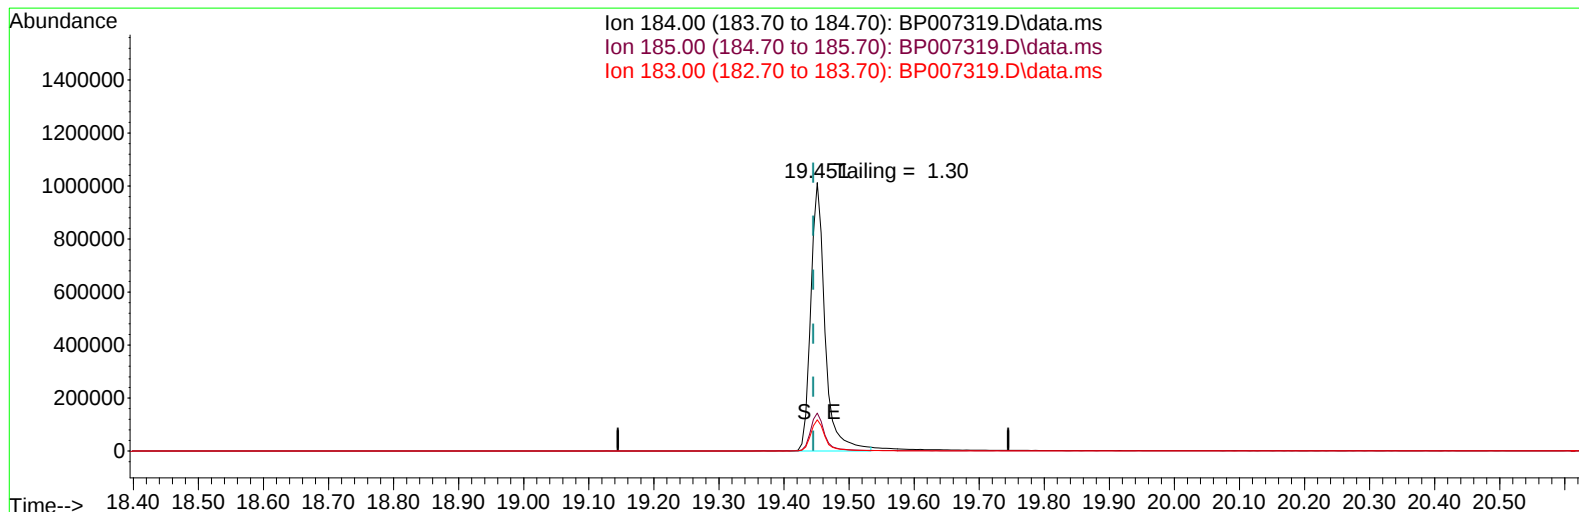

TIC: BP007319.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 174782.41 ng

response 1579173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.12
183.00	11.90	11.66
0.00	0.00	0.00