

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007321.D
 Acq On : 05 Oct 2021 10:51
 Operator : CG/JU
 Sample : PB139583BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139583BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	395	401	418	rBV	2970081	4523509	45.85%	10.520%
2	7.046	666	673	701	rBV	2559264	4363769	44.23%	10.148%
3	7.864	804	812	822	rBV	619982	966316	9.79%	2.247%
4	9.028	997	1010	1028	rBV	1637792	2842081	28.80%	6.610%
5	10.663	1279	1288	1305	rBV	679905	1253125	12.70%	2.914%
6	13.122	1699	1706	1731	rBV	4340630	6624175	67.14%	15.405%
7	14.498	1933	1940	1967	rBV	954411	1586275	16.08%	3.689%
8	15.998	2187	2195	2233	rBV	2758985	4841195	49.07%	11.259%
9	17.251	2402	2408	2423	rBV	1129156	1840143	18.65%	4.279%
10	19.810	2838	2843	2854	rBV	7810987	9866654	100.00%	22.946%
11	21.339	3099	3103	3113	rBV	1451712	2059958	20.88%	4.791%
12	23.751	3507	3513	3528	rVB	1023986	2232481	22.63%	5.192%




Sum of corrected areas: 42999681

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007321.D
Acq On : 05 Oct 2021 10:51
Operator : CG/JU
Sample : PB139583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139583BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

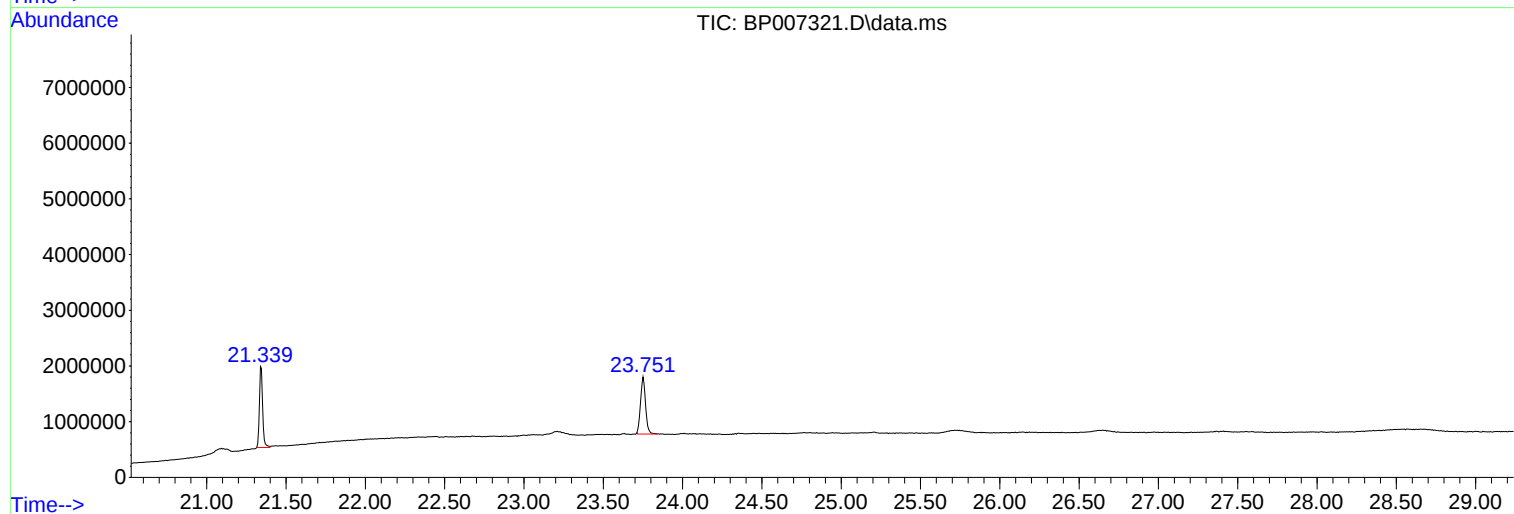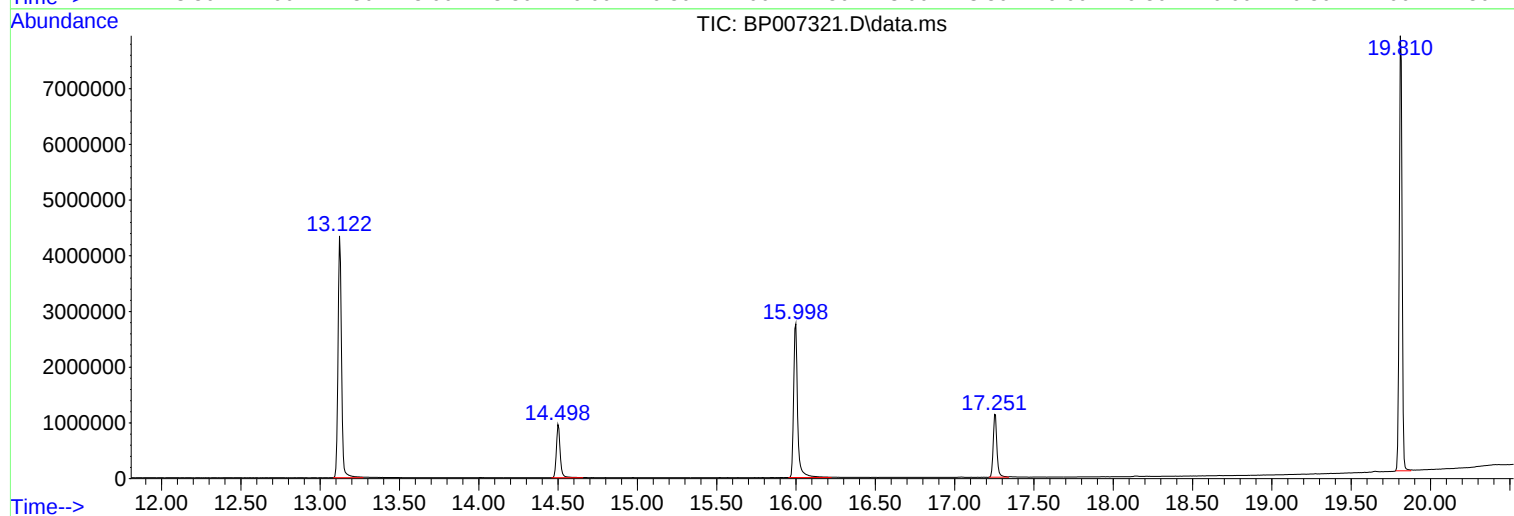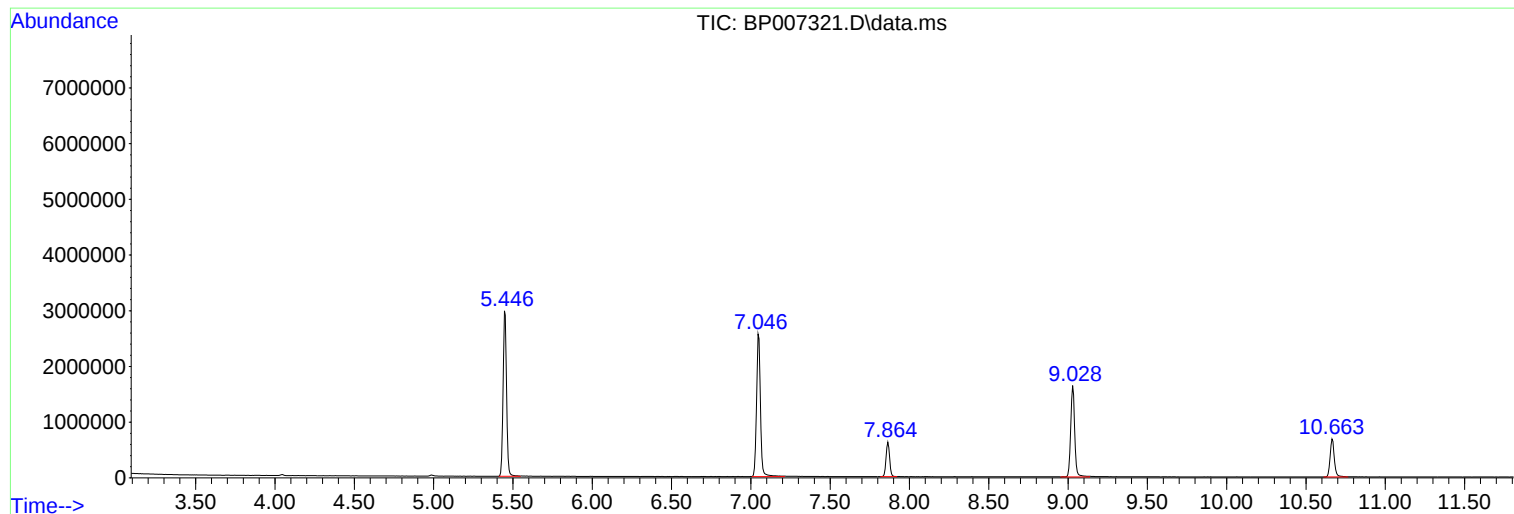

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007321.D
Acq On : 05 Oct 2021 10:51
Operator : CG/JU
Sample : PB139583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139583BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007321.D
Acq On : 05 Oct 2021 10:51
Operator : CG/JU
Sample : PB139583BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139583BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------