

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007329.D
 Acq On : 05 Oct 2021 16:28
 Operator : CG/JU
 Sample : PB139627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139627BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007329.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	420	rBV	3443731	5145016	54.55%	11.268%
2	7.046	665	673	703	rBV	2891968	4925520	52.23%	10.787%
3	7.864	804	812	822	rBV	686325	1112209	11.79%	2.436%
4	9.028	1001	1010	1037	rBV	1818946	3281218	34.79%	7.186%
5	10.663	1279	1288	1303	rBV	761801	1437154	15.24%	3.148%
6	13.122	1698	1706	1729	rBV	4634691	7476378	79.27%	16.374%
7	14.498	1933	1940	1956	rBV	1072845	1771248	18.78%	3.879%
8	15.992	2186	2194	2230	rBV	2689917	5220836	55.36%	11.434%
9	17.251	2401	2408	2424	rBV	1178125	1961332	20.80%	4.296%
10	19.810	2837	2843	2855	rBV	7593551	9431067	100.00%	20.655%
11	21.339	3098	3103	3115	rBV	1339171	2009159	21.30%	4.400%
12	23.745	3506	3512	3524	rVB2	797113	1888504	20.02%	4.136%




Sum of corrected areas: 45659641

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007329.D
Acq On : 05 Oct 2021 16:28
Operator : CG/JU
Sample : PB139627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139627BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

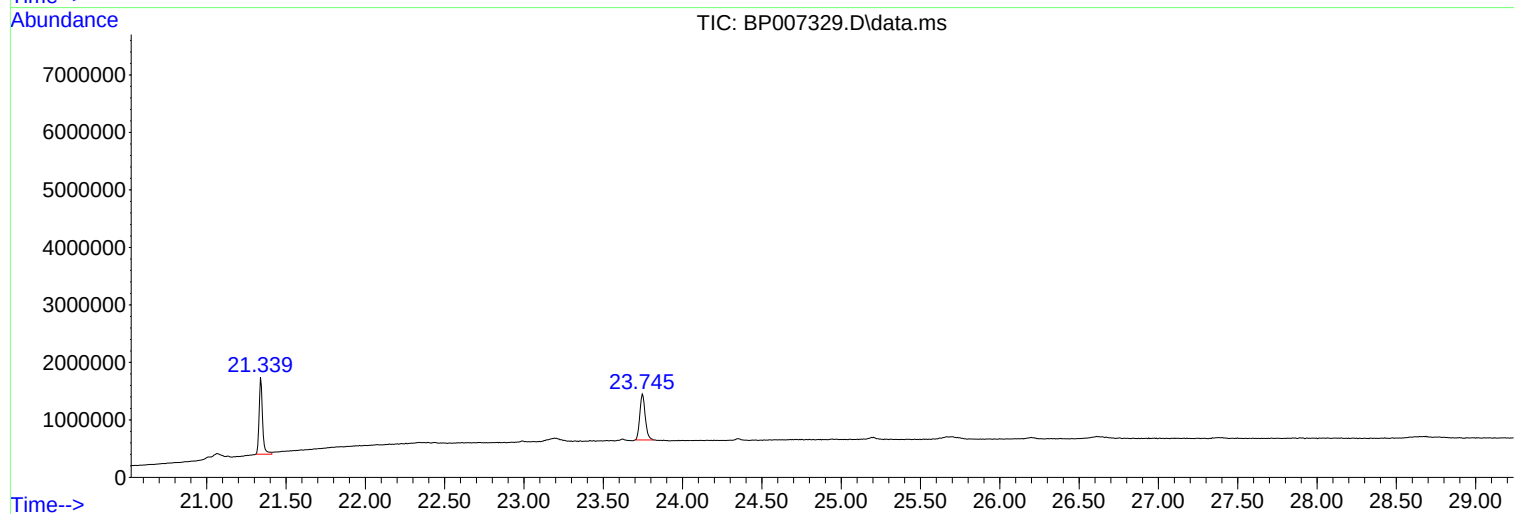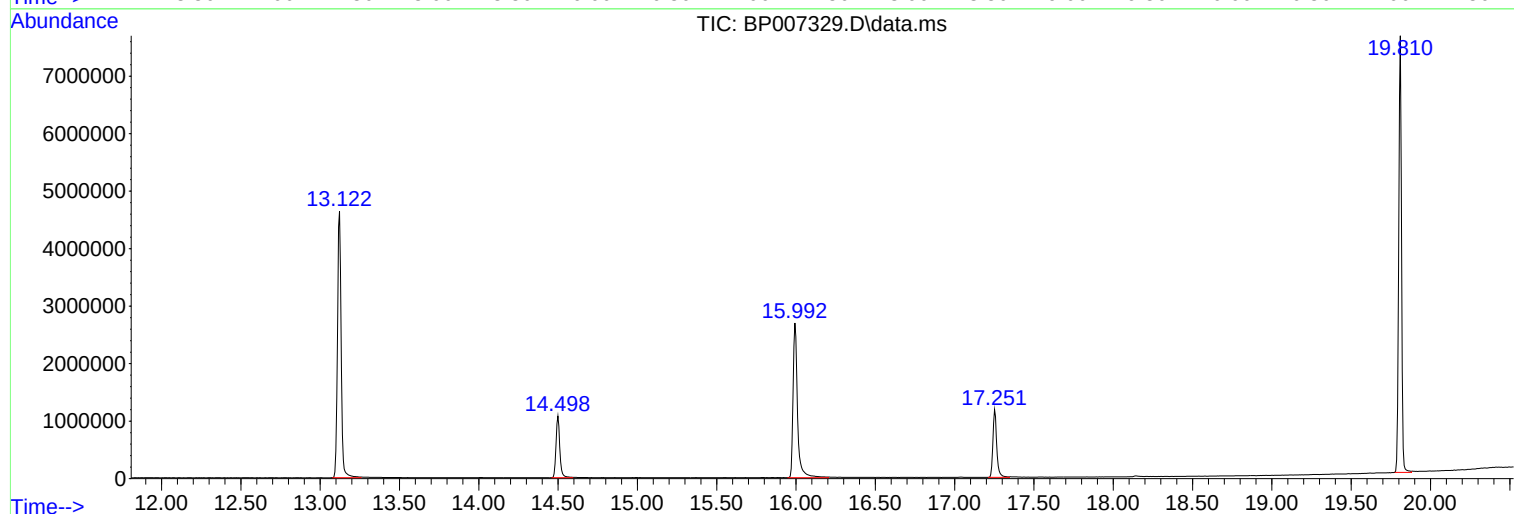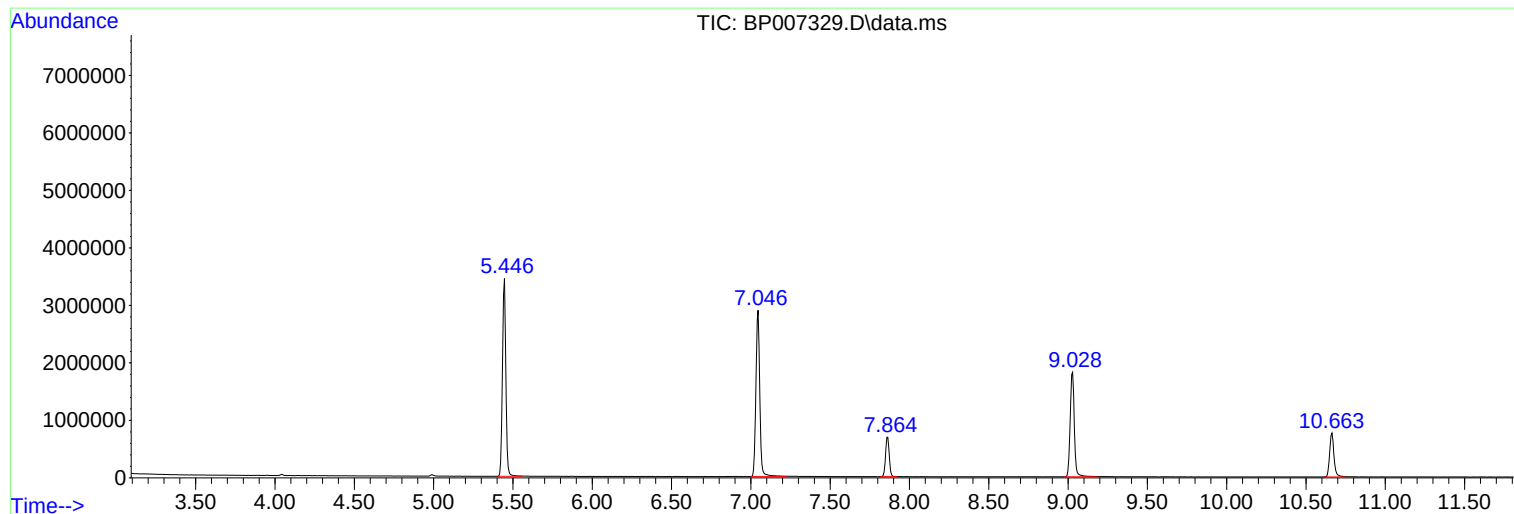

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007329.D
Acq On : 05 Oct 2021 16:28
Operator : CG/JU
Sample : PB139627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139627BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007329.D
Acq On : 05 Oct 2021 16:28
Operator : CG/JU
Sample : PB139627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139627BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------