
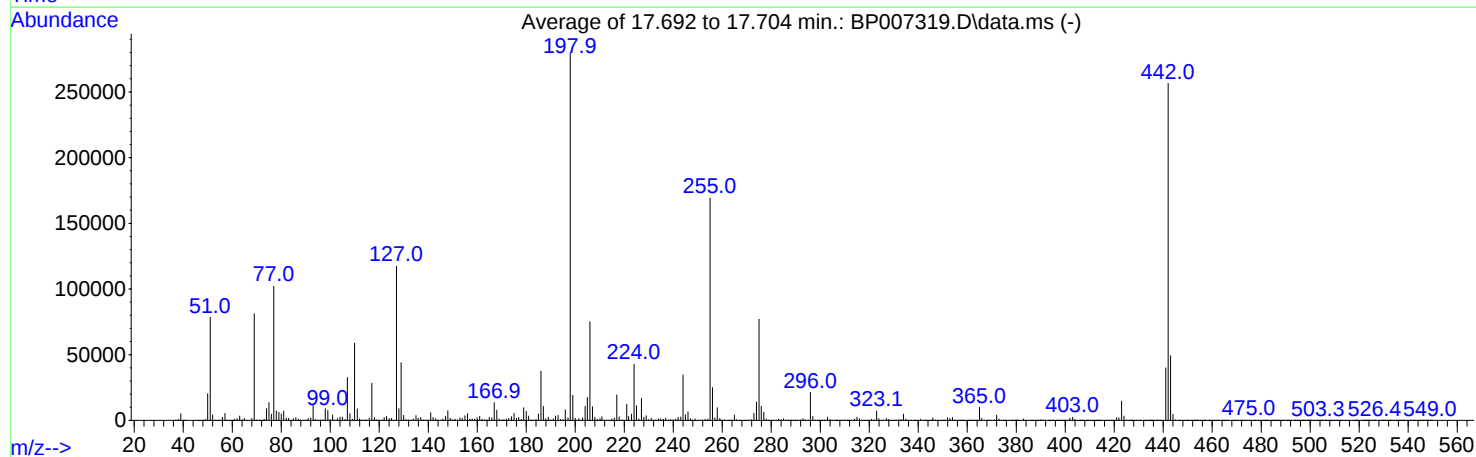


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007319.D
 Acq On : 05 Oct 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

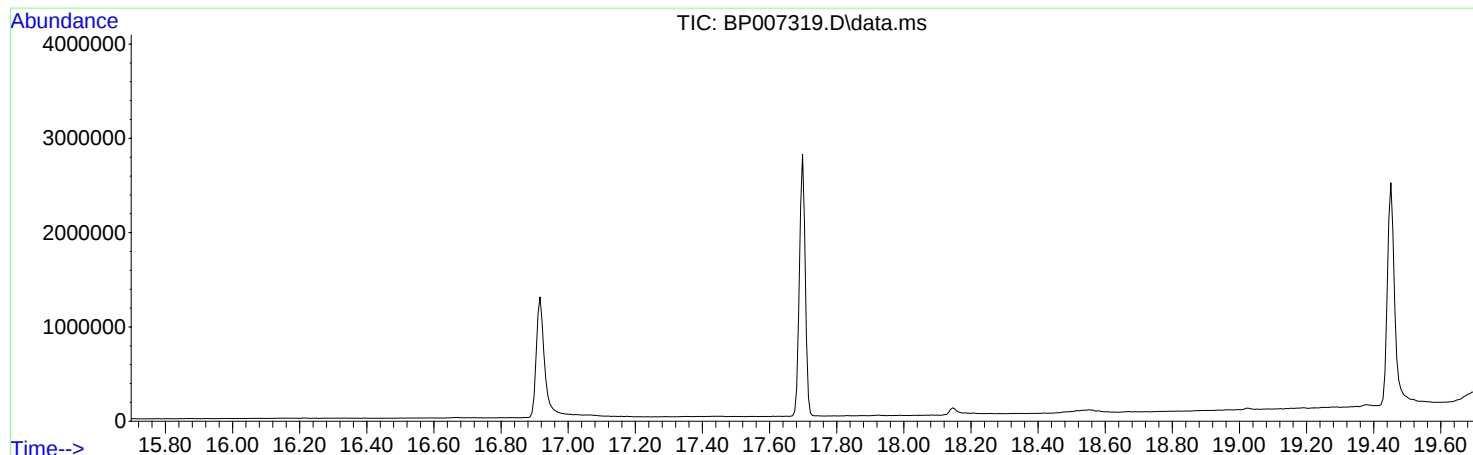




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	78434	PASS
68	69	0.00	2	1.7	1368	PASS
69	198	0.00	100	29.0	81177	PASS
70	69	0.00	2	0.5	412	PASS
127	198	10	80	41.9	117278	PASS
197	198	0.00	2	0.7	1912	PASS
198	198	100	100	100.0	280041	PASS
199	198	5	9	6.8	19061	PASS
275	198	10	60	27.5	76948	PASS
365	198	1	100	3.5	9854	PASS
441	198	0.01	100	14.3	39945	PASS
442	442	100	100	100.0	256491	PASS
443	442	15	24	19.2	49198	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007319.D
 Acq On : 05 Oct 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 05 11:35:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

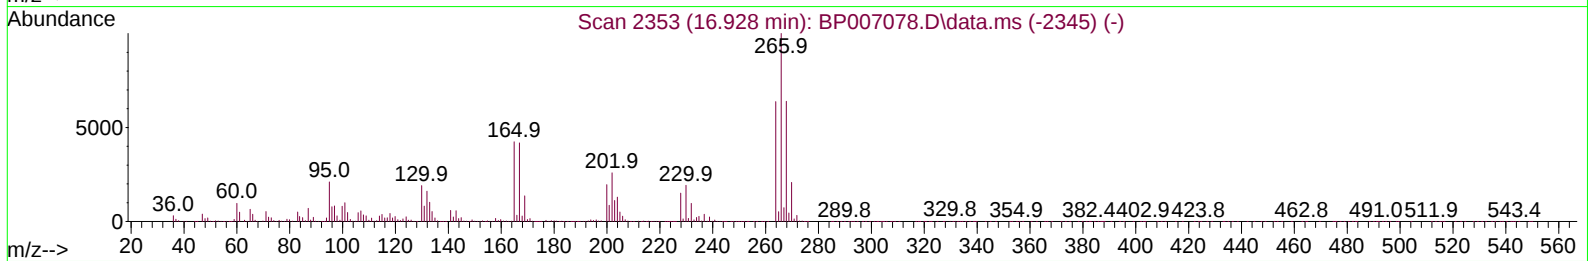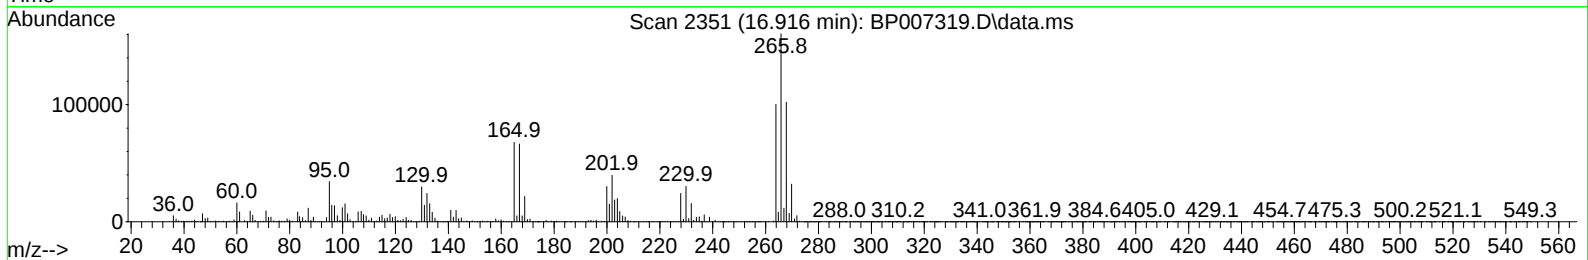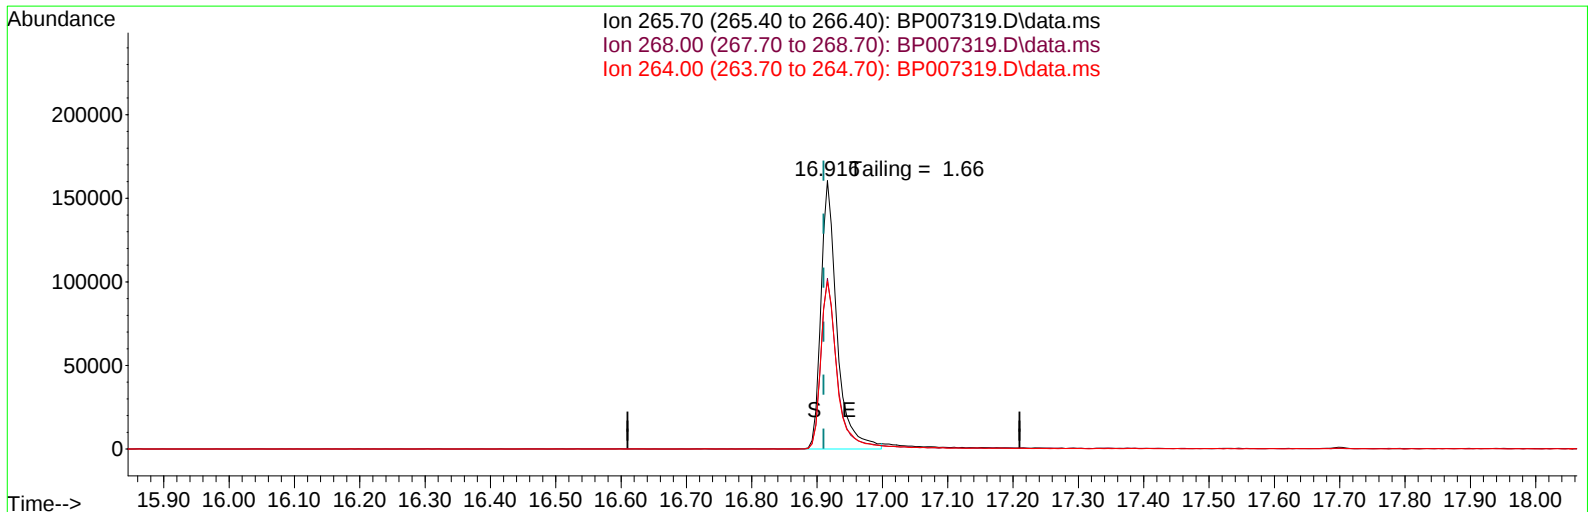

TIC: BP007319.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 221716.85 ng




response 281863

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.54
264.00	62.90	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007319.D
 Acq On : 05 Oct 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 05 11:35:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

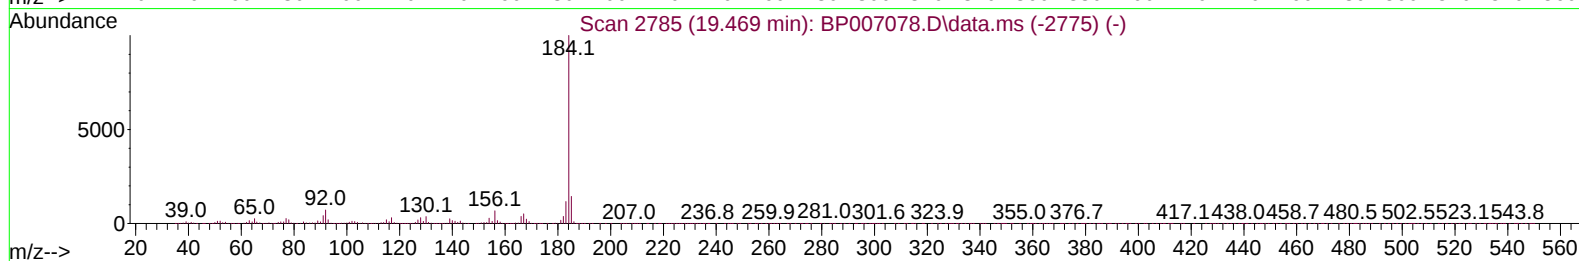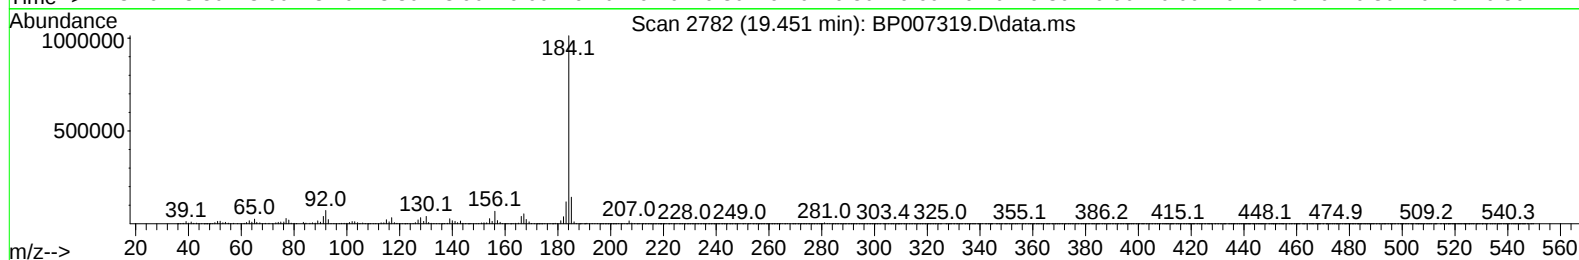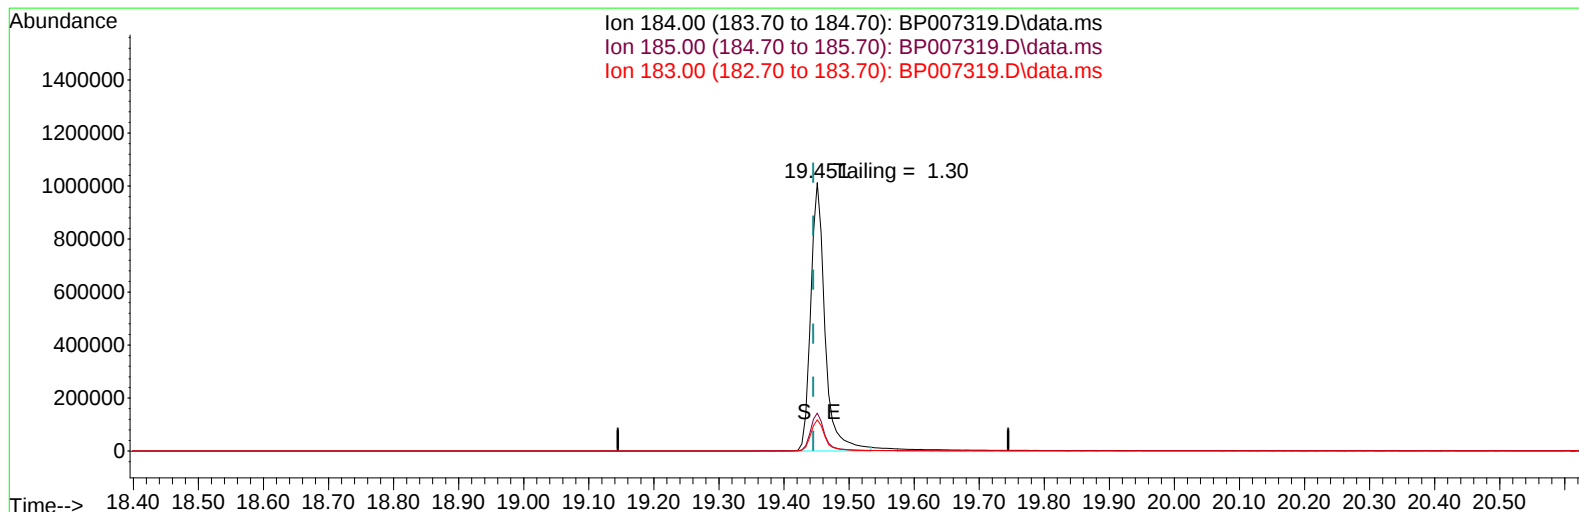

TIC: BP007319.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 174782.41 ng

response 1579173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.12
183.00	11.90	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2021	BNA_P	BP007319.D
Compound Name	Response	Retention Time
DDT	853031	20.65
DDD	12672	20.22
DDE	2555	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15227	868258	1.75

Instrument :
BNA_P
ClientSampleId :
DFTPP