
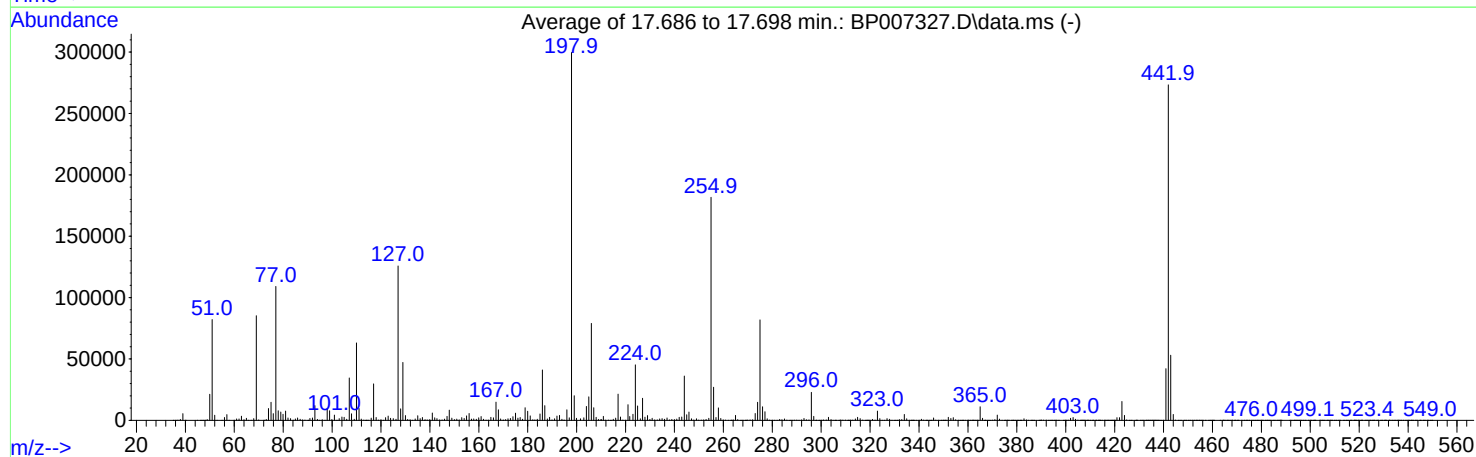


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007327.D
 Acq On : 05 Oct 2021 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

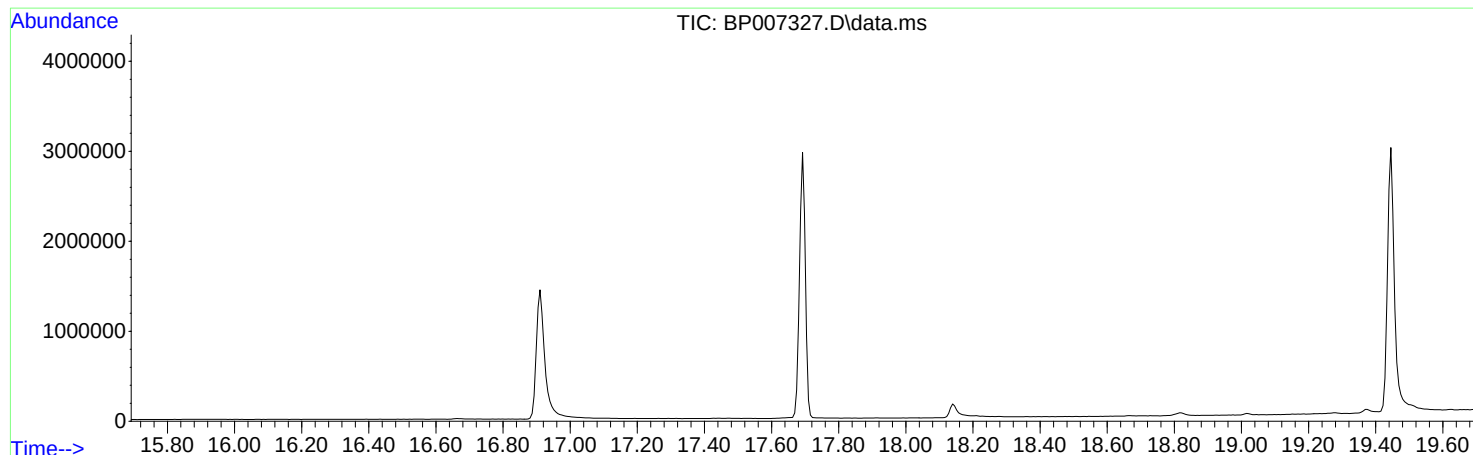




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	82127	PASS
68	69	0.00	2	1.6	1393	PASS
69	198	0.00	100	28.4	85241	PASS
70	69	0.00	2	0.5	398	PASS
127	198	10	80	42.0	125726	PASS
197	198	0.00	2	0.7	2155	PASS
198	198	100	100	100.0	299647	PASS
199	198	5	9	6.7	20069	PASS
275	198	10	60	27.3	81890	PASS
365	198	1	100	3.7	11024	PASS
441	198	0.01	100	14.1	42146	PASS
442	442	100	100	100.0	273319	PASS
443	442	15	24	19.4	53044	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
Data File : BP007327.D
Acq On : 05 Oct 2021 15:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 05 16:55:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 12:49:05 2021
Response via : Initial Calibration

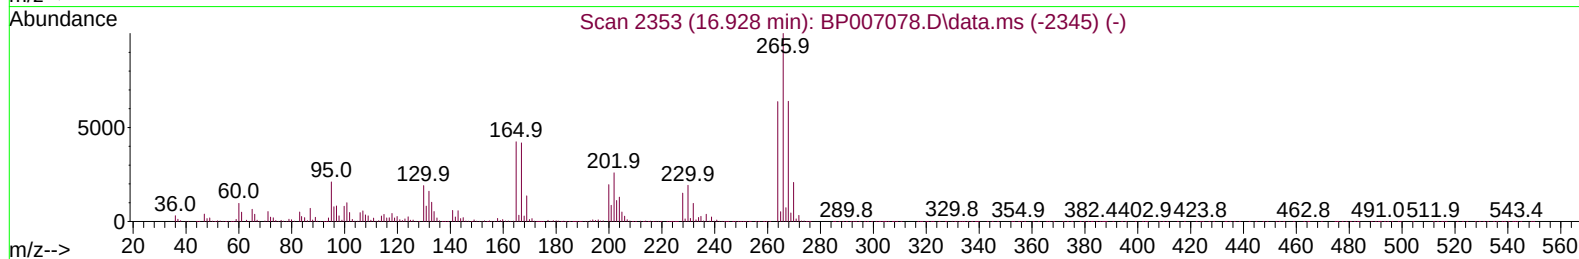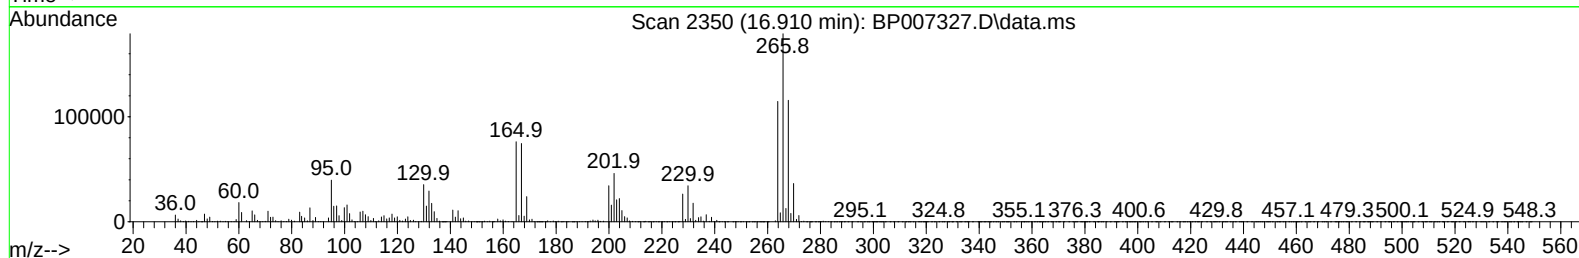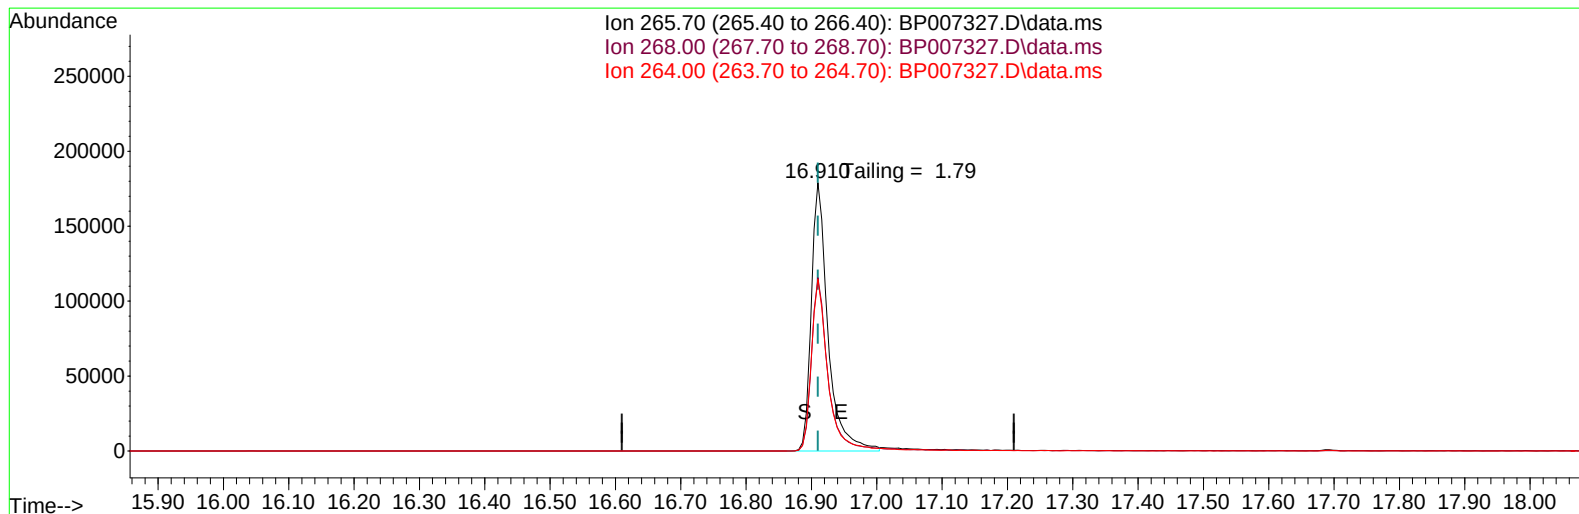

TIC: BP007327.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 74756.39 ng




response 325034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.57
264.00	62.90	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100521\
 Data File : BP007327.D
 Acq On : 05 Oct 2021 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 05 16:55:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

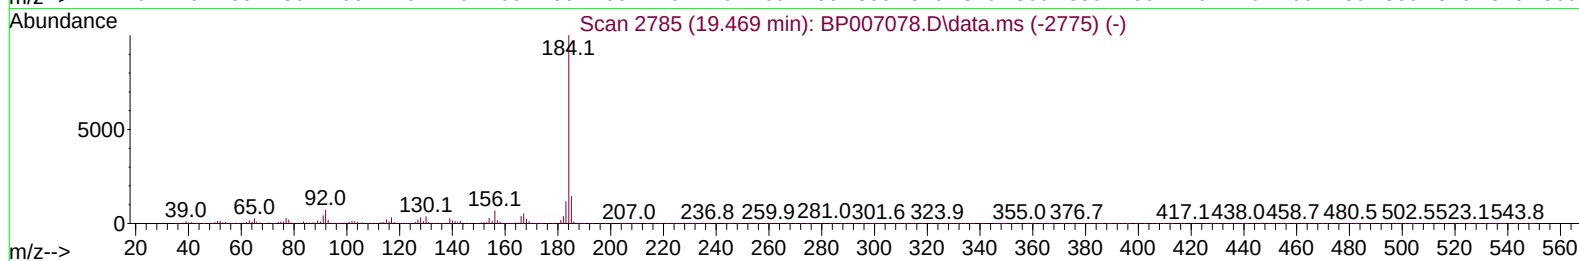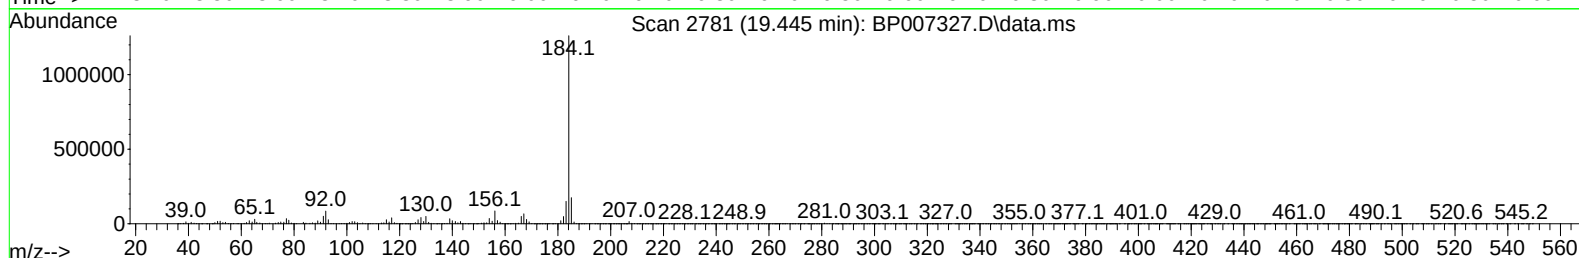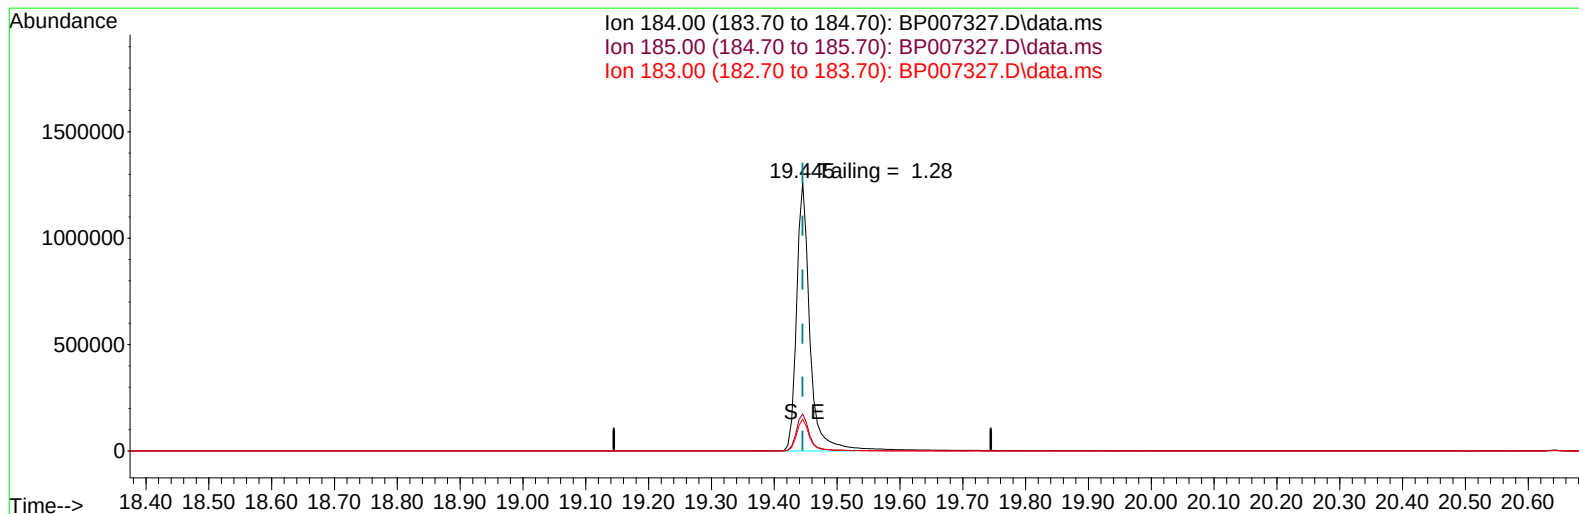

TIC: BP007327.D\data.ms

(77) Benzidine

19.445min (+ 0.000) 32587.47 ng

response 1894770

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.83
183.00	11.90	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2021	BNA_P	BP007327.D
Compound Name	Response	Retention Time
DDT	977156	20.63
DDD	10699	20.21
DDE	1474	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12173	989329	1.23