

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003522.D
 Acq On : 06 Oct 2020 15:16
 Operator : CG/JU
 Sample : PB132129BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132129BL

Quant Time: Oct 06 16:25:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 14:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.493	152	81213	20.00	ng	# 0.00
21) Naphthalene-d8	10.269	136	310759	20.00	ng	# 0.00
39) Acenaphthene-d10	14.151	164	181949	20.00	ng	0.00
64) Phenanthrene-d10	16.916	188	380706	20.00	ng	0.00
76) Chrysene-d12	21.022	240	408457	20.00	ng	0.00
86) Perylene-d12	23.186	264	446545	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.105	112	634847	136.50	ng	0.00
7) Phenol-d6	6.699	99	781407	126.05	ng	0.00
23) Nitrobenzene-d5	8.646	82	526999	99.63	ng	0.00
42) 2,4,6-Tribromophenol	15.657	330	284315	102.45	ng	0.00
45) 2-Fluorobiphenyl	12.763	172	1121057	90.11	ng	-0.01
79) Terphenyl-d14	19.498	244	1617142	82.49	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003522.D
Acq On : 06 Oct 2020 15:16
Operator : CG/JU
Sample : PB132129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132129BL

Quant Time: Oct 06 16:25:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

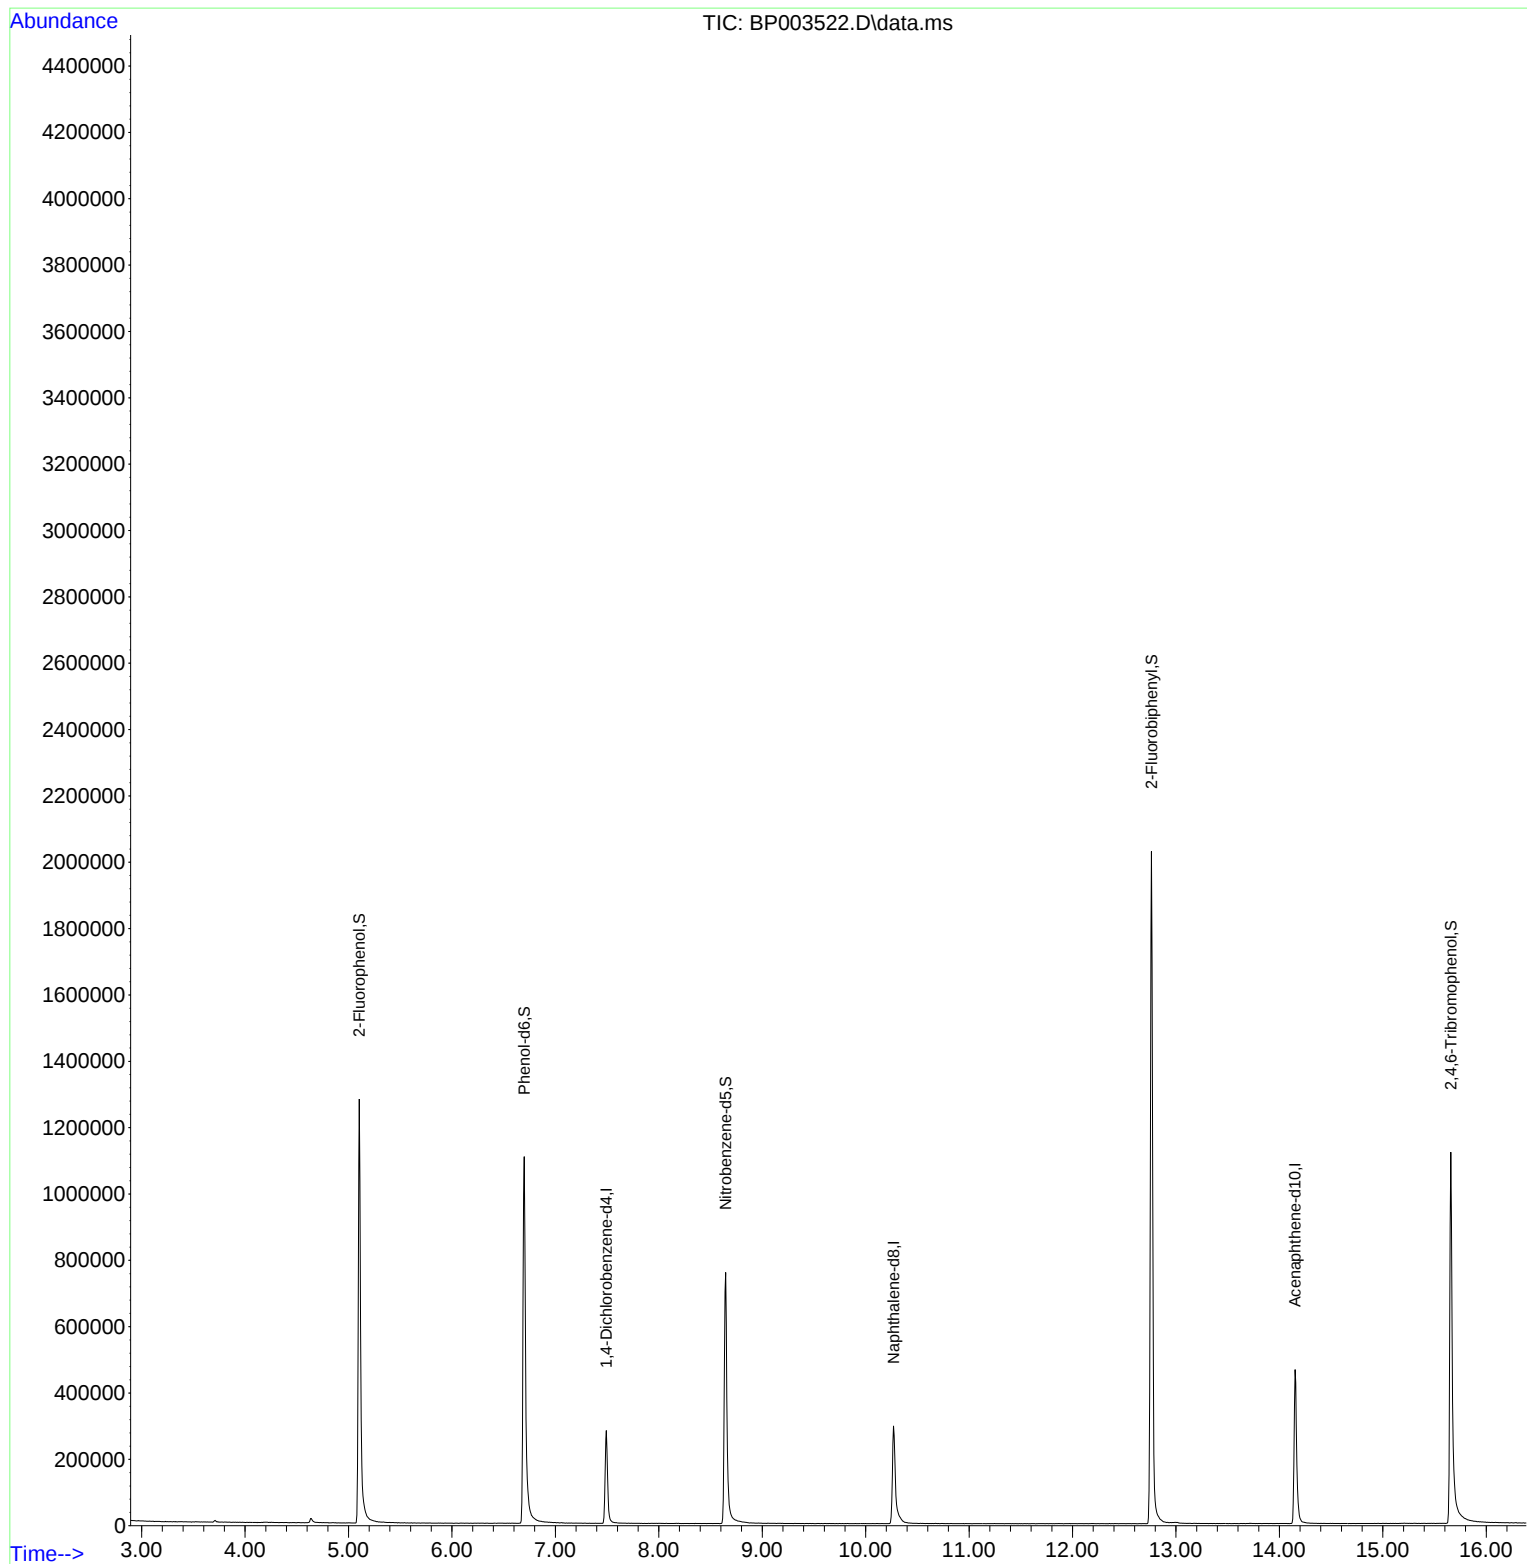

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003522.D
Acq On : 06 Oct 2020 15:16
Operator : CG/JU
Sample : PB132129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132129BL

Quant Time: Oct 06 16:25:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

