

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003551.D
 Acq On : 07 Oct 2020 10:41
 Operator : CG/JU
 Sample : L4271-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GV-CONCRETE

Quant Time: Oct 07 13:07:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 14:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.493	152	74163	20.00	ng	# 0.00
21) Naphthalene-d8	10.269	136	295764	20.00	ng	# 0.00
39) Acenaphthene-d10	14.151	164	187903	20.00	ng	0.00
64) Phenanthrene-d10	16.910	188	440181	20.00	ng	# 0.00
76) Chrysene-d12	21.016	240	540306	20.00	ng	-0.01
86) Perylene-d12	23.186	264	529137	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.175	112	3837	0.90	ng	0.06
7) Phenol-d6	6.722	99	67629	11.95	ng	0.02
23) Nitrobenzene-d5	8.646	82	389459	77.36	ng	0.00
42) 2,4,6-Tribromophenol	15.663	330	5	0.00	ng	0.00
45) 2-Fluorobiphenyl	12.763	172	865129	67.34	ng	-0.01
79) Terphenyl-d14	19.492	244	1495177	57.66	ng	-0.01
Target Compounds						
50) Dimethylphthalate	13.634	163	48884	3.26	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003551.D
Acq On : 07 Oct 2020 10:41
Operator : CG/JU
Sample : L4271-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GV-CONCRETE

Quant Time: Oct 07 13:07:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

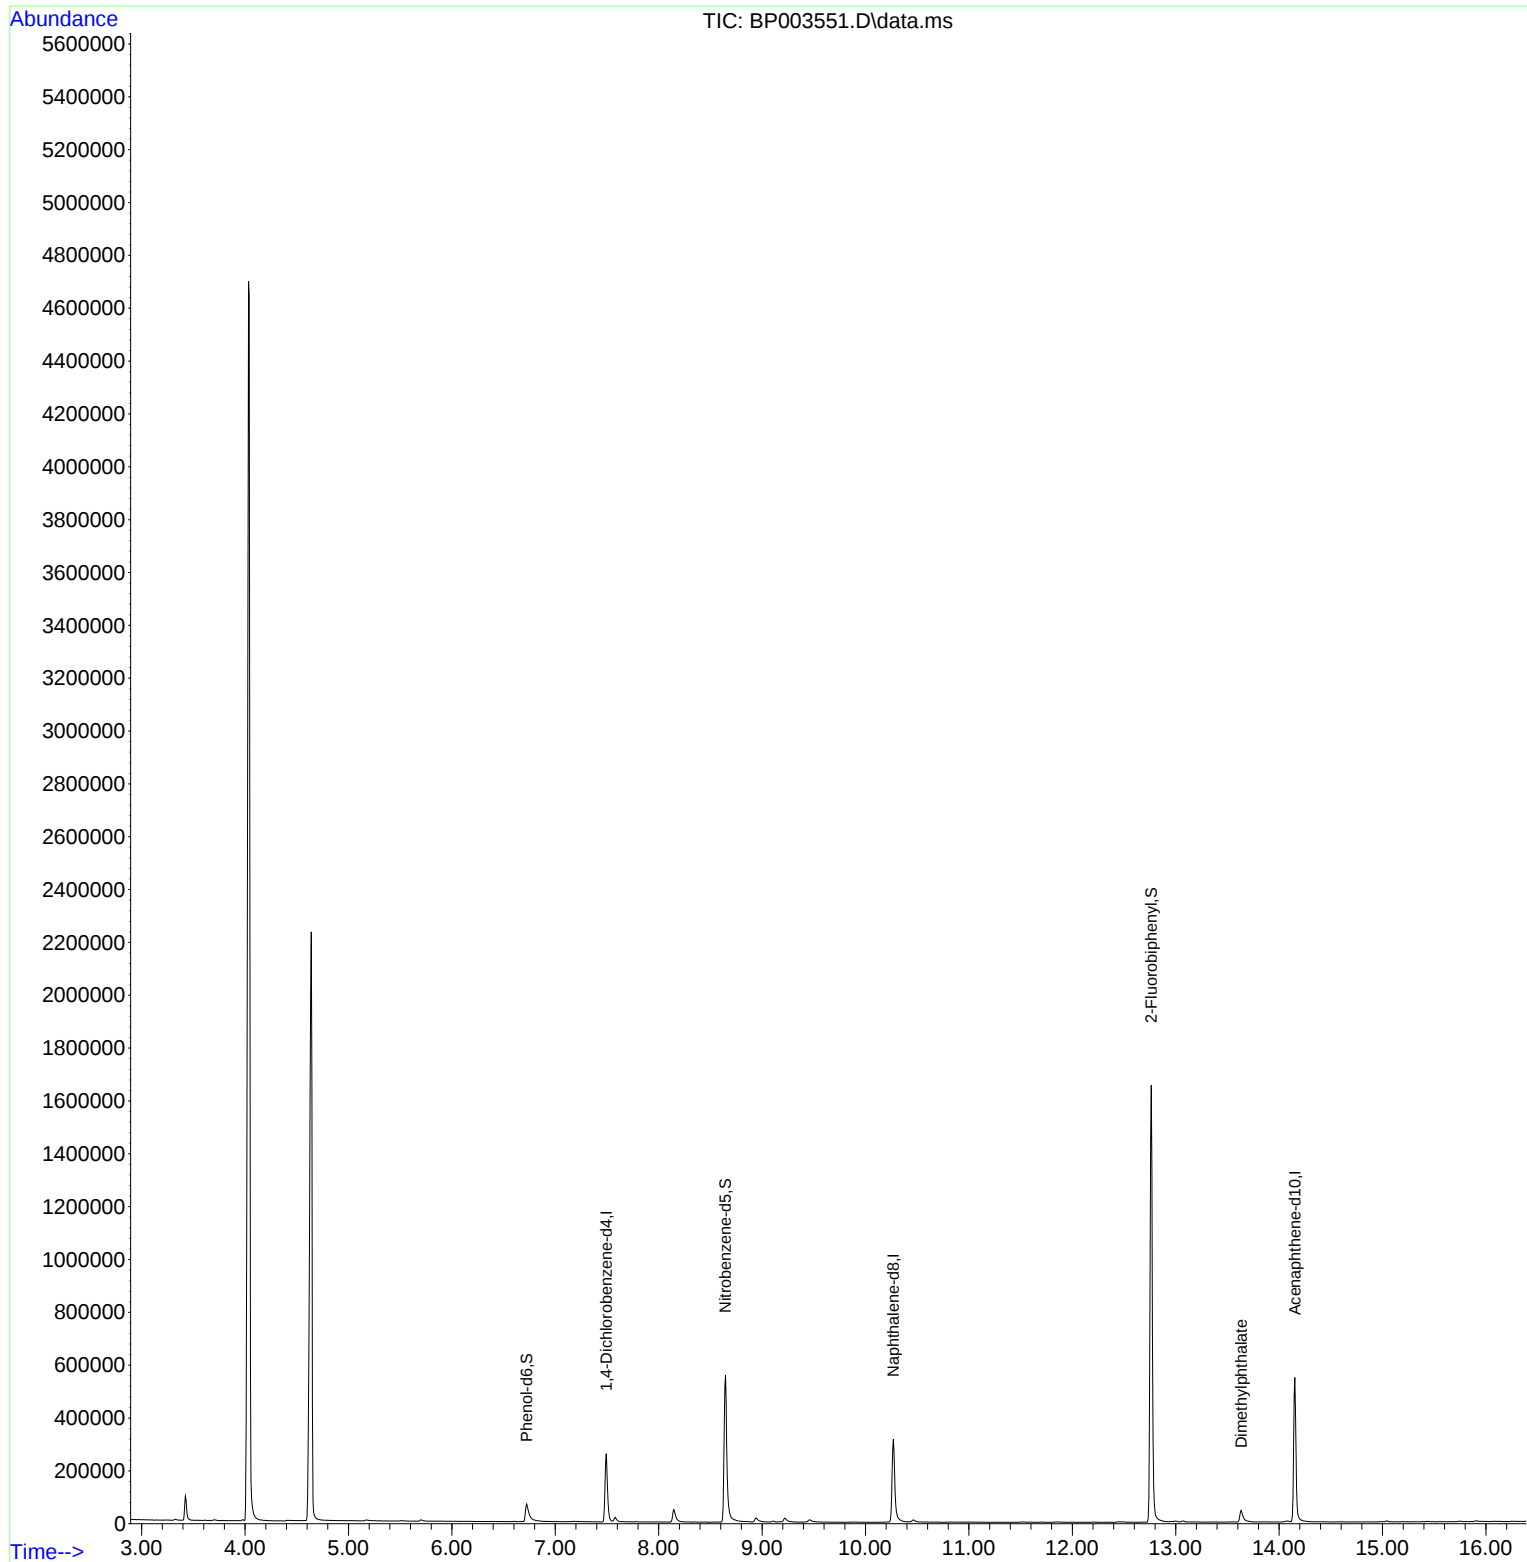

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003551.D
Acq On : 07 Oct 2020 10:41
Operator : CG/JU
Sample : L4271-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GV-CONCRETE

Quant Time: Oct 07 13:07:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

