

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003526.D
 Acq On : 06 Oct 2020 17:40
 Operator : CG/JU
 Sample : L4272-31
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-4-(6.5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	403	rBV	964747	1624246	37.73%	7.926%
2	6.699	642	648	681	rBV	895270	1665765	38.70%	8.128%
3	7.493	776	783	794	rBV	259908	423420	9.84%	2.066%
4	8.646	971	979	1004	rBV	606458	1140565	26.50%	5.565%
5	10.269	1248	1255	1275	rBV	305431	586378	13.62%	2.861%
6	12.763	1671	1679	1693	rBV	1696238	2602637	60.46%	12.700%
7	13.622	1818	1825	1843	rBV	182843	314720	7.31%	1.536%
8	14.151	1908	1915	1935	rVB	550986	815712	18.95%	3.980%
9	15.657	2164	2171	2192	rBV	1241748	1974514	45.87%	9.635%
10	16.910	2378	2384	2400	rBV	648366	1005118	23.35%	4.905%
11	19.492	2818	2823	2836	rBV2	3191510	4304674	100.00%	21.005%
12	20.745	3031	3036	3045	rBV	415508	588456	13.67%	2.871%
13	21.022	3077	3083	3095	rBV	1005895	1424225	33.09%	6.950%
14	21.610	3178	3183	3191	rBV6	29094	75607	1.76%	0.369%
15	22.533	3336	3340	3345	rBV2	41336	64695	1.50%	0.316%
16	23.080	3430	3433	3440	rVB3	39681	59640	1.39%	0.291%
17	23.186	3445	3451	3467	rVB2	823414	1604593	37.28%	7.830%
18	23.704	3536	3539	3546	rVB3	43955	71968	1.67%	0.351%
19	23.786	3549	3553	3564	rVB2	60825	146664	3.41%	0.716%




Sum of corrected areas: 20493597

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003526.D
Acq On : 06 Oct 2020 17:40
Operator : CG/JU
Sample : L4272-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-4-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

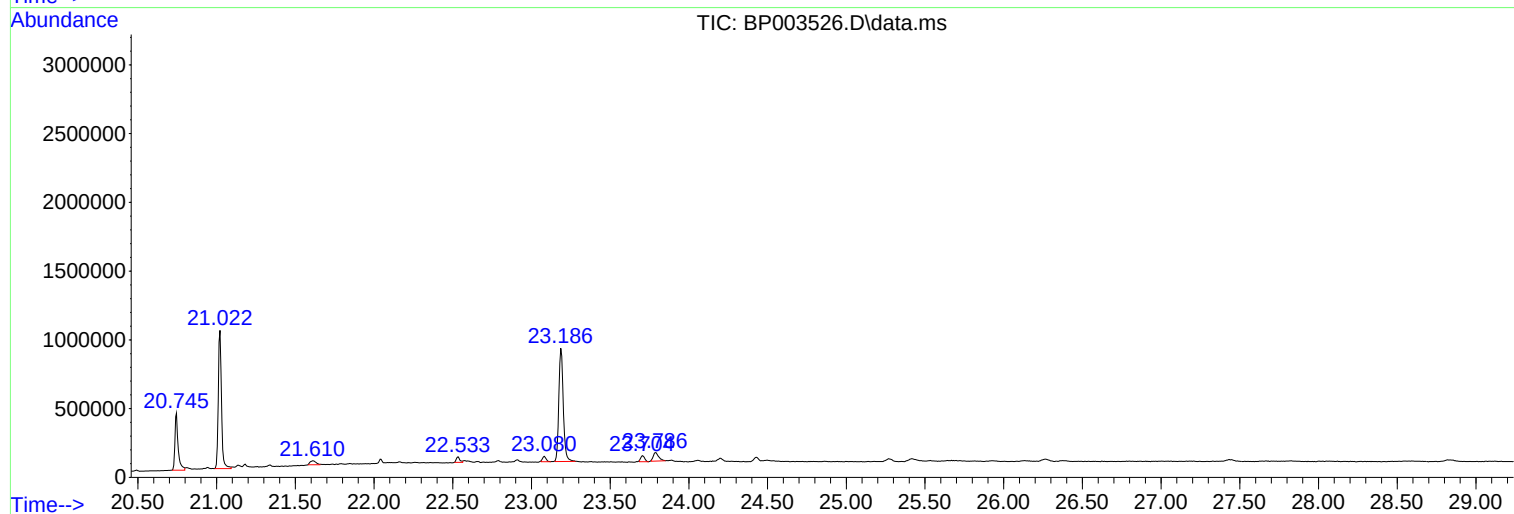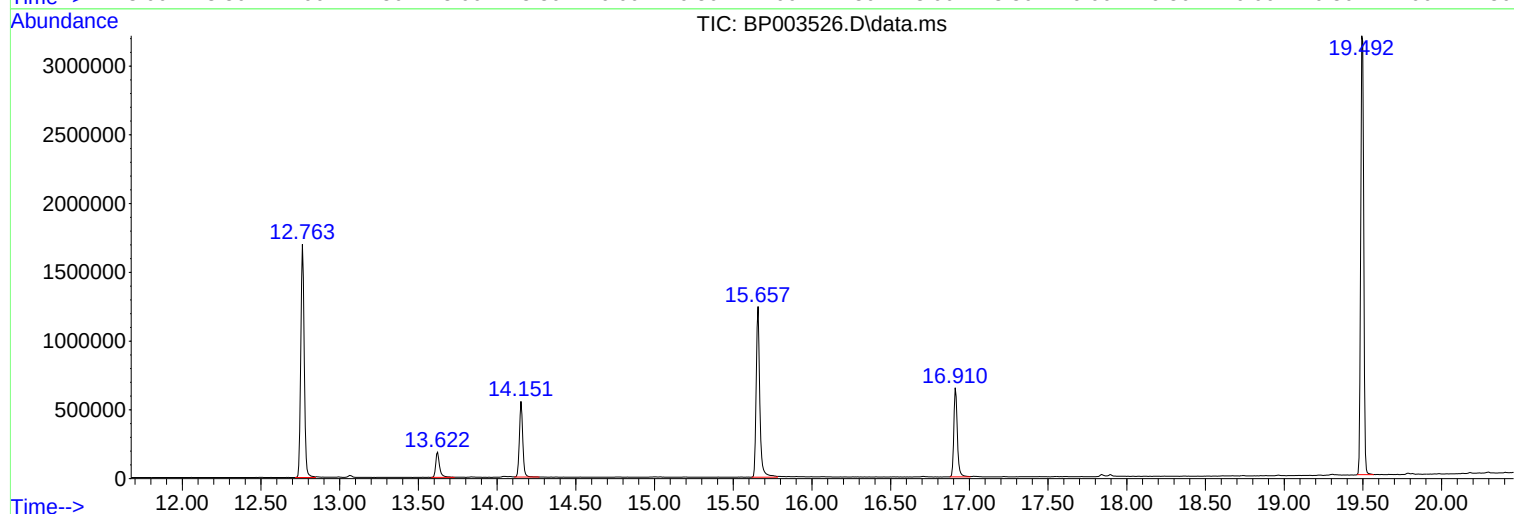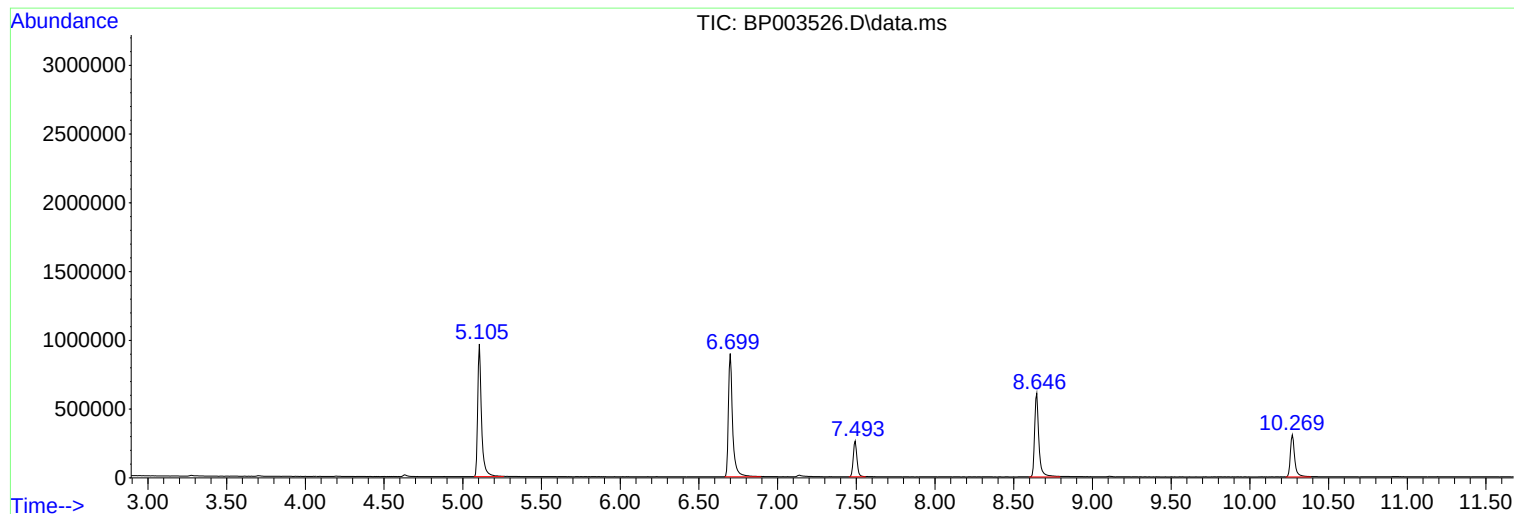

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003526.D
Acq On : 06 Oct 2020 17:40
Operator : CG/JU
Sample : L4272-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-4-(6.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Nonadecanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.745	8.26 ng	588456	Chrysene-d12	21.022

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		n-Nonadecanol-1	284	C19H40O	001454-84-8	94
2		Behenic alcohol	326	C22H46O	000661-19-8	94
3		5-Octadecene, (E)-	252	C18H36	007206-21-5	93
4		Cyclopentadecane	210	C15H30	000295-48-7	93
5		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91

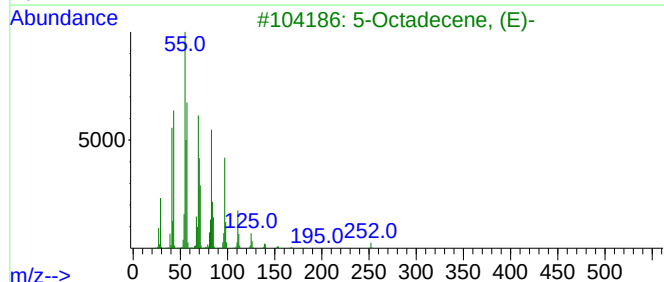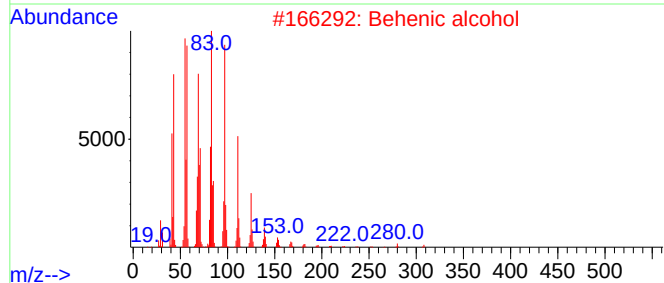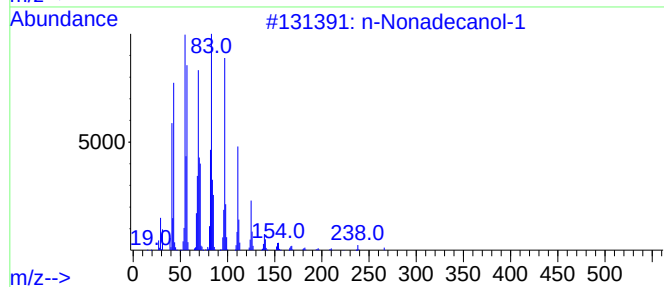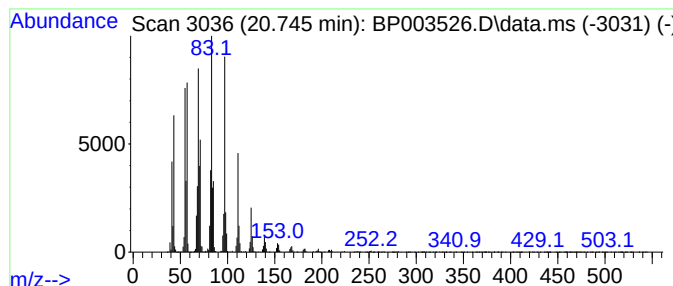

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003526.D
Acq On : 06 Oct 2020 17:40
Operator : CG/JU
Sample : L4272-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-4-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Nonadecanol-1	20.745	8.3	ng	588456	5	21.022	1424230	20.0