

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003530.D
 Acq On : 06 Oct 2020 19:56
 Operator : CG/JU
 Sample : L4272-43
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-8-(6.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	403	rBV	1095178	1837198	35.56%	8.439%
2	6.699	641	648	679	rBV	1059320	1930496	37.36%	8.868%
3	7.493	776	783	796	rBV	234761	386704	7.48%	1.776%
4	8.646	971	979	1011	rBV	710318	1324152	25.63%	6.083%
5	10.269	1248	1255	1274	rBV	265255	531717	10.29%	2.442%
6	12.763	1672	1679	1699	rBV	1974413	3059095	59.20%	14.052%
7	13.622	1819	1825	1845	rBV	182130	319948	6.19%	1.470%
8	14.151	1909	1915	1932	rVB	482962	739429	14.31%	3.397%
9	15.657	2164	2171	2194	rBV	1357053	2292322	44.36%	10.530%
10	16.910	2378	2384	2400	rBV	568756	923831	17.88%	4.244%
11	19.498	2818	2824	2839	rBV	4044568	5167112	100.00%	23.736%
12	20.745	3031	3036	3046	rBV	224656	355351	6.88%	1.632%
13	21.021	3078	3083	3096	rBV	948961	1340784	25.95%	6.159%
14	23.186	3444	3451	3467	rBV2	787599	1561394	30.22%	7.172%




Sum of corrected areas: 21769533

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003530.D
Acq On : 06 Oct 2020 19:56
Operator : CG/JU
Sample : L4272-43
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-8-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

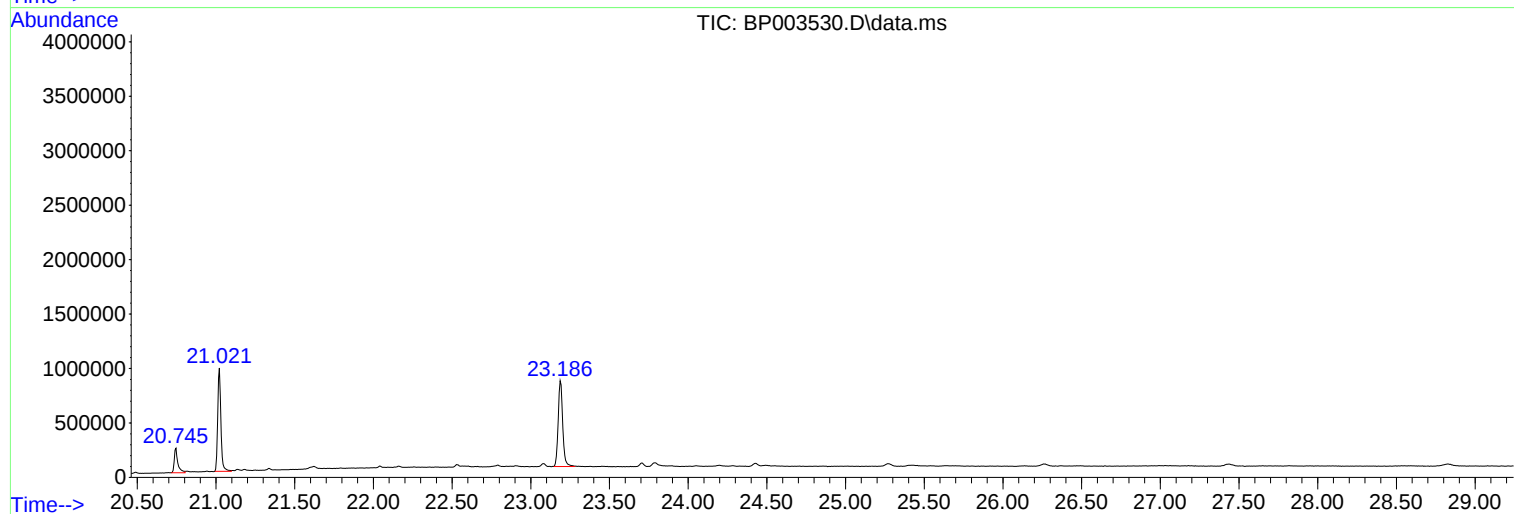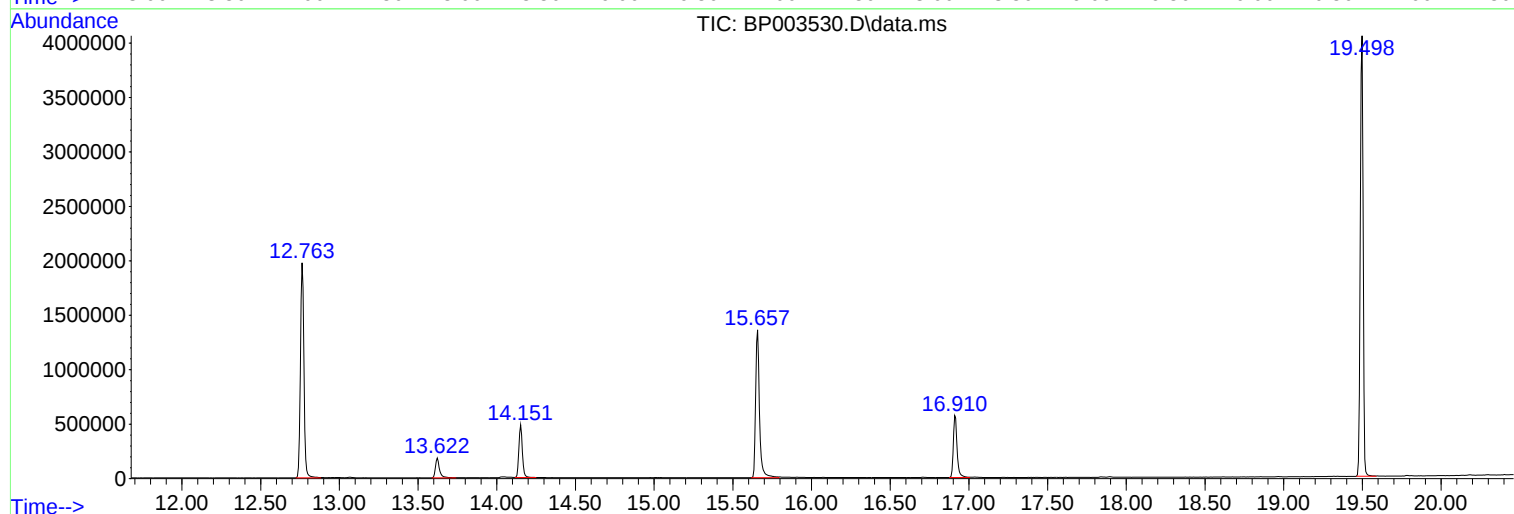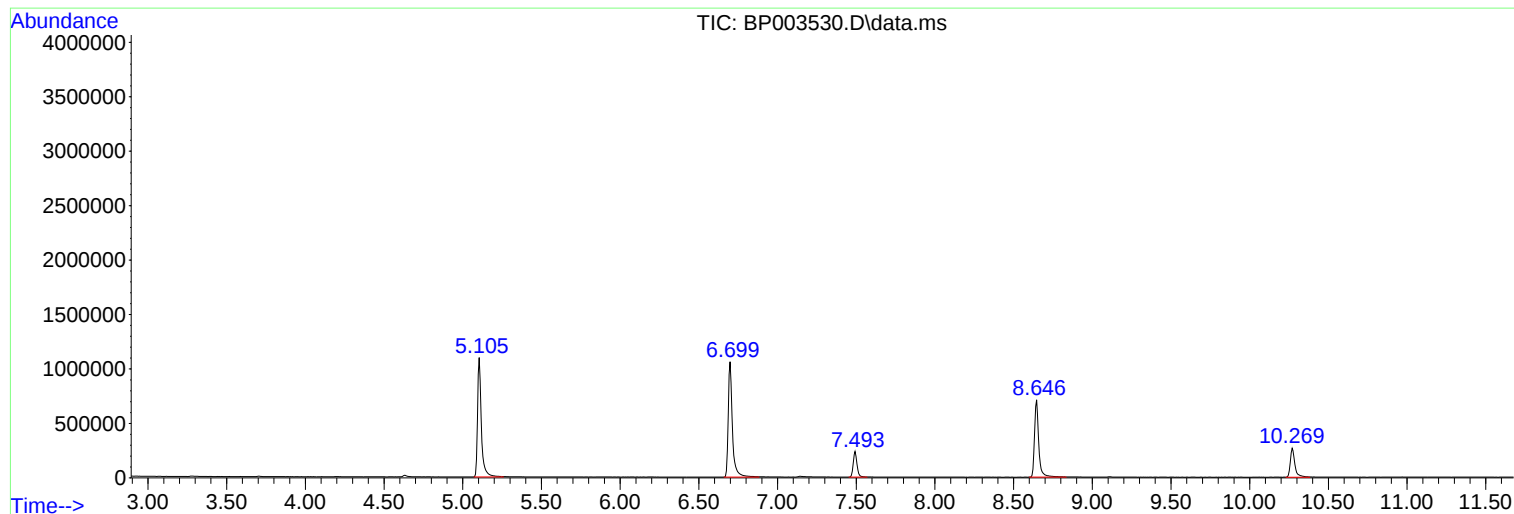

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003530.D
Acq On : 06 Oct 2020 19:56
Operator : CG/JU
Sample : L4272-43
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-8-(6.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.745	5.30 ng	355351	Chrysene-d12	21.021

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenic alcohol	326	C22H46O	000661-19-8	95
2			Cyclopentadecane	210	C15H30	000295-48-7	93
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	93
4			n-Tetracosanol-1	354	C24H50O	000506-51-4	92
5			3-Eicosene, (E)-	280	C20H40	074685-33-9	91

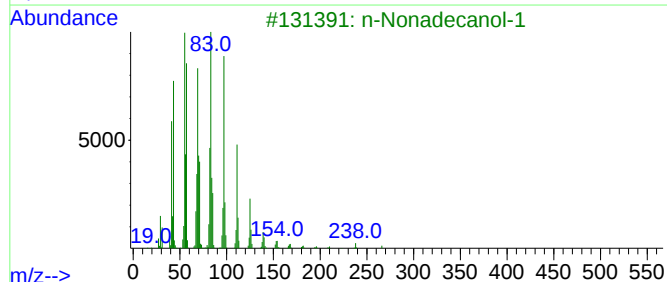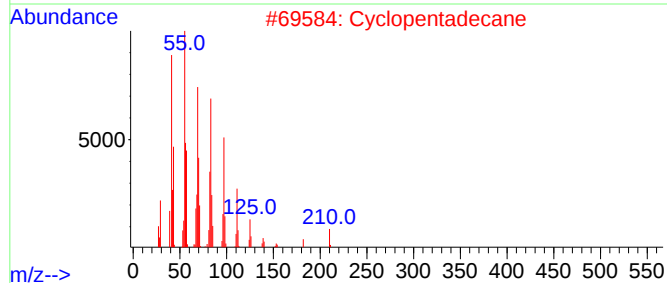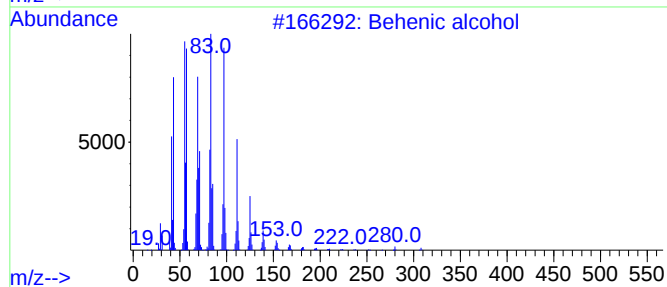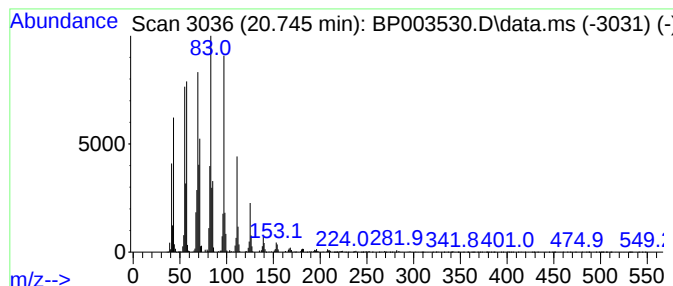

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003530.D
Acq On : 06 Oct 2020 19:56
Operator : CG/JU
Sample : L4272-43
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-8-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	20.745	5.3	ng	355351	5	21.021	1340780	20.0