

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003532.D
 Acq On : 06 Oct 2020 21:04
 Operator : CG/JU
 Sample : L4272-55
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-12-(3.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	408	rBV	1256947	2115548	38.81%	8.659%
2	6.699	641	648	678	rBV	1228996	2198532	40.33%	8.999%
3	7.493	774	783	795	rBV	267143	446742	8.19%	1.829%
4	8.646	971	979	1008	rBV	828869	1525810	27.99%	6.245%
5	10.269	1247	1255	1276	rBV	316858	612786	11.24%	2.508%
6	12.763	1672	1679	1701	rBV	2269831	3444238	63.18%	14.097%
7	13.622	1818	1825	1844	rBV	221577	389987	7.15%	1.596%
8	14.151	1909	1915	1934	rVB	565827	855735	15.70%	3.503%
9	15.651	2164	2170	2199	rBV	1559068	2597764	47.65%	10.633%
10	16.910	2378	2384	2400	rBV	655091	1052509	19.31%	4.308%
11	19.492	2818	2823	2837	rBV	4063831	5451573	100.00%	22.313%
12	20.739	3031	3035	3053	rBV	336829	511163	9.38%	2.092%
13	21.016	3077	3082	3097	rBV	1076944	1482828	27.20%	6.069%
14	23.180	3444	3450	3465	rVB	826690	1645224	30.18%	6.734%
15	23.780	3548	3552	3562	rVB4	44563	101637	1.86%	0.416%




Sum of corrected areas: 24432076

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003532.D
Acq On : 06 Oct 2020 21:04
Operator : CG/JU
Sample : L4272-55
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-12-(3.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

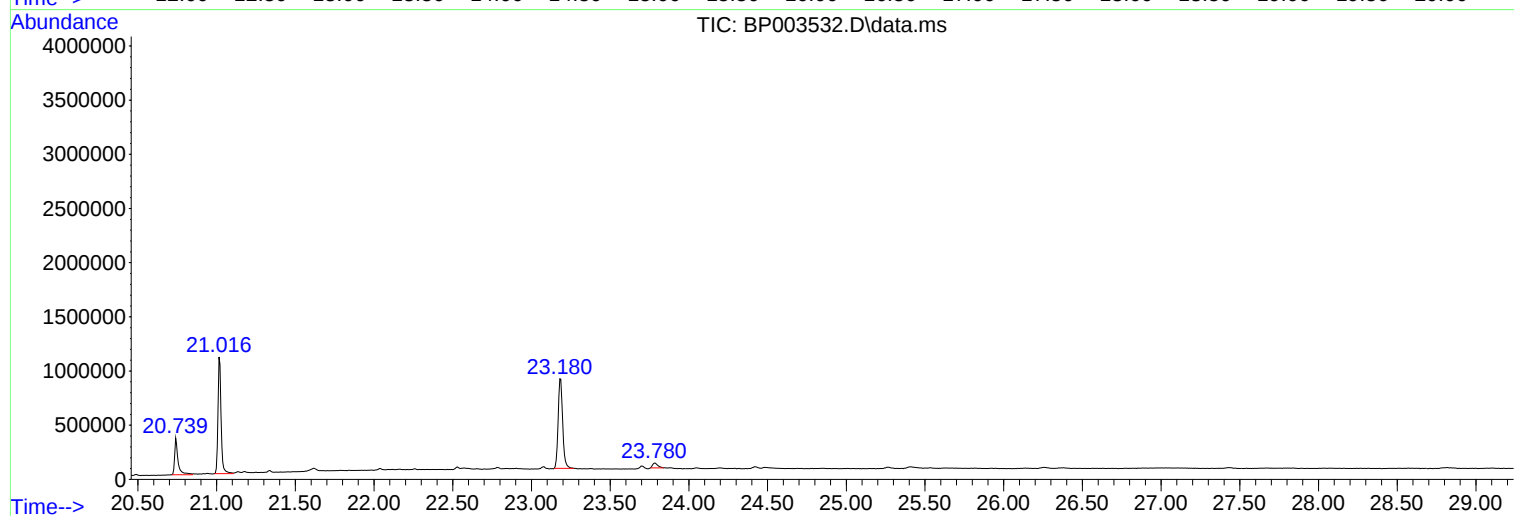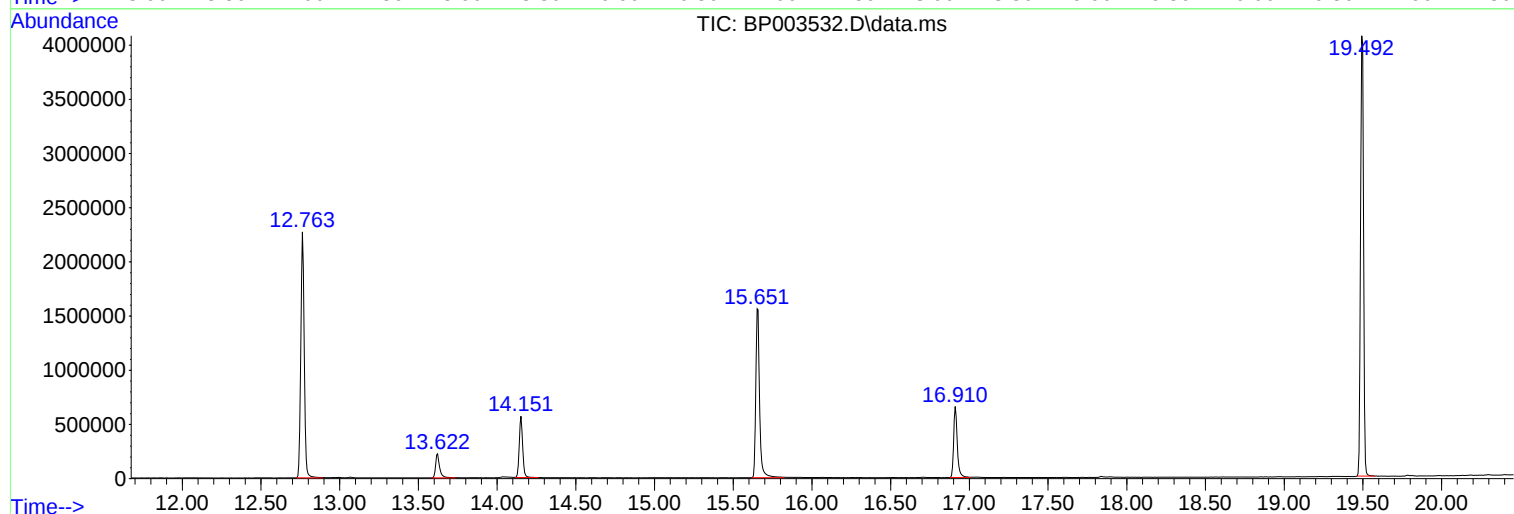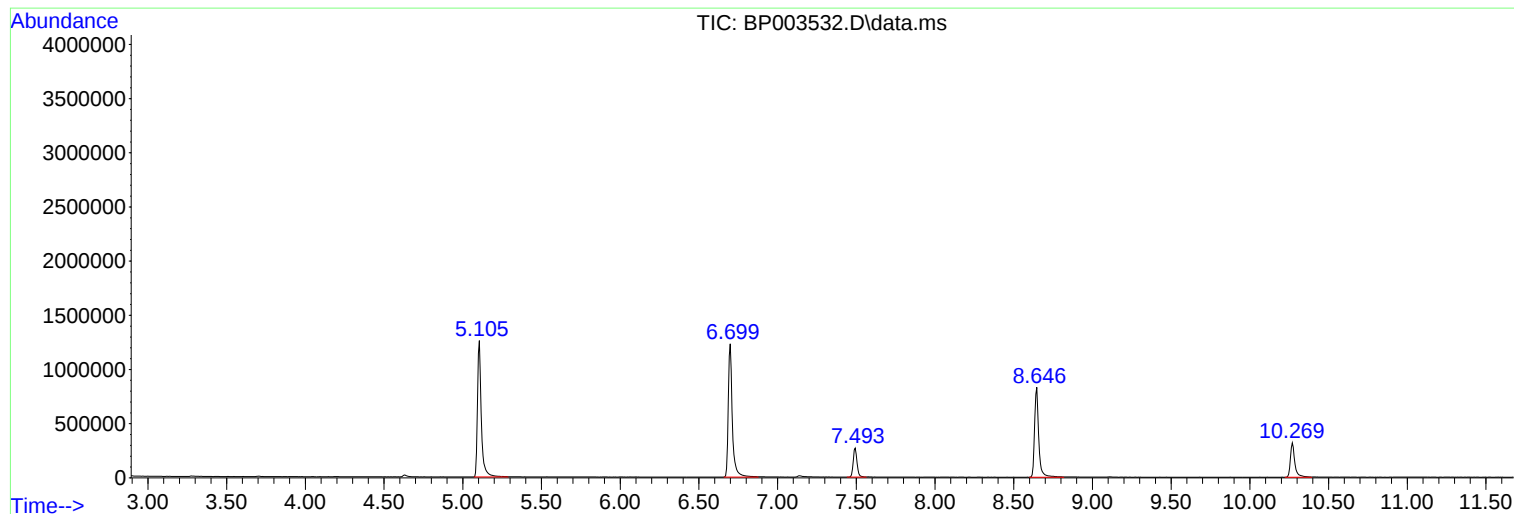

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003532.D
Acq On : 06 Oct 2020 21:04
Operator : CG/JU
Sample : L4272-55
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-12-(3.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 9-Eicosene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.739	6.89 ng	511163	Chrysene-d12	21.016

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		9-Eicosene, (E)-	280	C20H40	074685-29-3	94
2		n-Nonadecanol-1	284	C19H40O	001454-84-8	94
3		Behenic alcohol	326	C22H46O	000661-19-8	94
4		Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	93
5		3-Eicosene, (E)-	280	C20H40	074685-33-9	91

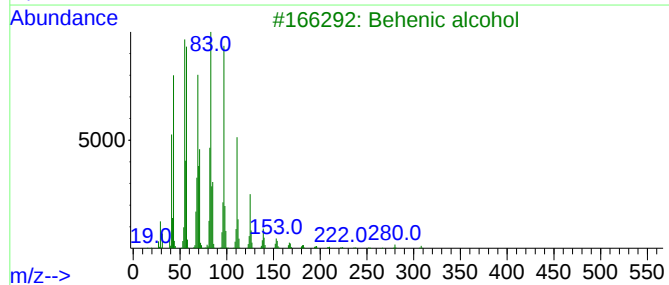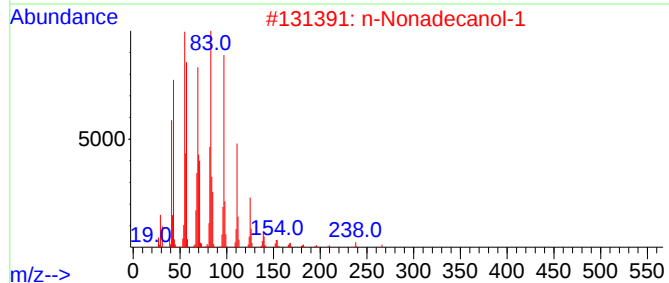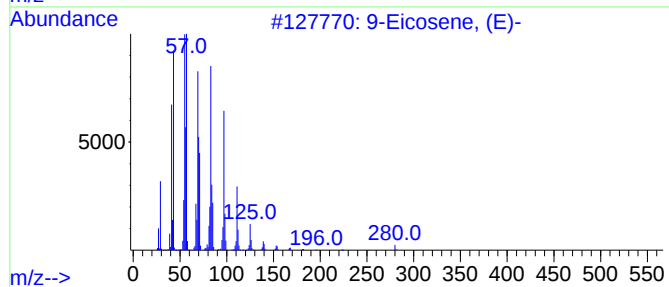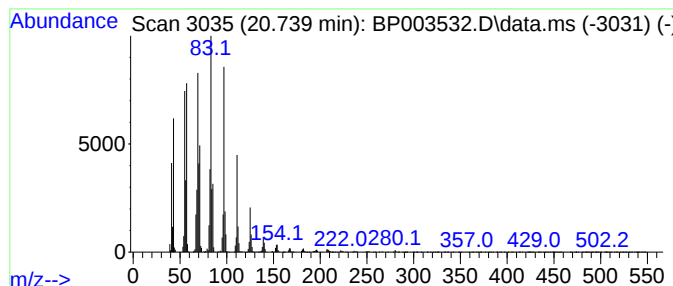

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003532.D
Acq On : 06 Oct 2020 21:04
Operator : CG/JU
Sample : L4272-55
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-12-(3.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
9-Eicosene, (E)-	20.739	6.9	ng	511163	5	21.016	1482830	20.0