

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003534.D
 Acq On : 06 Oct 2020 22:12
 Operator : CG/JU
 Sample : L4272-28
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-3-(6.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	402	rBV	1034343	1765533	38.69%	8.237%
2	6.699	641	648	679	rBV	984539	1836526	40.24%	8.568%
3	7.493	777	783	795	rBV	264772	442939	9.71%	2.066%
4	8.646	971	979	1010	rBV	667421	1255775	27.52%	5.859%
5	10.269	1248	1255	1276	rBV	309031	607892	13.32%	2.836%
6	12.763	1672	1679	1699	rBV	1789356	2833207	62.08%	13.218%
7	13.622	1818	1825	1844	rBV	204499	355974	7.80%	1.661%
8	14.151	1908	1915	1931	rVB	561073	836578	18.33%	3.903%
9	15.657	2164	2171	2193	rBV	1269357	2130353	46.68%	9.939%
10	16.910	2378	2384	2394	rBV	642580	1031901	22.61%	4.814%
11	19.492	2818	2823	2838	rVB	3446620	4563529	100.00%	21.291%
12	20.739	3031	3035	3045	rBV	372331	545149	11.95%	2.543%
13	21.016	3077	3082	3097	rBV	1063427	1469403	32.20%	6.855%
14	23.186	3444	3451	3463	rVB2	817242	1607476	35.22%	7.499%
15	23.780	3547	3552	3565	rBV2	59562	152255	3.34%	0.710%




Sum of corrected areas: 21434490

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003534.D
Acq On : 06 Oct 2020 22:12
Operator : CG/JU
Sample : L4272-28
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-3-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

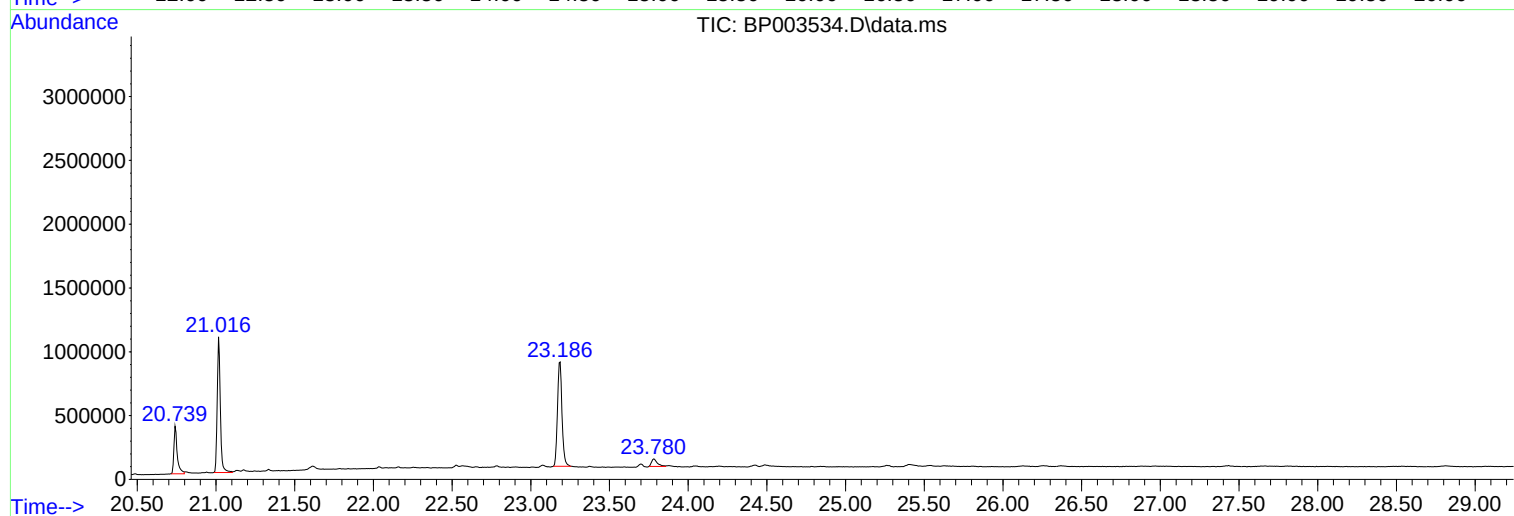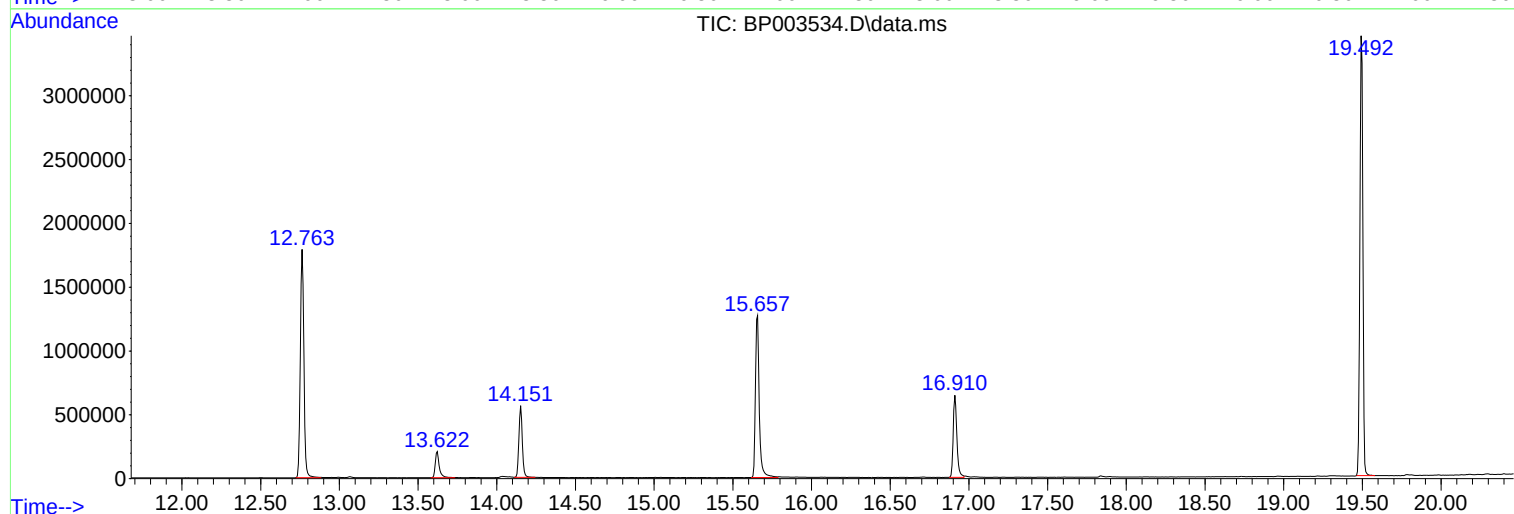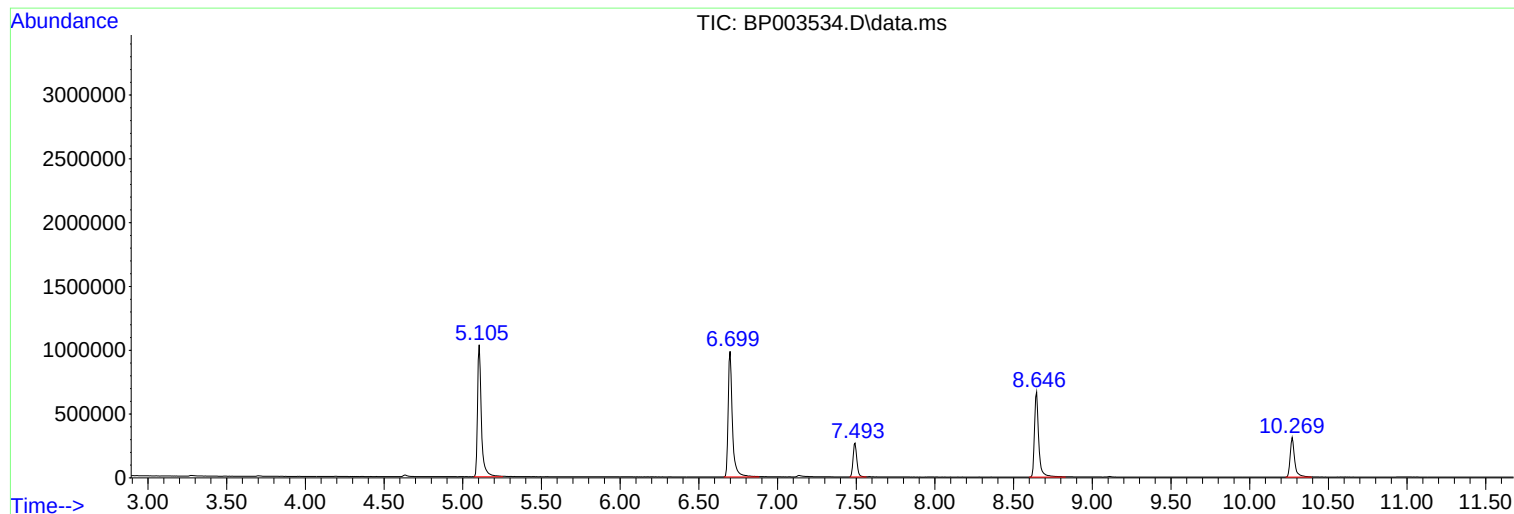

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003534.D
Acq On : 06 Oct 2020 22:12
Operator : CG/JU
Sample : L4272-28
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-3-(6.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclohexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.739	7.42 ng	545149	Chrysene-d12	21.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexadecane	224	C16H32	000295-65-8	94
2			Behenic alcohol	326	C22H46O	000661-19-8	94
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	94
4			1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
5			Cyclopentadecane	210	C15H30	000295-48-7	93

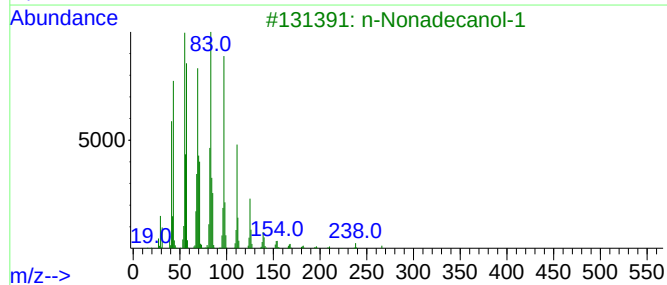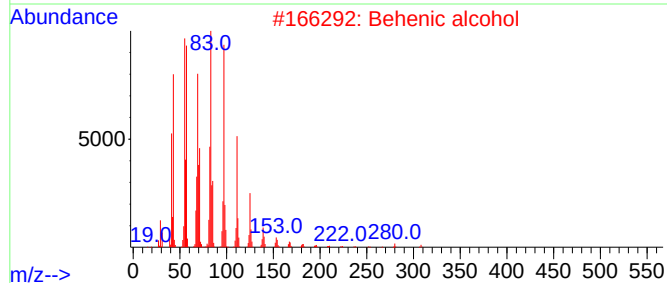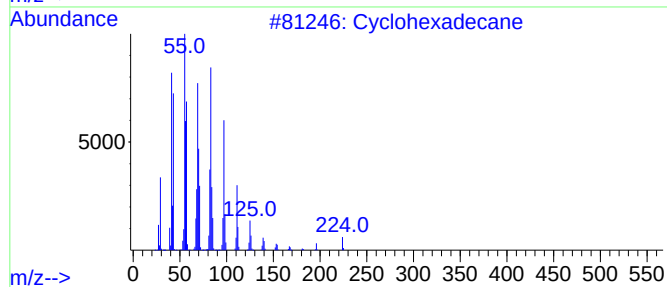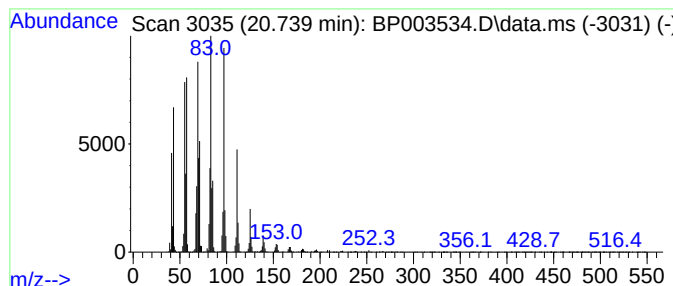

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003534.D
Acq On : 06 Oct 2020 22:12
Operator : CG/JU
Sample : L4272-28
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-3-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclohexadecane	20.739	7.4	ng	545149	5	21.016	1469400	20.0