

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003536.D
 Acq On : 06 Oct 2020 23:20
 Operator : CG/JU
 Sample : L4272-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-1-(6.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	402	rBV	779261	1359112	37.40%	7.125%
2	6.699	642	648	676	rBV	732815	1408025	38.75%	7.382%
3	7.493	776	783	793	rBV	275894	456658	12.57%	2.394%
4	8.646	970	979	1003	rBV	496380	960468	26.43%	5.035%
5	10.269	1247	1255	1280	rBV	329403	643510	17.71%	3.374%
6	12.763	1672	1679	1701	rBV	1445130	2259459	62.18%	11.845%
7	13.063	1724	1730	1740	rBV	41069	68505	1.89%	0.359%
8	13.622	1819	1825	1850	rVB	160272	271991	7.49%	1.426%
9	14.151	1908	1915	1926	rBV	577792	886532	24.40%	4.648%
10	15.657	2164	2171	2191	rBV	966151	1650898	45.43%	8.655%
11	16.910	2378	2384	2394	rBV	711219	1120374	30.83%	5.874%
12	19.492	2818	2823	2836	rBV	2940972	3633667	100.00%	19.049%
13	20.739	3031	3035	3046	rBV	272751	428566	11.79%	2.247%
14	21.016	3077	3082	3094	rBV	1156231	1598753	44.00%	8.381%
15	22.257	3289	3293	3298	rVB3	55848	74439	2.05%	0.390%
16	22.527	3335	3339	3342	rBV	49380	75854	2.09%	0.398%
17	22.568	3343	3346	3357	rVB3	64593	137552	3.79%	0.721%
18	23.180	3443	3450	3471	rVB2	920835	1795159	49.40%	9.411%
19	23.698	3534	3538	3544	rVB2	65377	118899	3.27%	0.623%
20	23.780	3548	3552	3564	rVB2	53452	126533	3.48%	0.663%




Sum of corrected areas: 19074954

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003536.D
Acq On : 06 Oct 2020 23:20
Operator : CG/JU
Sample : L4272-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-1-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

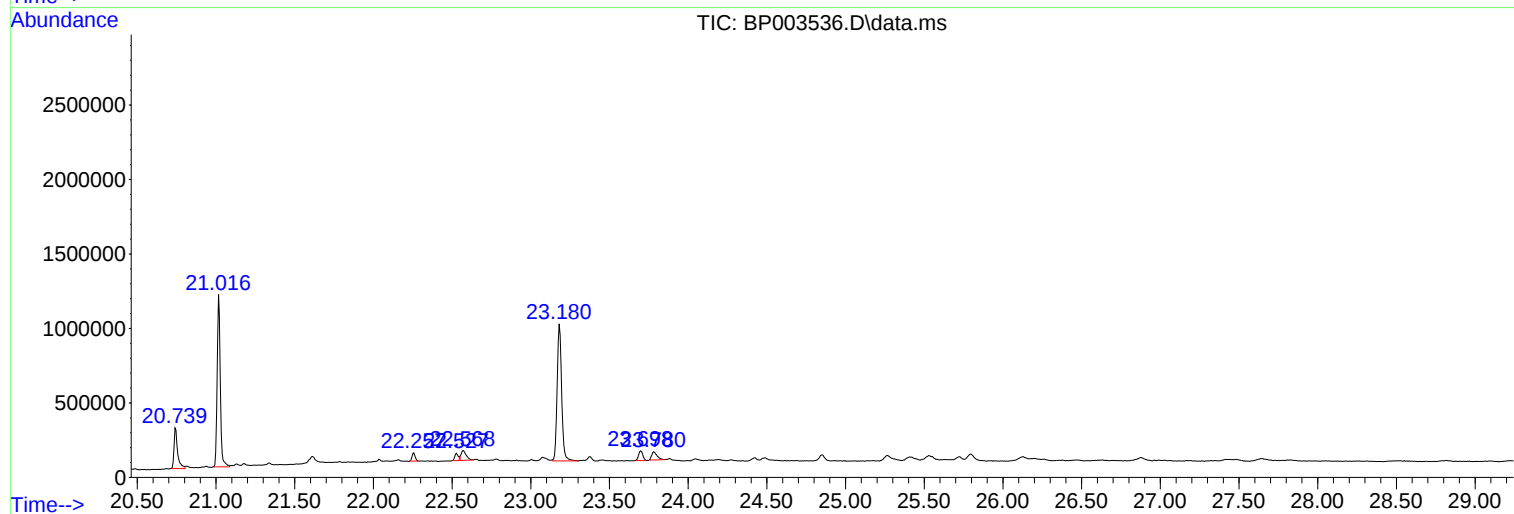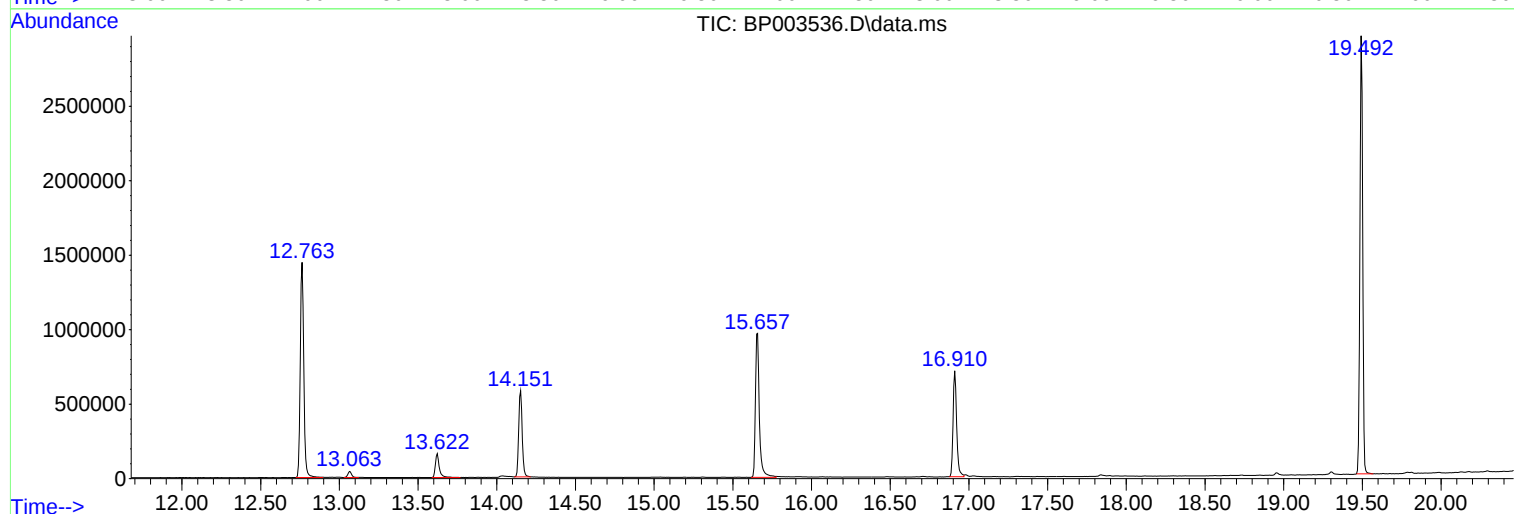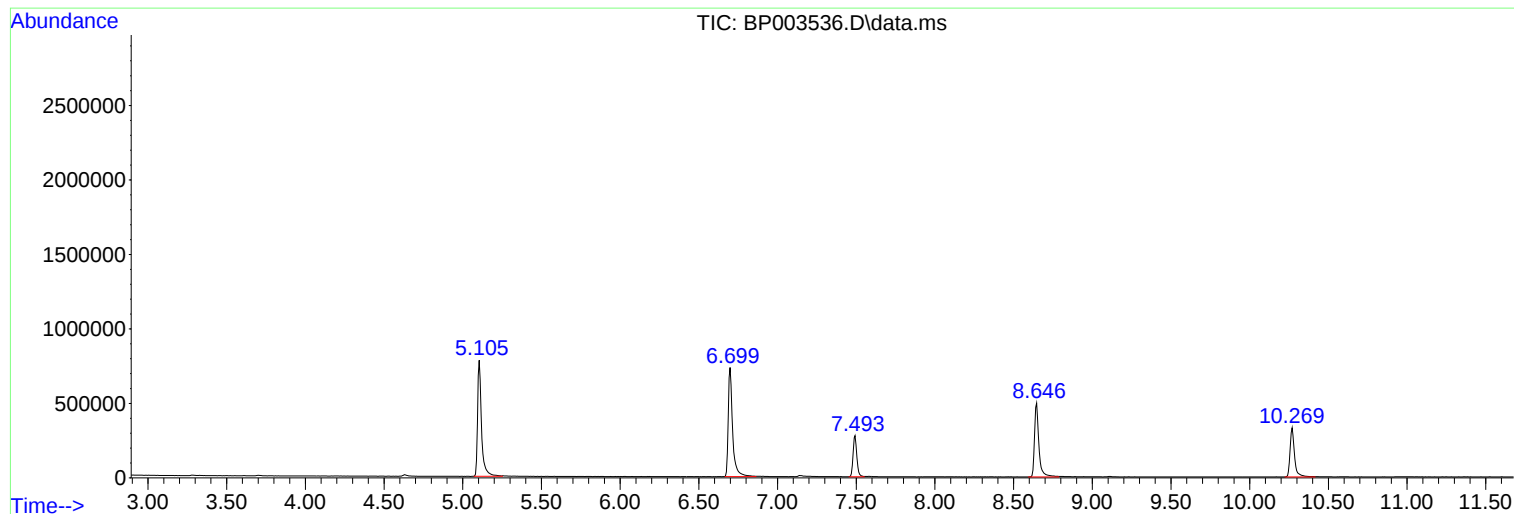

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003536.D
Acq On : 06 Oct 2020 23:20
Operator : CG/JU
Sample : L4272-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-1-(6.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.739	5.36 ng	428566	Chrysene-d12	21.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Behenic alcohol	326	C22H46O	000661-19-8	94
2			n-Nonadecanol-1	284	C19H40O	001454-84-8	93
3			1-Heneicosanol	312	C21H44O	015594-90-8	91
4			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91
5			3-Eicosene, (E)-	280	C20H40	074685-33-9	91

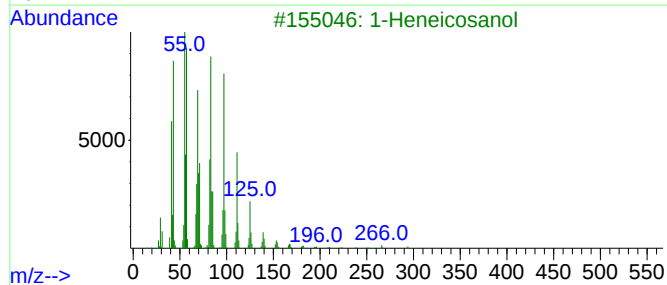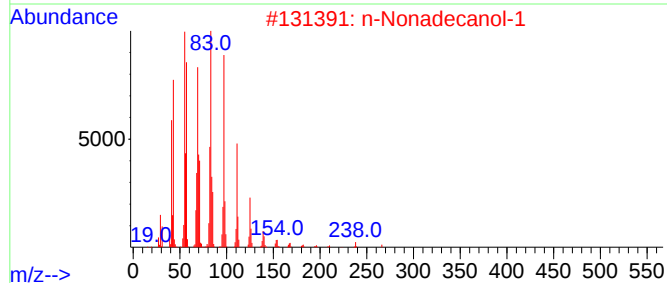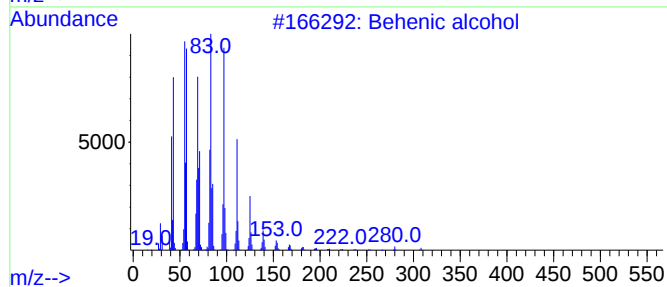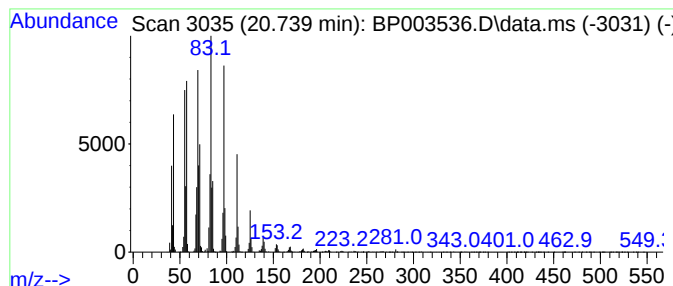

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003536.D
Acq On : 06 Oct 2020 23:20
Operator : CG/JU
Sample : L4272-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-1-(6.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	20.739	5.4	ng	428566	5	21.016	1598750	20.0