

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003538.D
 Acq On : 07 Oct 2020 00:28
 Operator : CG/JU
 Sample : L4272-49
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SC-10-(3.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.105	371	377	399	rBV	878410	1494073	36.19%	7.496%
2	6.699	642	648	677	rBV	841540	1580176	38.27%	7.928%
3	7.493	776	783	795	rBV	268109	454313	11.00%	2.279%
4	8.646	971	979	1007	rBV	575067	1103117	26.72%	5.535%
5	10.269	1248	1255	1277	rBV	330746	637670	15.45%	3.199%
6	12.763	1672	1679	1697	rBV	1614512	2555254	61.89%	12.820%
7	13.622	1818	1825	1839	rBV	135146	243758	5.90%	1.223%
8	14.151	1908	1915	1936	rVB2	570960	902940	21.87%	4.530%
9	15.651	2164	2170	2193	rBV	1145255	1901728	46.06%	9.541%
10	16.910	2378	2384	2400	rBV	725427	1108700	26.85%	5.563%
11	19.492	2818	2823	2838	rVB	3271136	4128529	100.00%	20.714%
12	20.739	3031	3035	3045	rBV	300322	419972	10.17%	2.107%
13	21.016	3077	3082	3096	rBV	1241627	1555829	37.68%	7.806%
14	23.180	3443	3450	3466	rVB2	936477	1746152	42.29%	8.761%
15	23.780	3548	3552	3562	rVB3	44402	98941	2.40%	0.496%




Sum of corrected areas: 19931152

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003538.D
Acq On : 07 Oct 2020 00:28
Operator : CG/JU
Sample : L4272-49
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-10-(3.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

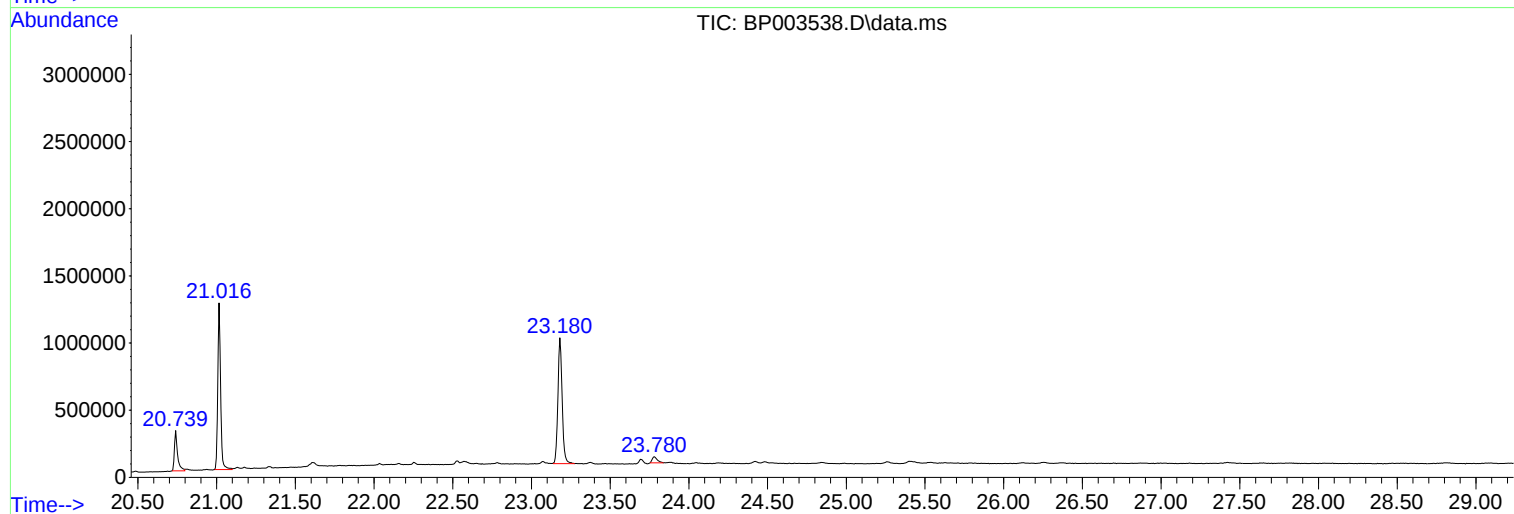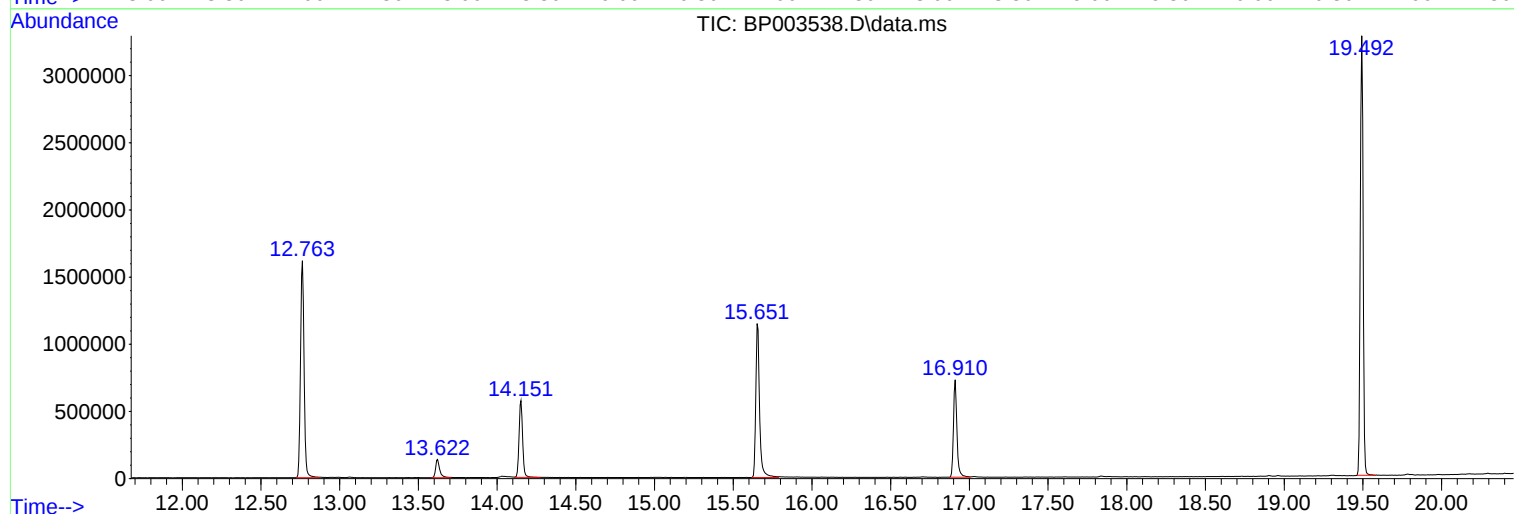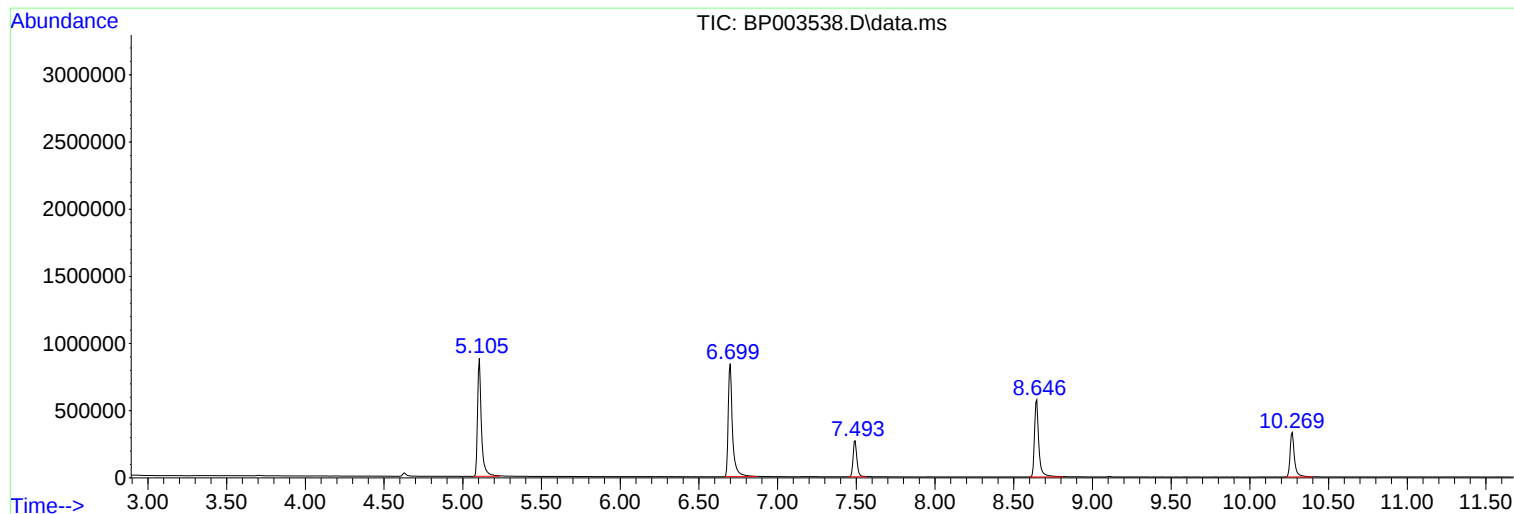

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003538.D
Acq On : 07 Oct 2020 00:28
Operator : CG/JU
Sample : L4272-49
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-10-(3.5)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 5-Octadecene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.739	5.40 ng	419972	Chrysene-d12	21.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Octadecene, (E)-	252	C18H36	007206-21-5	94
2			Behenic alcohol	326	C22H46O	000661-19-8	94
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	94
4			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	93
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91

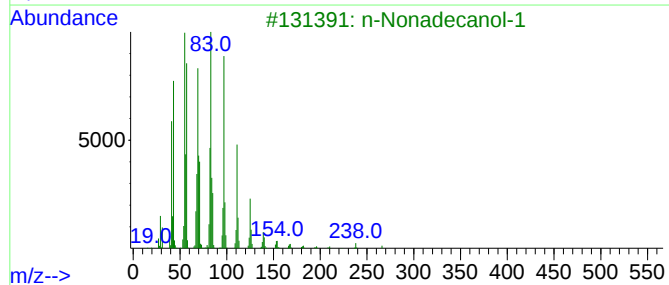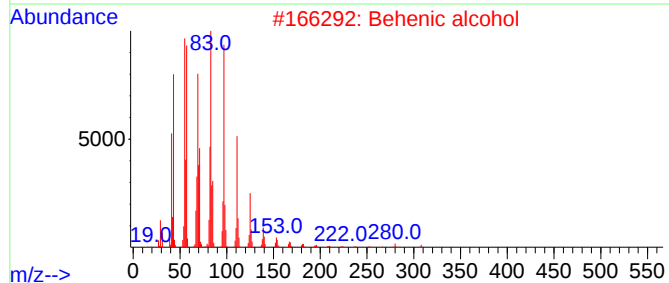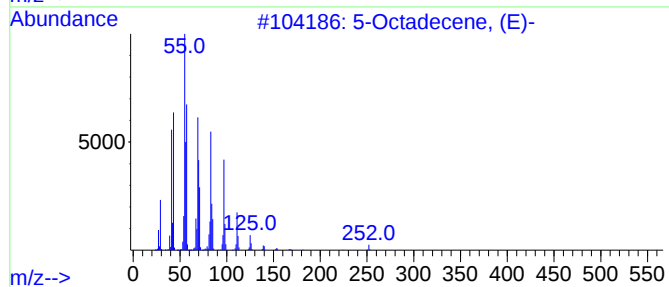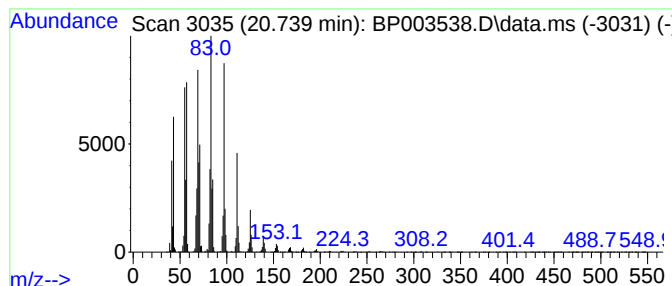

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
Data File : BP003538.D
Acq On : 07 Oct 2020 00:28
Operator : CG/JU
Sample : L4272-49
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SC-10-(3.5)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
5-Octadecene, (E)-	20.739	5.4	ng	419972	5	21.016	1555830	20.0