
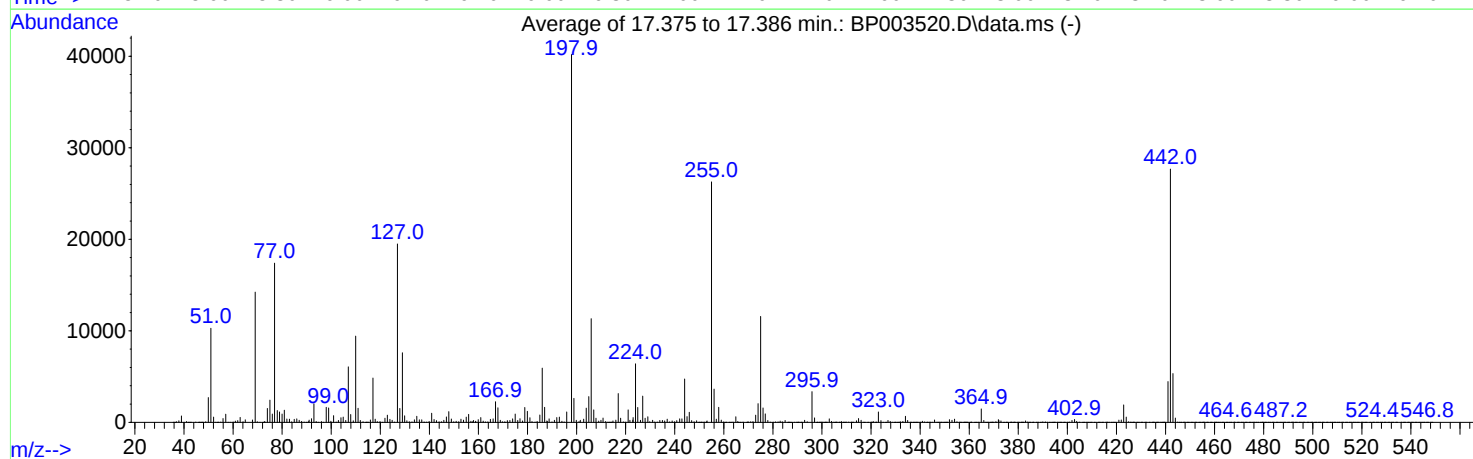


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003520.D
 Acq On : 06 Oct 2020 13:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 14:33:14 2020

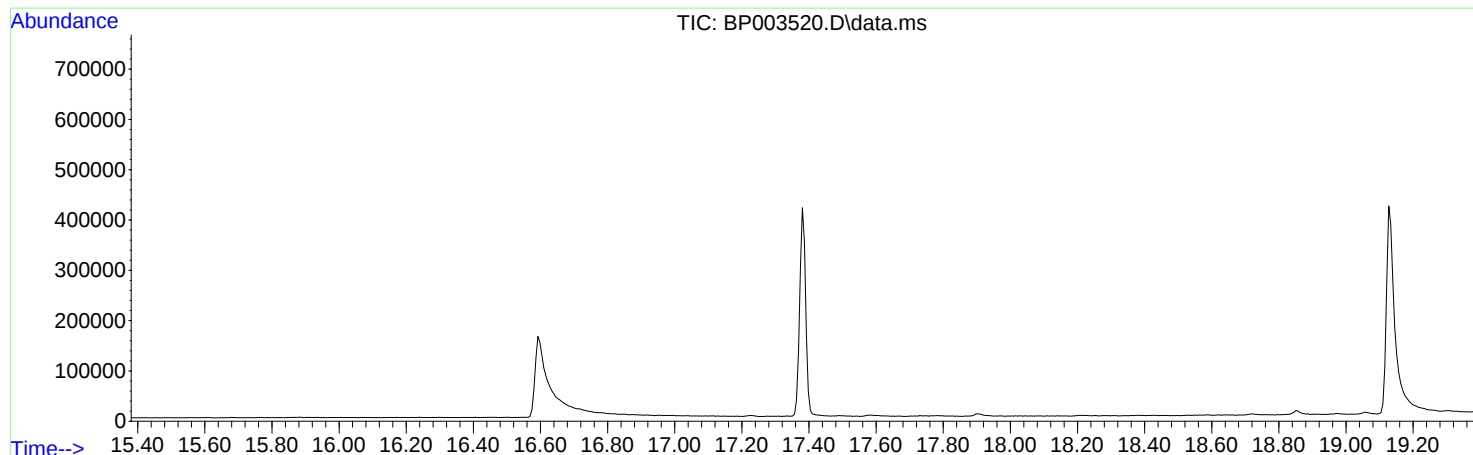

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	10277	PASS
68	69	0.00	2	1.9	265	PASS
69	198	0.00	100	35.4	14226	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	48.5	19491	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40194	PASS
199	198	5	9	6.5	2616	PASS
275	198	10	60	28.8	11583	PASS
365	198	1	100	3.6	1463	PASS
441	198	0.01	100	11.1	4465	PASS
442	198	50	100	68.9	27679	PASS
443	442	15	24	19.3	5339	PASS