
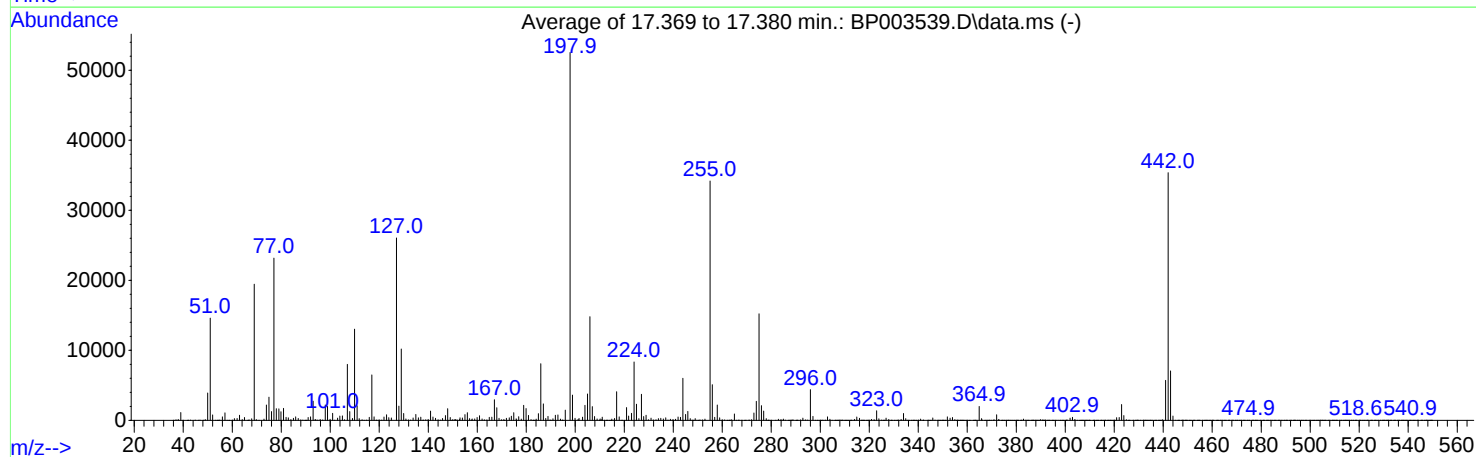


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100620\
 Data File : BP003539.D
 Acq On : 07 Oct 2020 03:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 14:33:14 2020

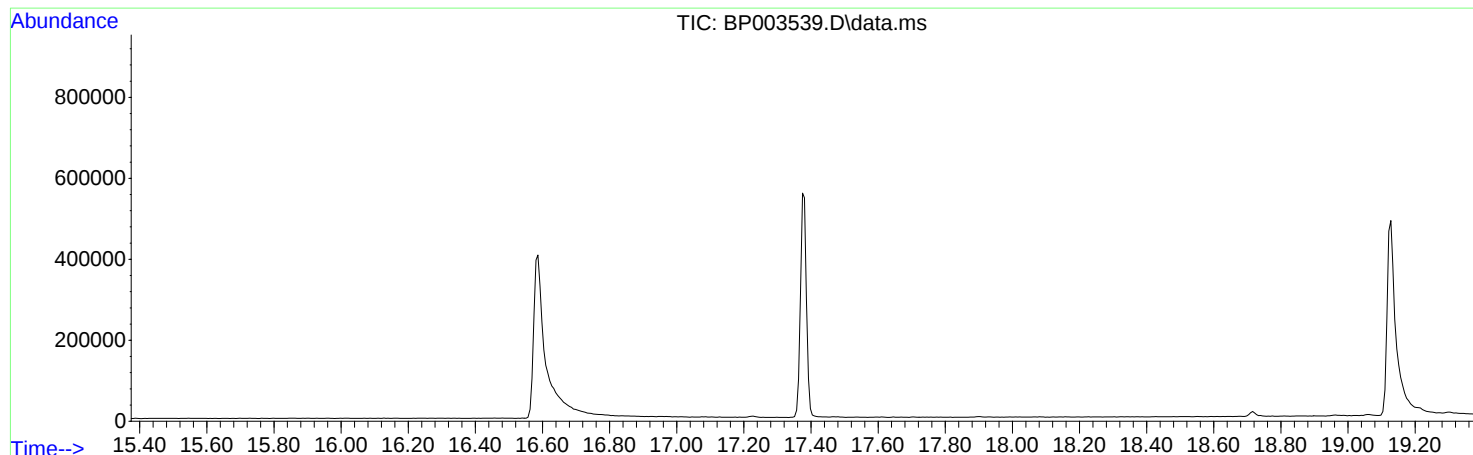

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	14598	PASS
68	69	0.00	2	1.2	240	PASS
69	198	0.00	100	37.0	19437	PASS
70	69	0.00	2	0.6	121	PASS
127	198	10	80	49.6	26043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52531	PASS
199	198	5	9	6.9	3615	PASS
275	198	10	60	29.0	15227	PASS
365	198	1	100	3.8	1999	PASS
441	198	0.01	100	10.9	5723	PASS
442	198	50	100	67.3	35360	PASS
443	442	15	24	19.9	7053	PASS