
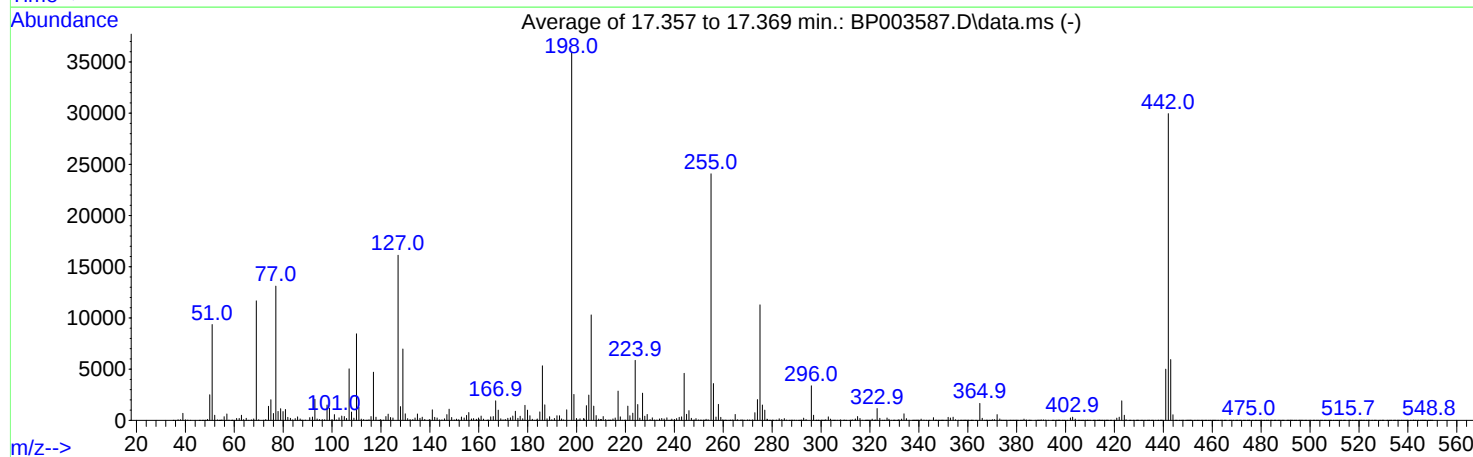


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100920\
 Data File : BP003587.D
 Acq On : 09 Oct 2020 10:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 08 15:55:58 2020

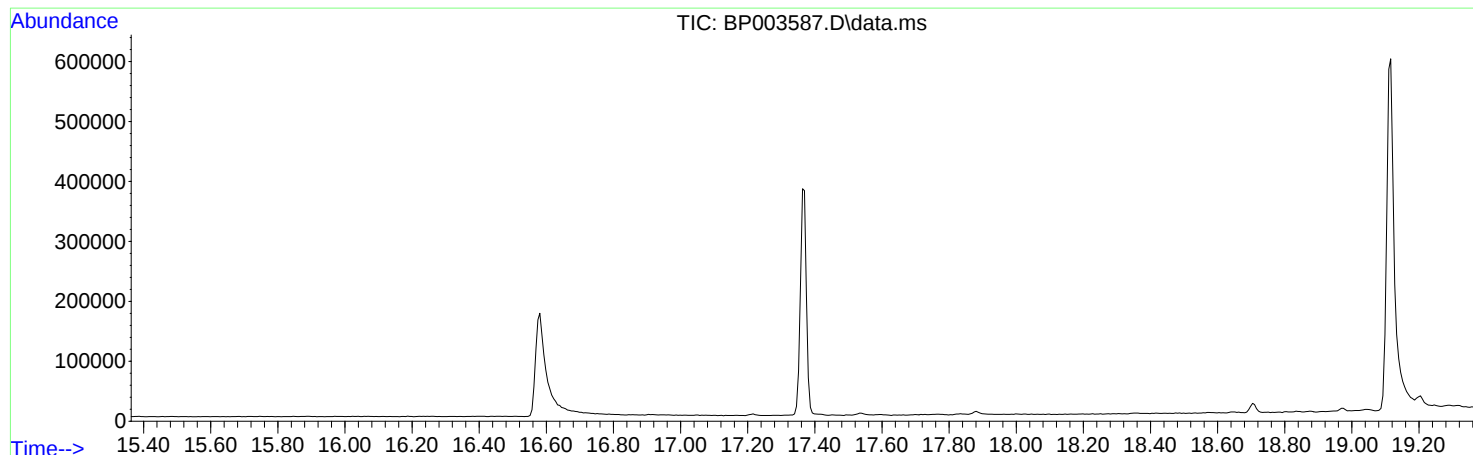

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	9359	PASS
68	69	0.00	2	1.2	135	PASS
69	198	0.00	100	32.5	11679	PASS
70	69	0.00	2	0.6	70	PASS
127	198	10	80	44.9	16123	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35928	PASS
199	198	5	9	7.1	2538	PASS
275	198	10	60	31.4	11282	PASS
365	198	1	100	4.6	1659	PASS
441	198	0.01	100	13.9	5001	PASS
442	198	50	100	83.4	29950	PASS
443	442	15	24	19.8	5945	PASS