




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012236.D
Acq On : 21 Oct 2022 09:46
Operator : CG/JU
Sample : N5103-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BB4

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

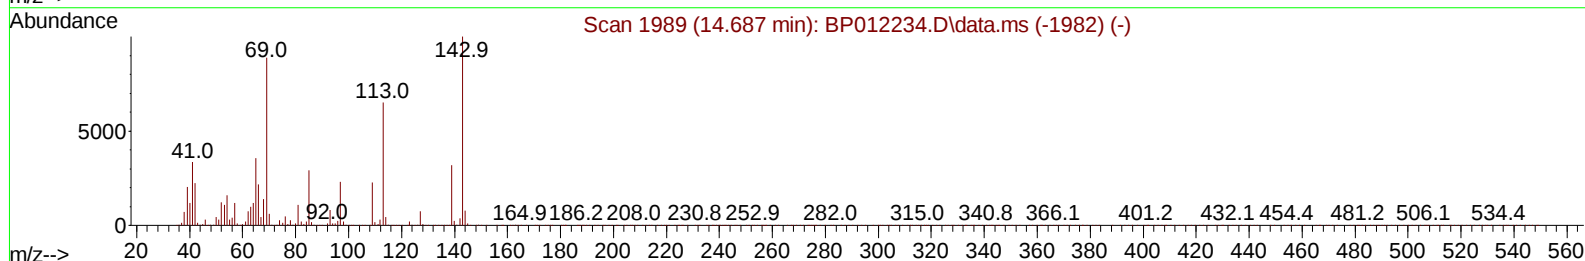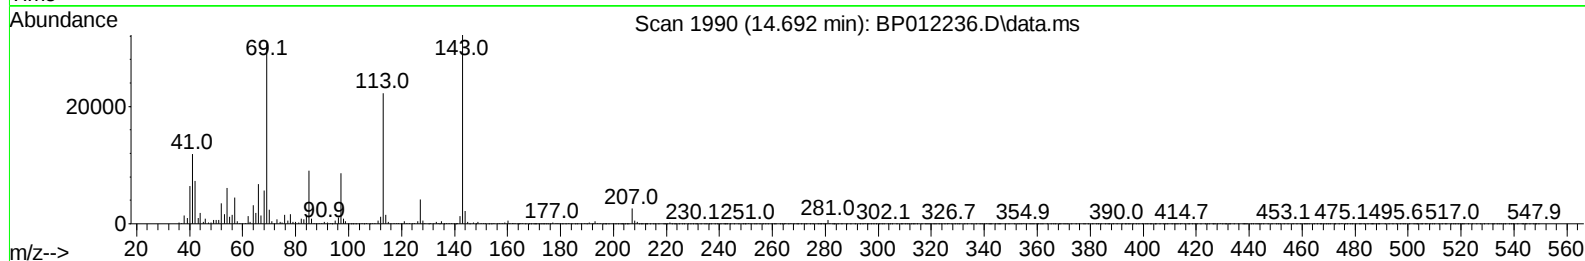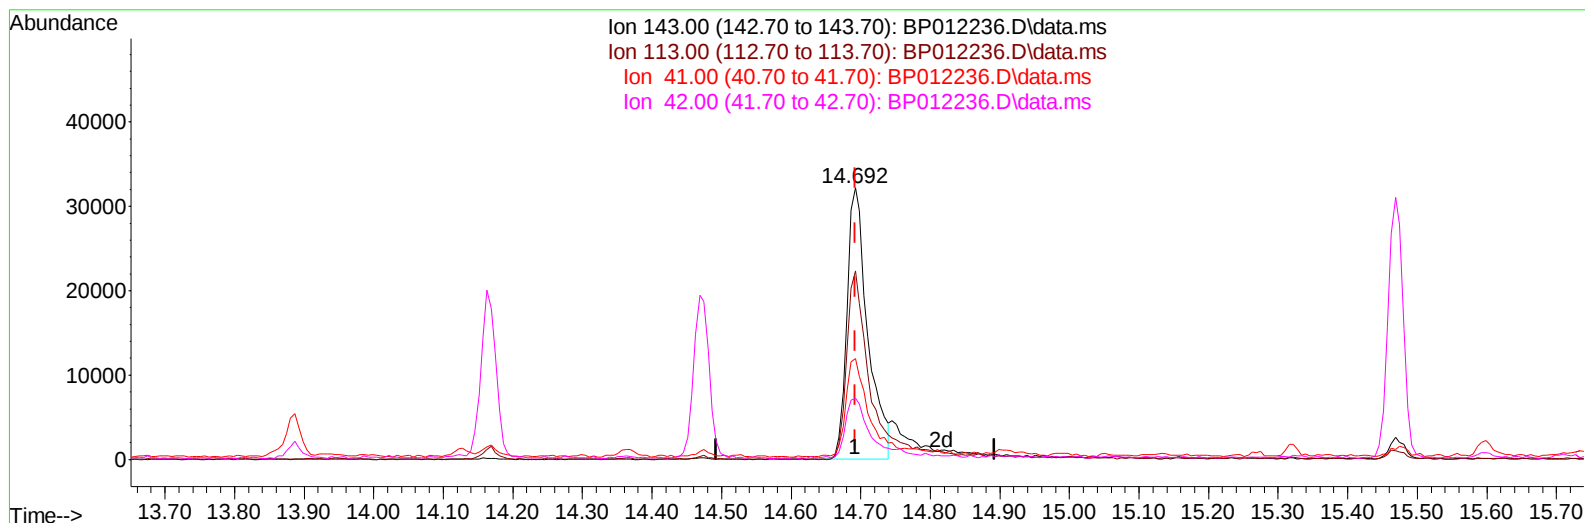

TIC: BP012236.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (-0.000) 4.25 ng/u1

response 66619

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	69.33
41.00	35.10	37.09
42.00	23.90	22.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012236.D
Acq On : 21 Oct 2022 09:46
Operator : CG/JU
Sample : N5103-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BB4

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

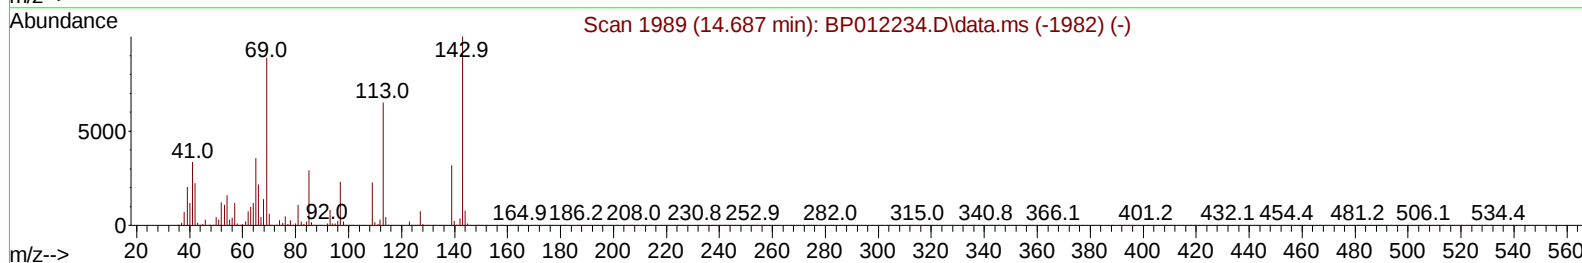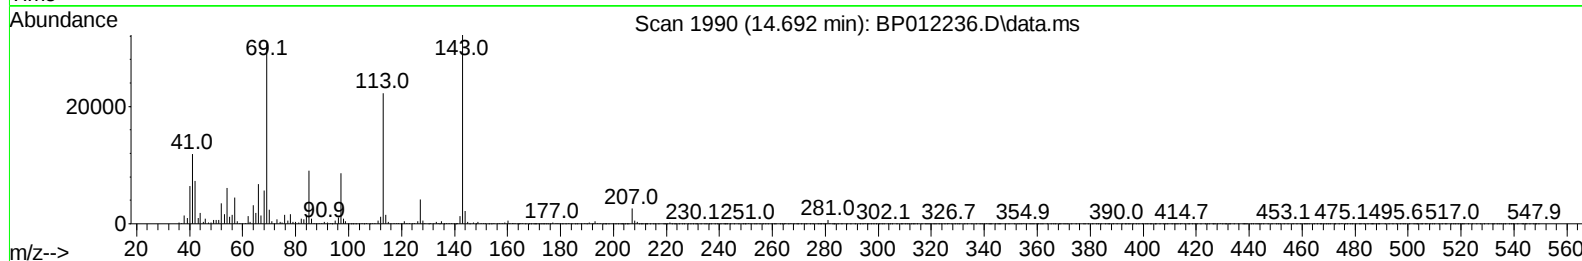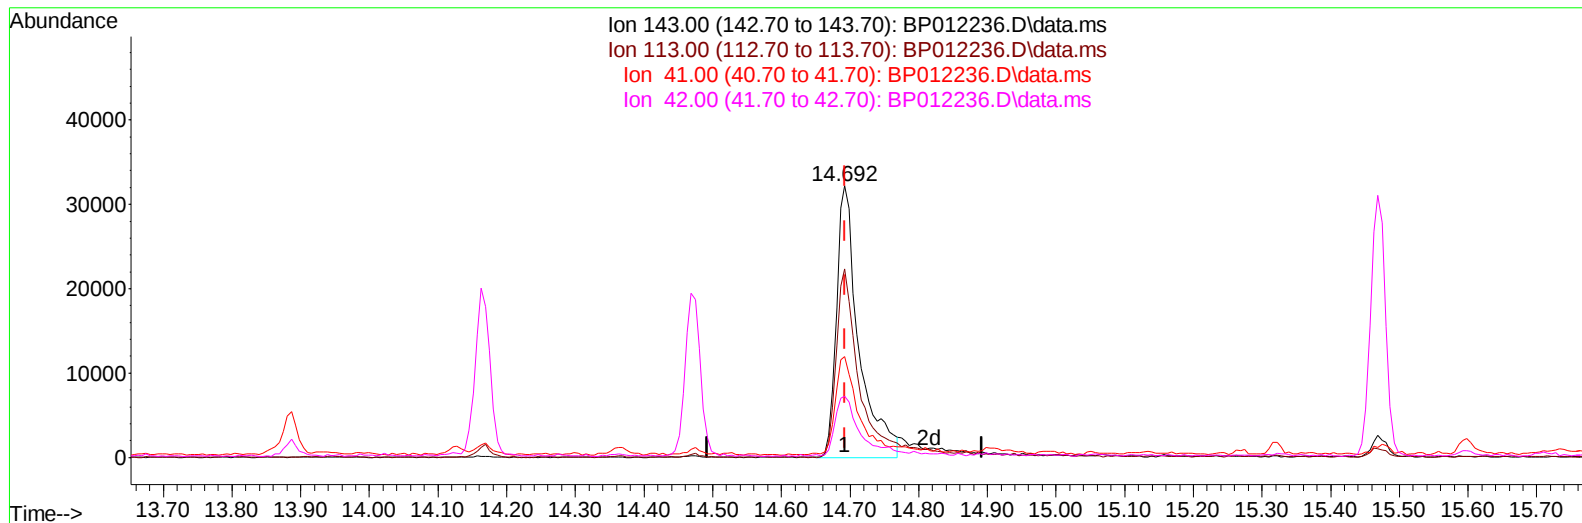

TIC: BP012236.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (-0.000) 4.64 ng/ul m

response 72794

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	69.33
41.00	35.10	37.09
42.00	23.90	22.60

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012236.D
 Acq On : 21 Oct 2022 09:46
 Operator : CG/JU
 Sample : N5103-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BB4

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:29:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	443870	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	1920670	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.475	164	1202987	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	2518675	20.000	ng/ul	0.00
79) Chrysene-d12	21.327	240	2036150	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264	1871286	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	31212	2.846	ng/uL	0.00
4) Pyridine-d5	3.681	84	279595	8.847	ng/ul	0.00
7) Phenol-d5	6.993	99	416919	10.880	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	636838	27.403	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	620462	21.272	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	498056	16.723	ng/ul	-0.01
21) Nitrobenzene-d5	8.993	128	424144	29.834	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	371494	24.219	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	675264	23.470	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	1013464	24.792	ng/ul	-0.01
46) Dimethylphthalate-d6	13.886	166	2619853	31.307	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	2945617	30.838	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.692	143	72794m	4.643	ng/ul	0.00
60) Fluorene-d10	15.469	176	2253488	31.302	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	32255	2.251	ng/ul	0.00
73) Anthracene-d10	17.333	188	3555627	32.207	ng/ul	0.00
81) Pyrene-d10	19.574	212	3825818	33.001	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.574	264	3124164	33.292	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	13.934	163	90832	1.036	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012236.D
Acq On : 21 Oct 2022 09:46
Operator : CG/JU
Sample : N5103-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BB4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

