




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

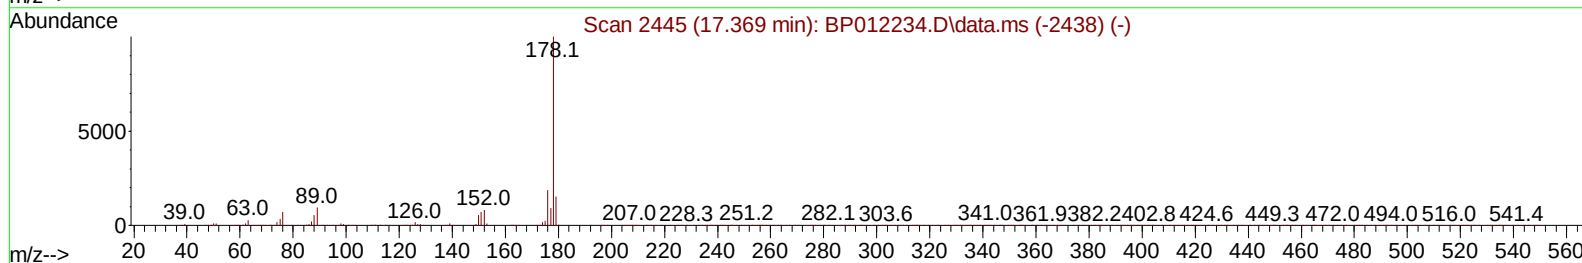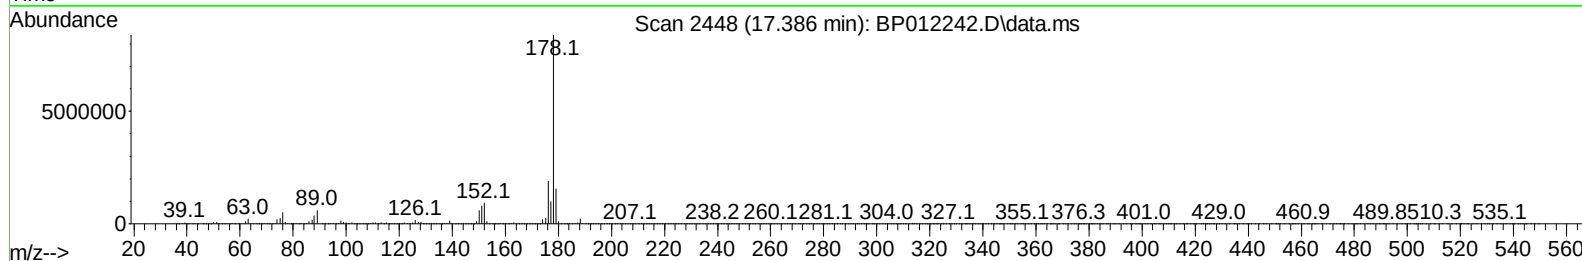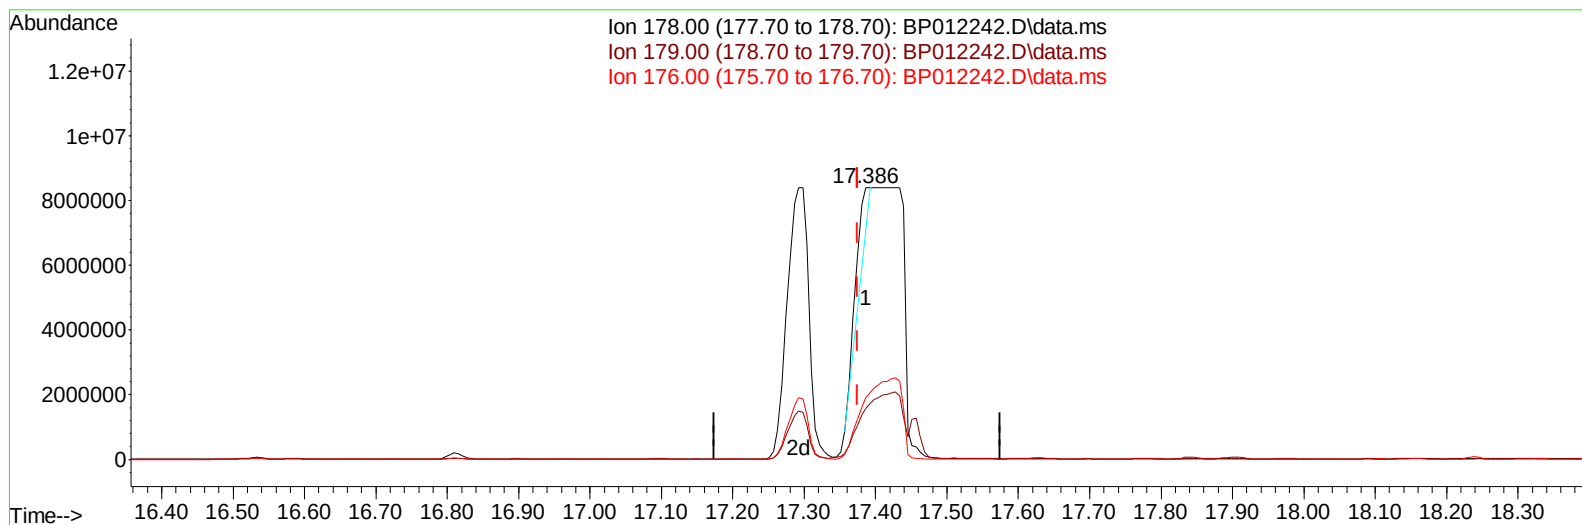

TIC: BP012242.D\data.ms

(74) Anthracene

17.386min (+ 0.012) 45.86 ng/ul

response 3781793

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	18.81#
176.00	18.70	22.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

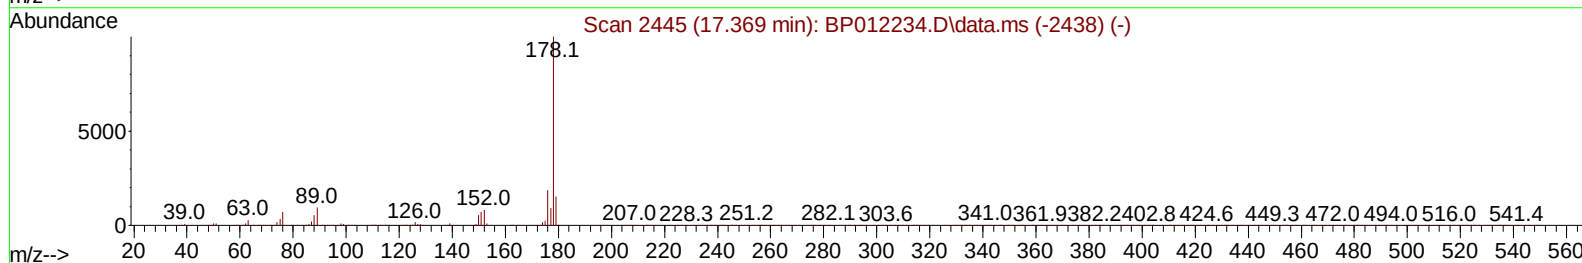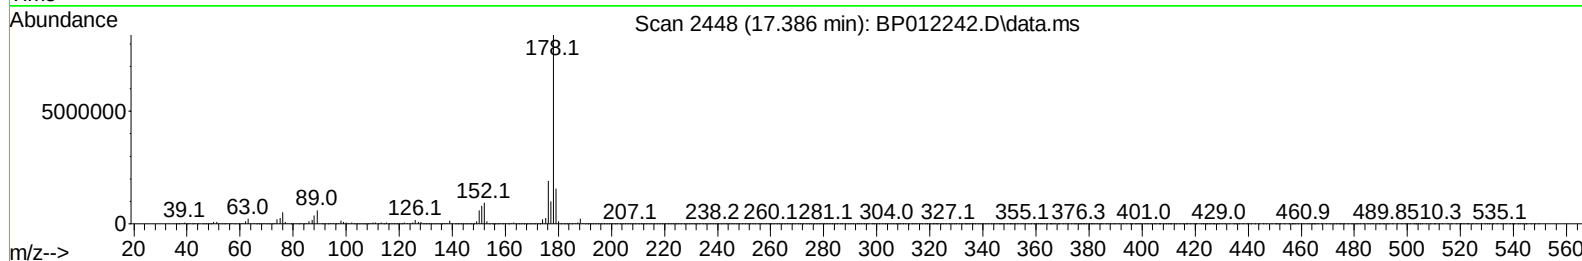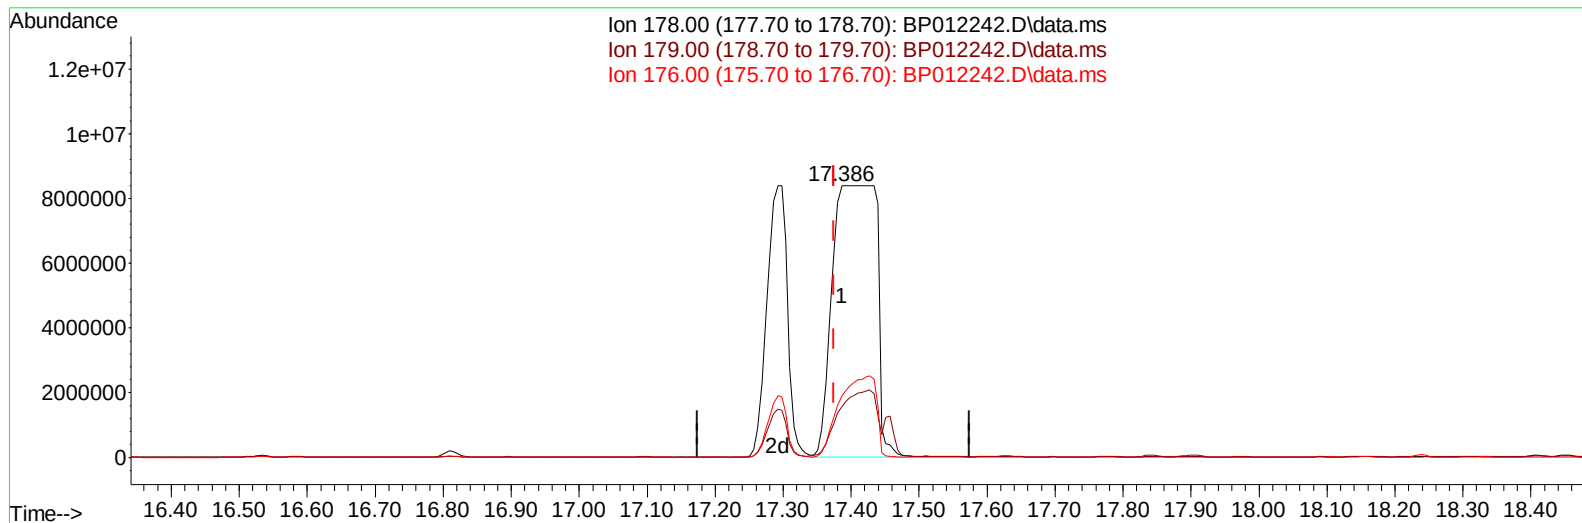

TIC: BP012242.D\data.ms

(74) Anthracene

17.386min (+ 0.012) 460.07 ng/uL m

response 37936156

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	18.81#
176.00	18.70	22.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

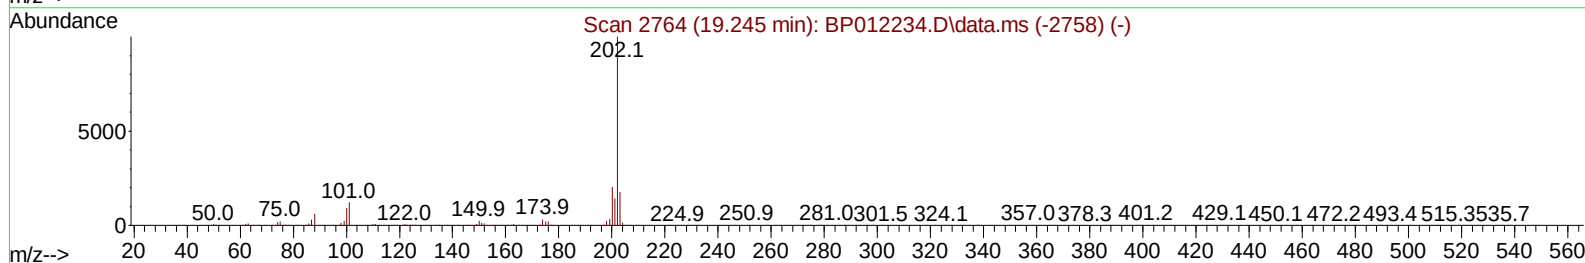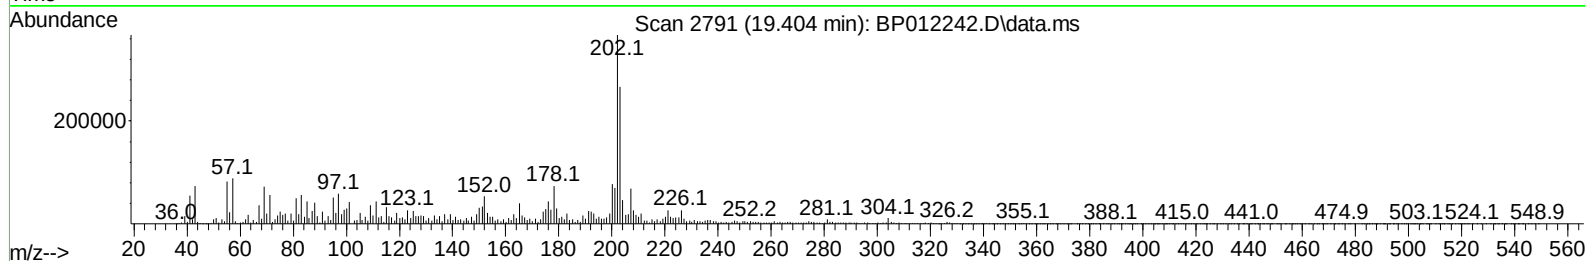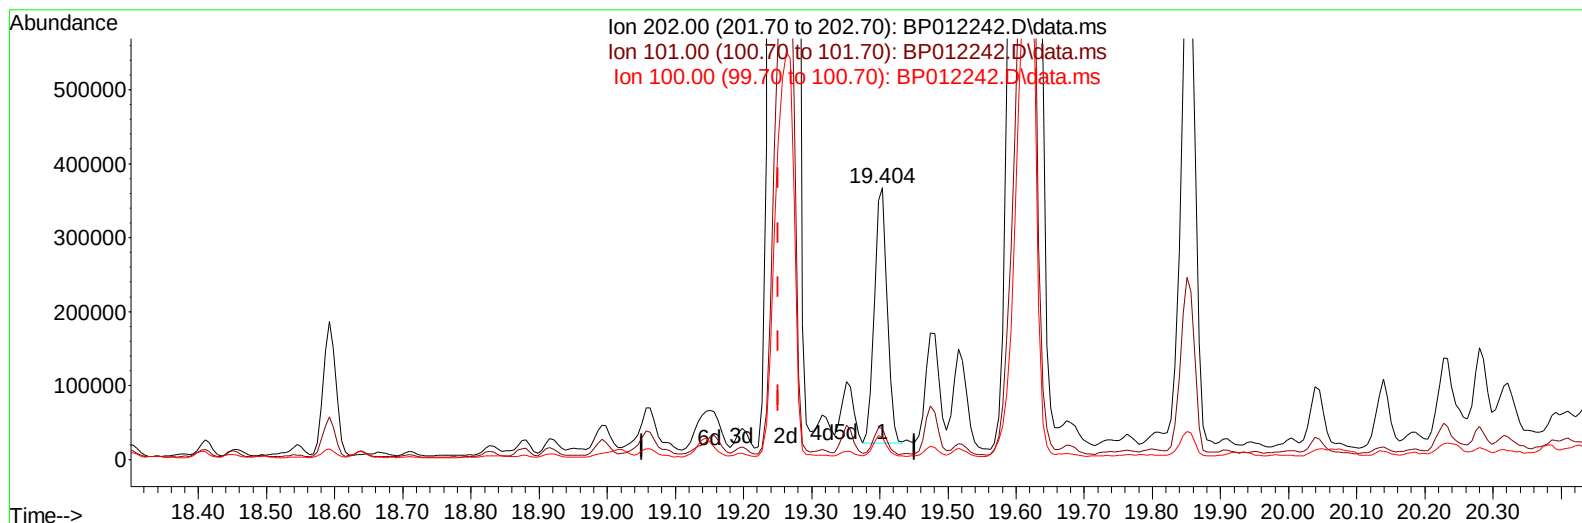

TIC: BP012242.D\data.ms

(80) Fluoranthene

19.404min (+ 0.153) 5.52 ng/u1

response 452129

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	11.48
100.00	9.60	8.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

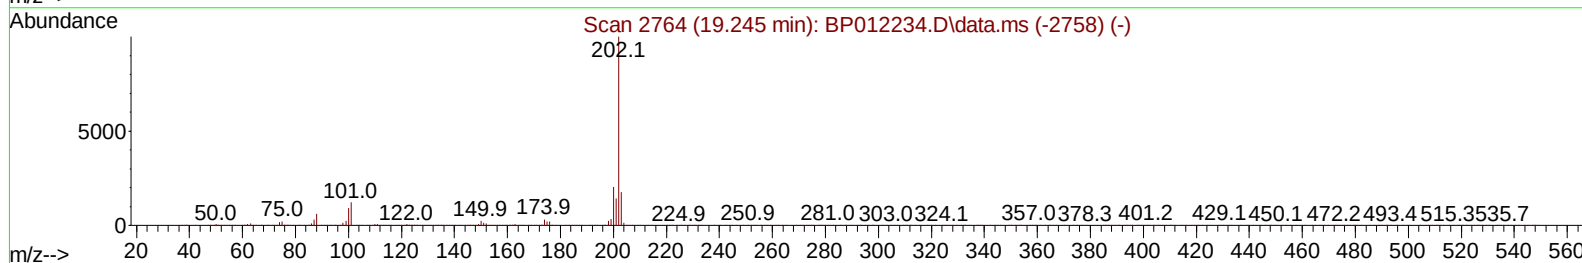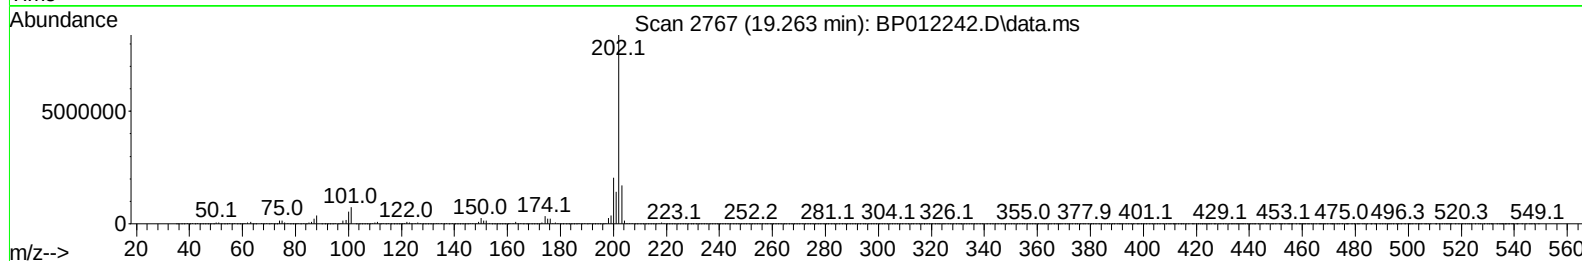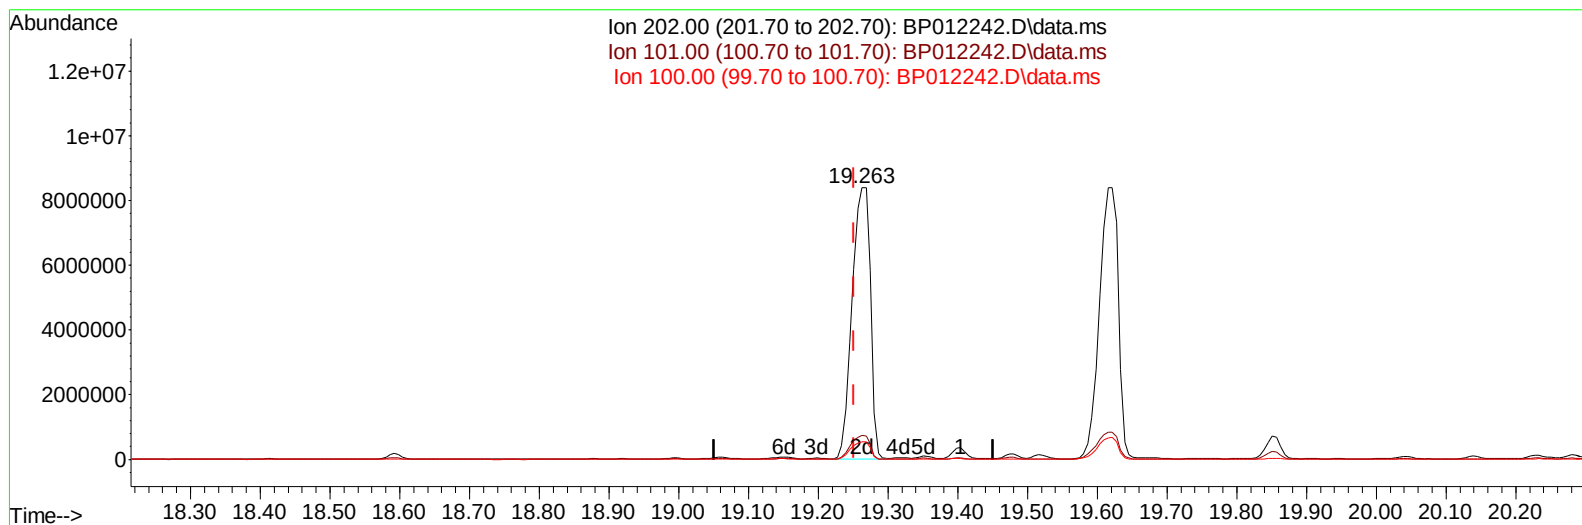

TIC: BP012242.D\data.ms

(80) Fluoranthene

19.263min (+ 0.012) 187.69 ng/ul m

response 15383297

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	8.76#
100.00	9.60	6.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

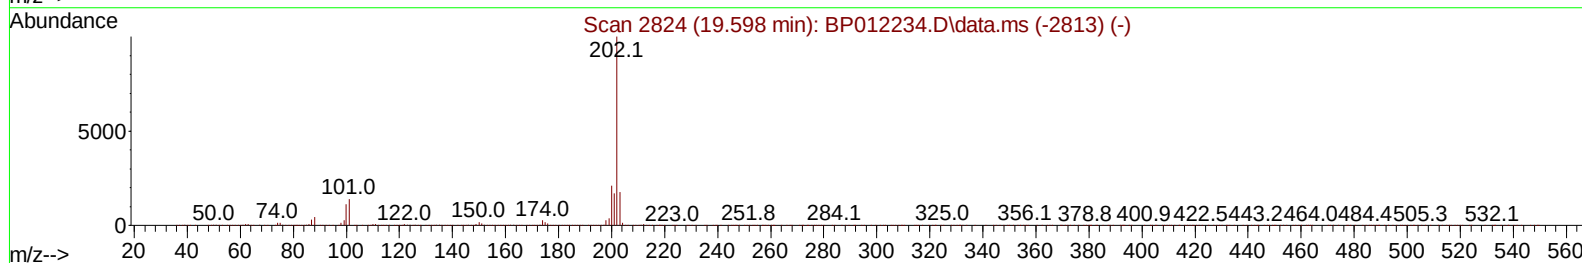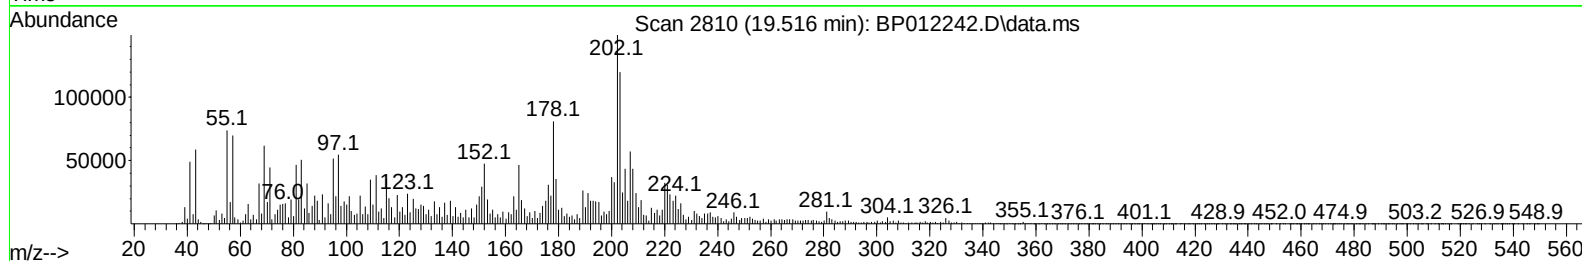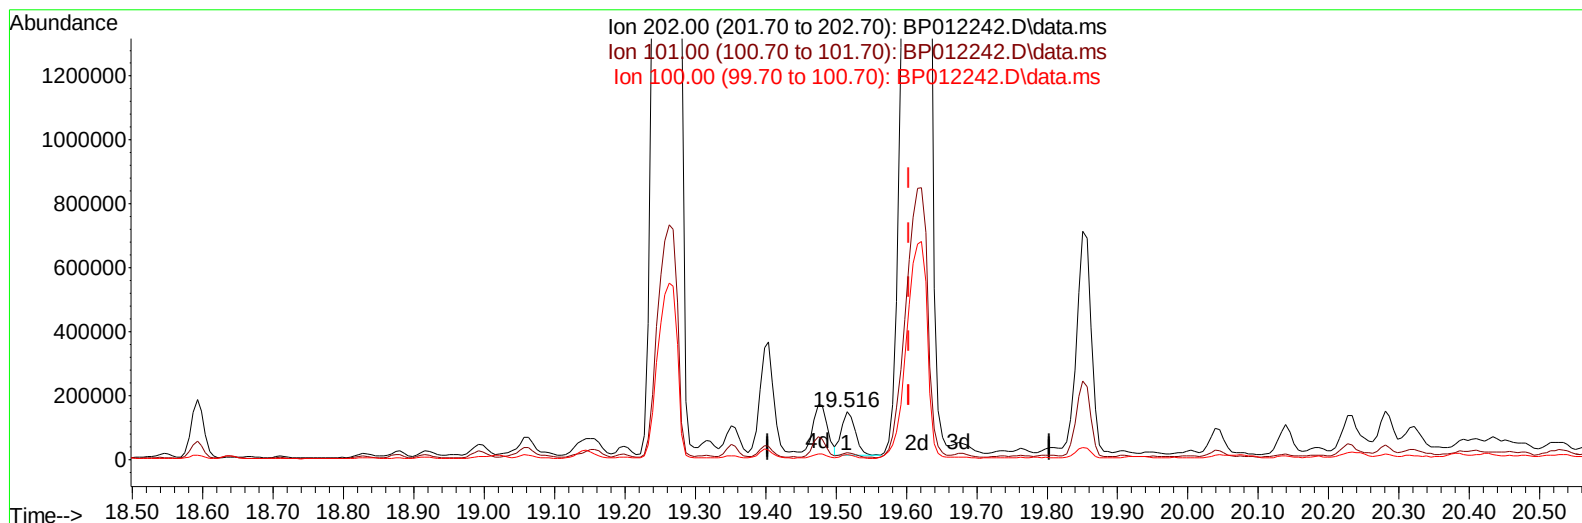

TIC: BP012242.D\data.ms

(82) Pyrene

19.516min (-0.088) 2.17 ng/u1

response 182224

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.40	14.53
100.00	12.50	10.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

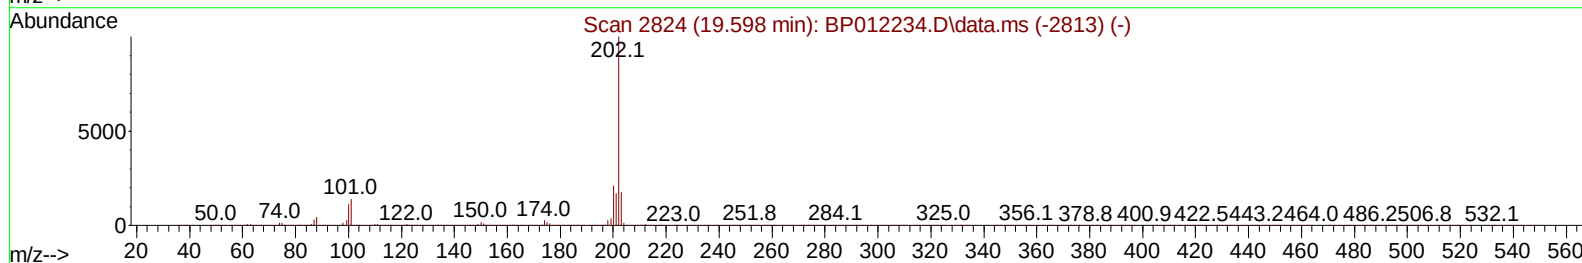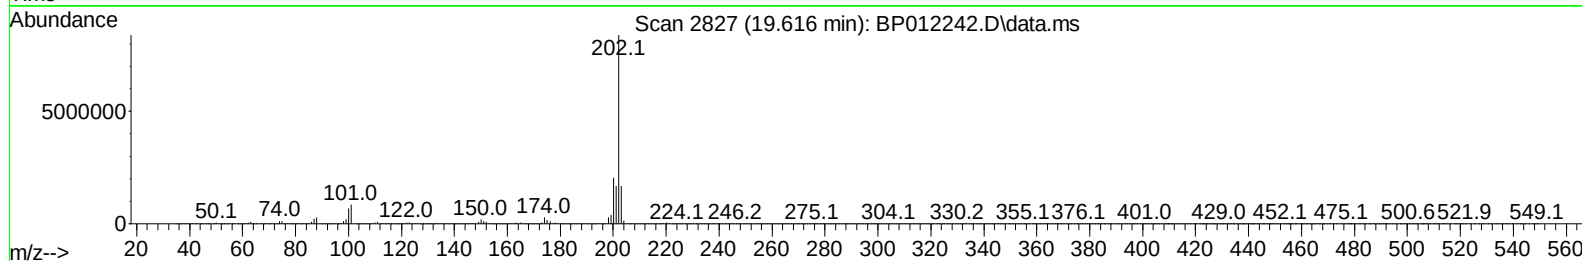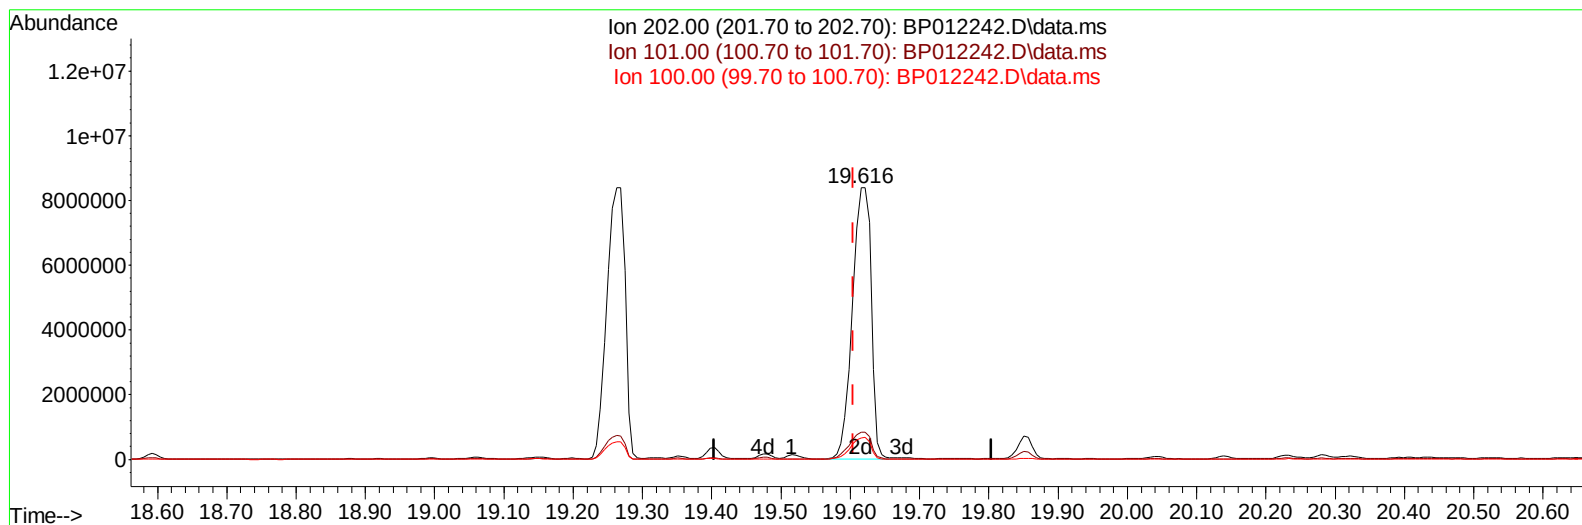

TIC: BP012242.D\data.ms

(82) Pyrene

19.616min (+ 0.012) 188.04 ng/ul m

response 15768533

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.40	10.12#
100.00	12.50	8.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

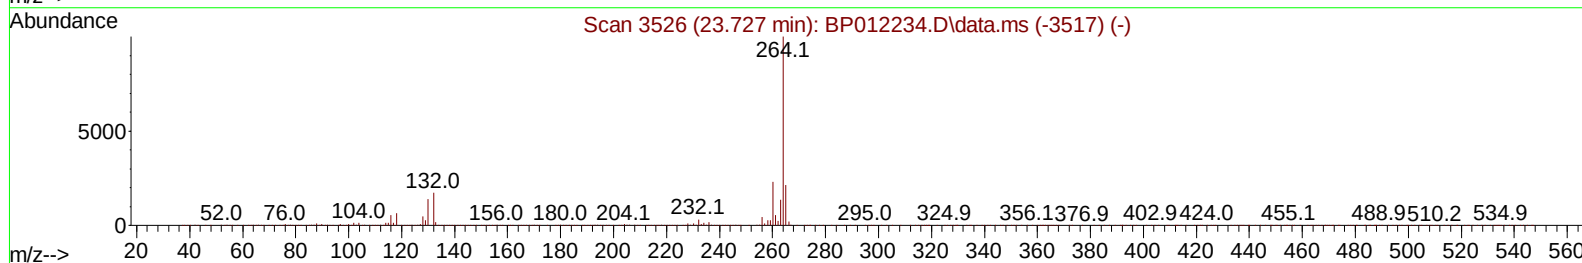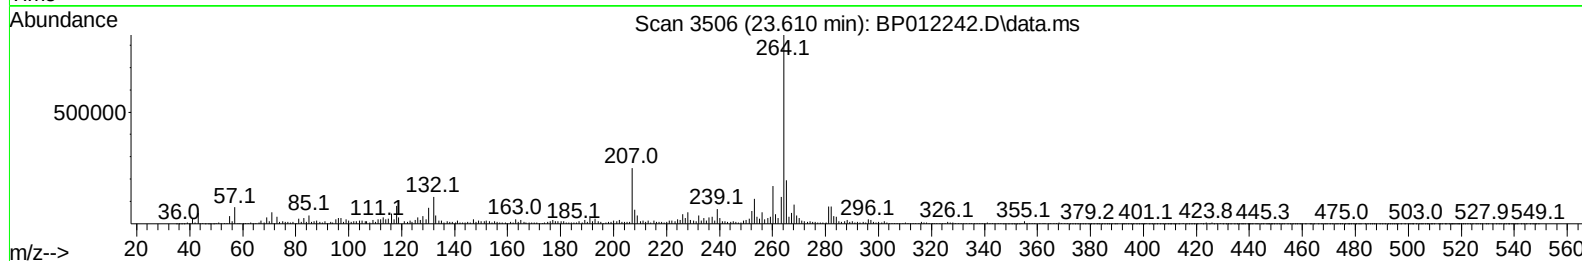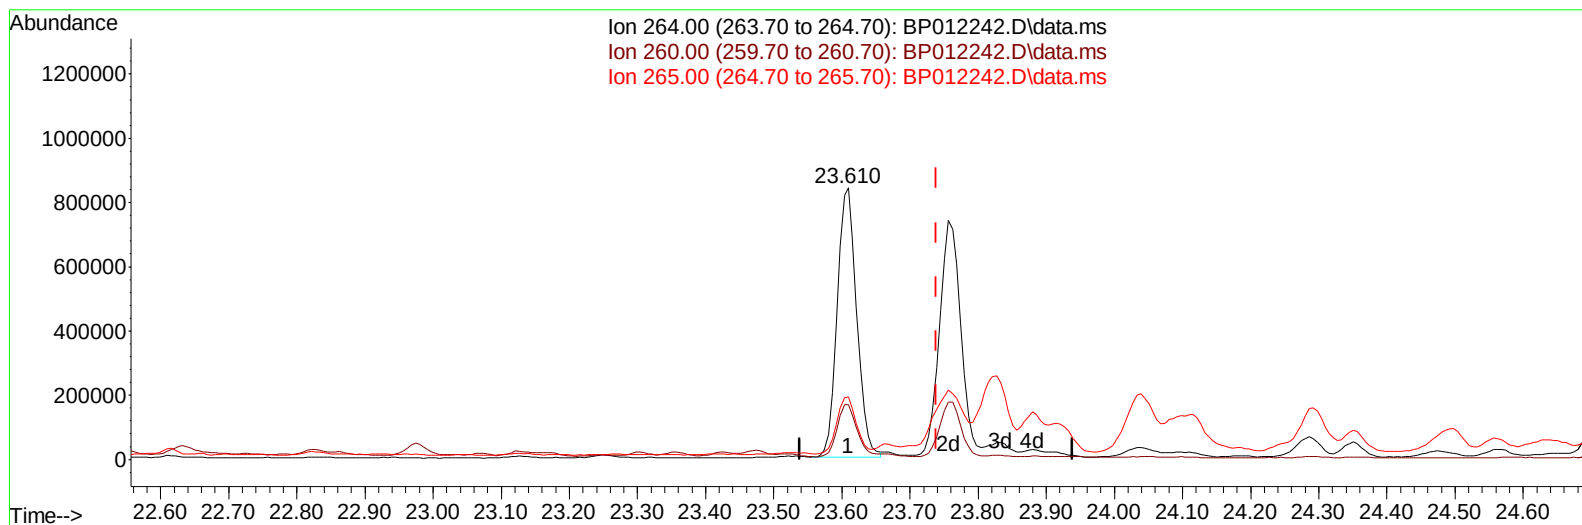

TIC: BP012242.D\data.ms

(88) Perylene-d12 (I)

23.610min (-0.129) 20.00 ng/u1

response 1667108

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	23.70	20.13
265.00	22.20	23.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

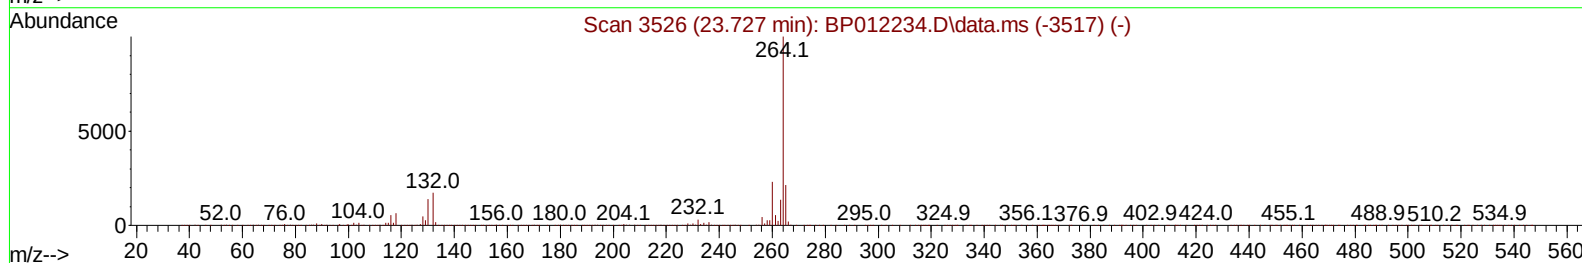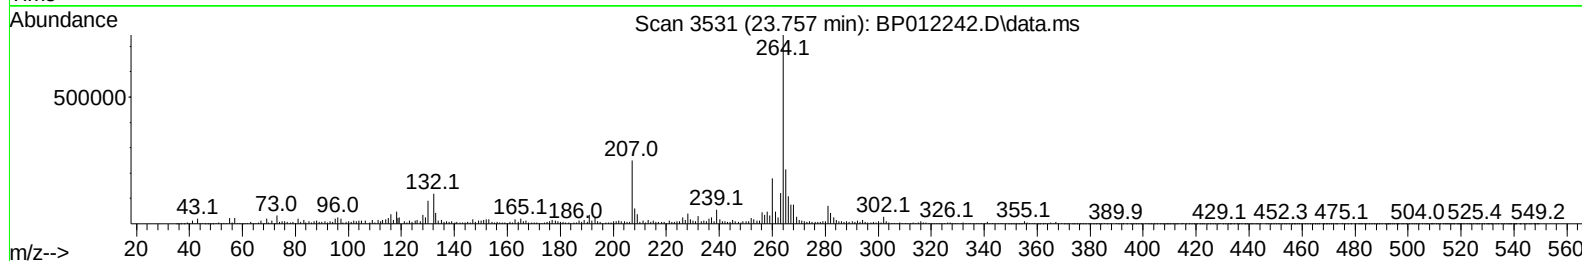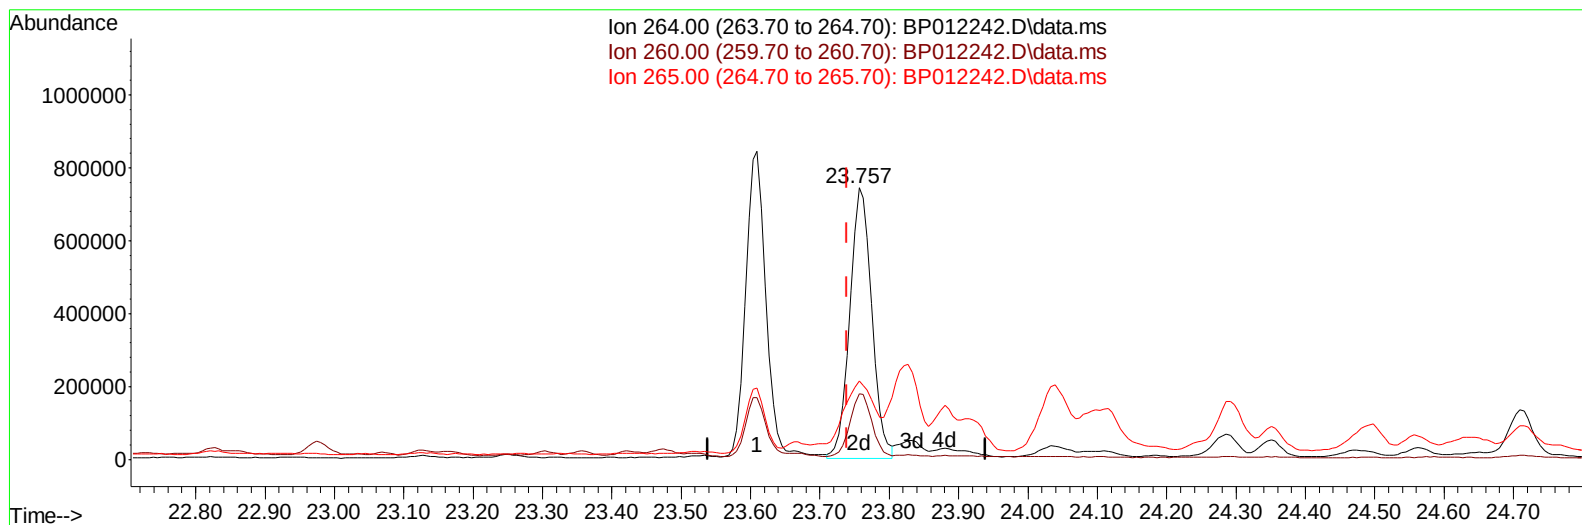

TIC: BP012242.D\data.ms

(88) Perylene-d12 (I)

23.757min (+ 0.018) 20.00 ng/ul m

response 1635014

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	23.70	24.10
265.00	22.20	28.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

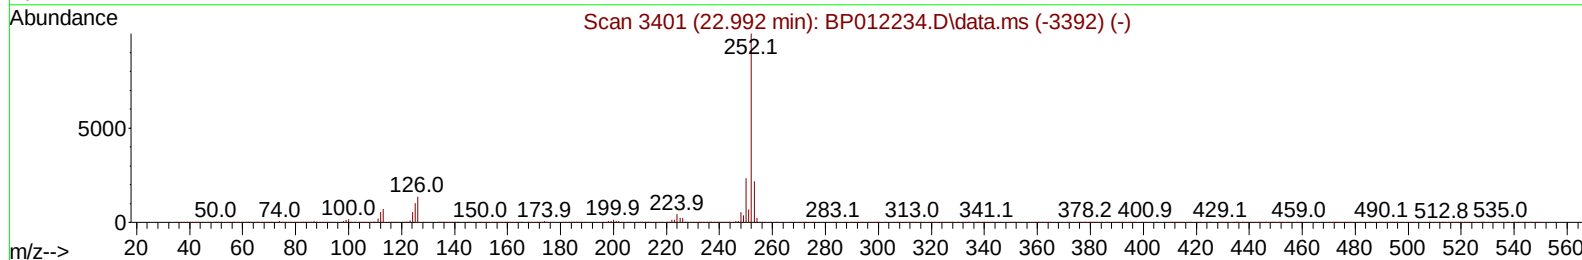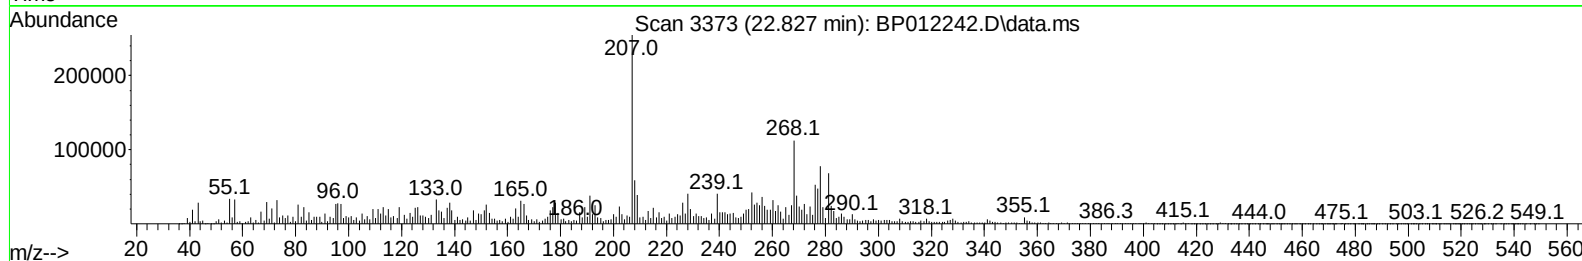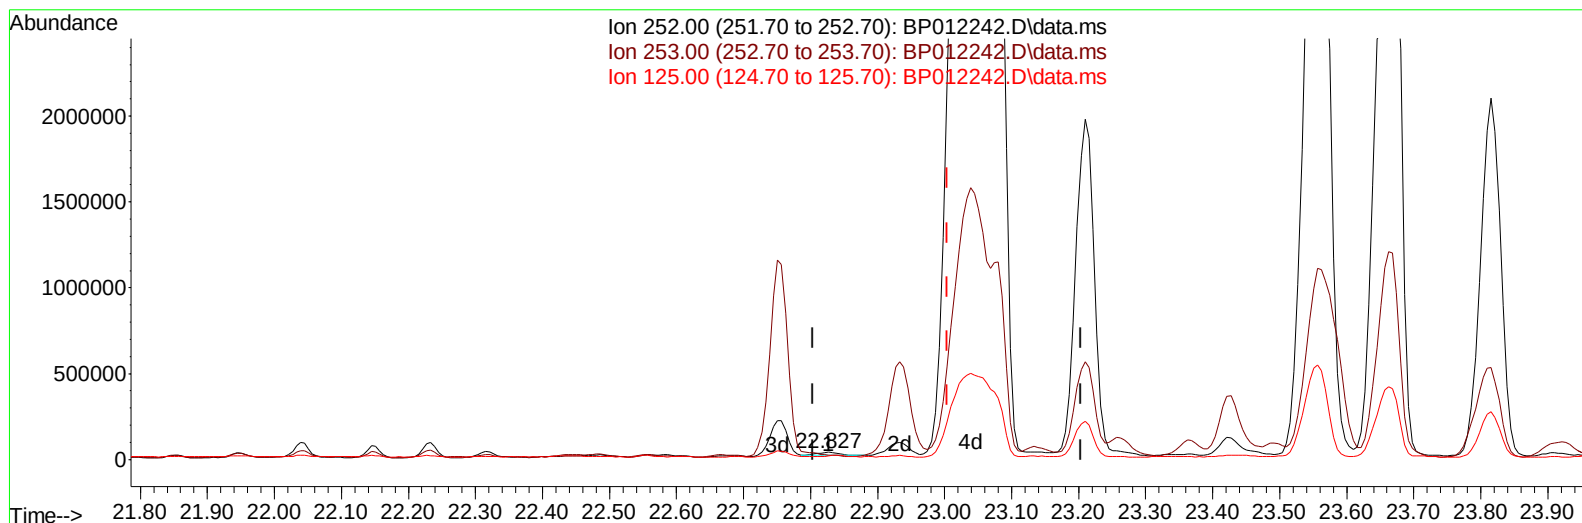

TIC: BP012242.D\data.ms

(90) Benzo(b)fluoranthene

22.827min (-0.176) 0.40 ng/u1

response 43152

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	61.33#
125.00	10.60	51.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

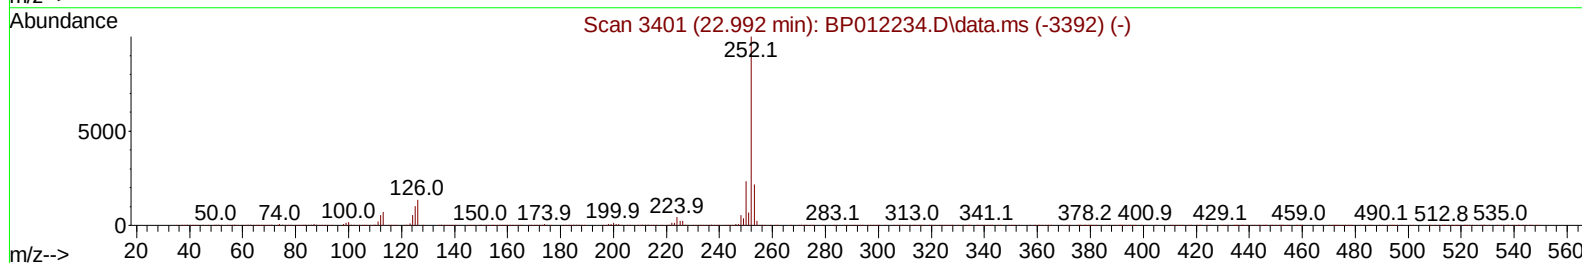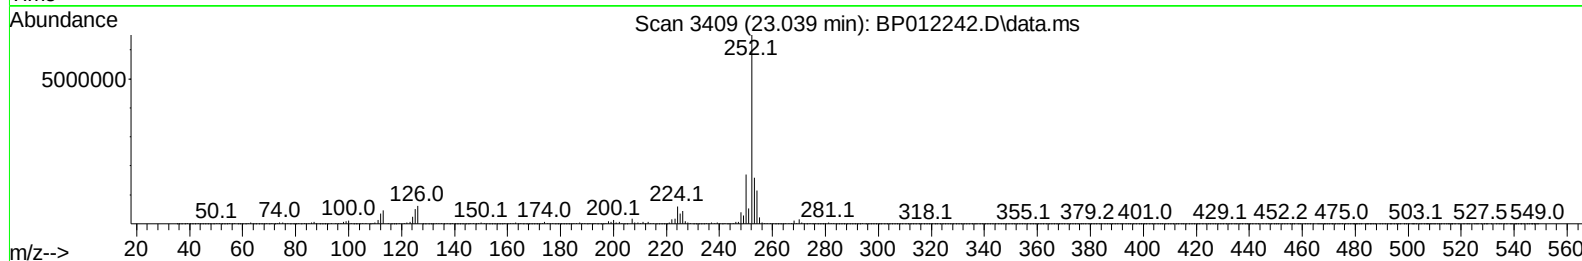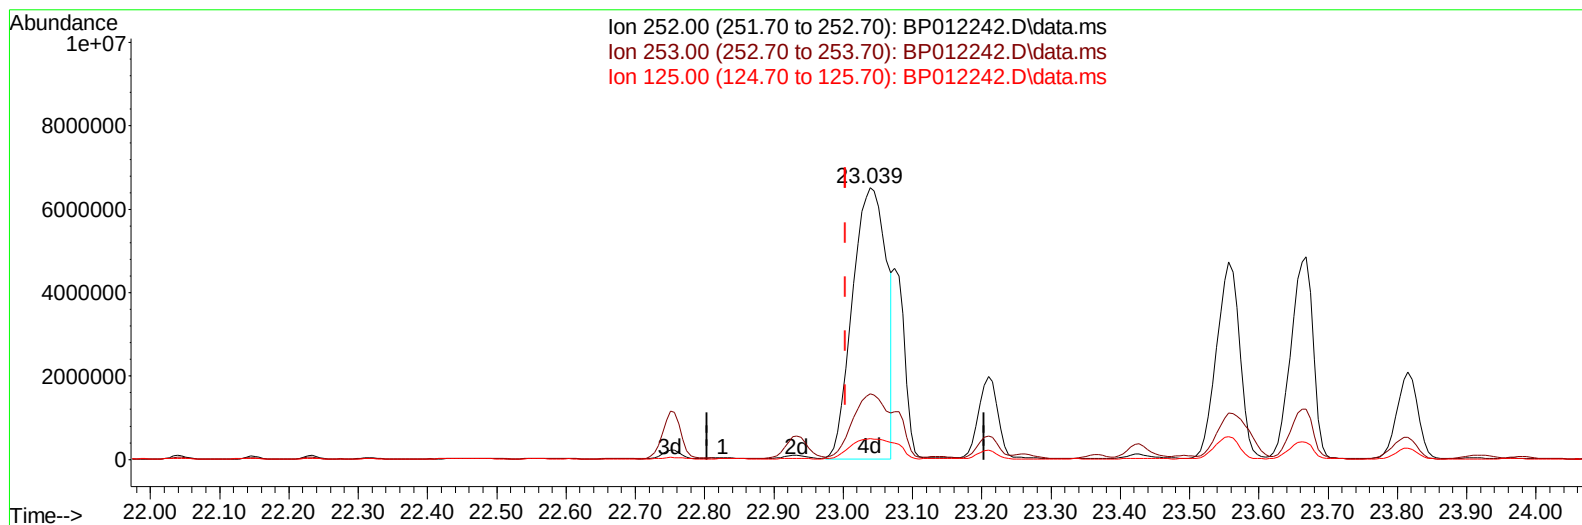

TIC: BP012242.D\data.ms

(90) Benzo(b)fluoranthene

23.039min (+ 0.035) 203.73 ng/ul m

response 22199393

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.90	24.28
125.00	10.60	7.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

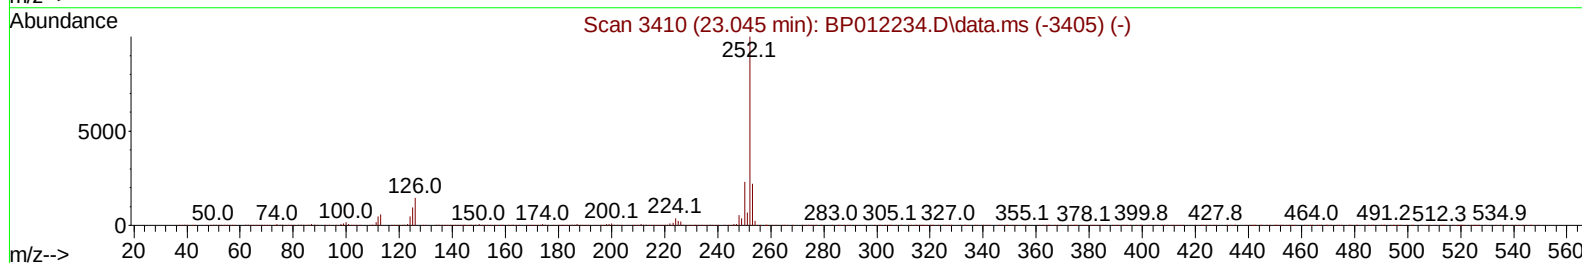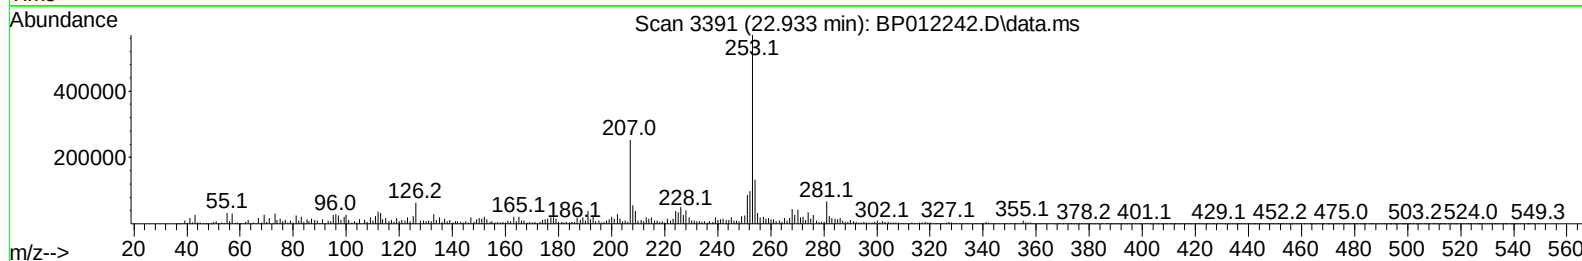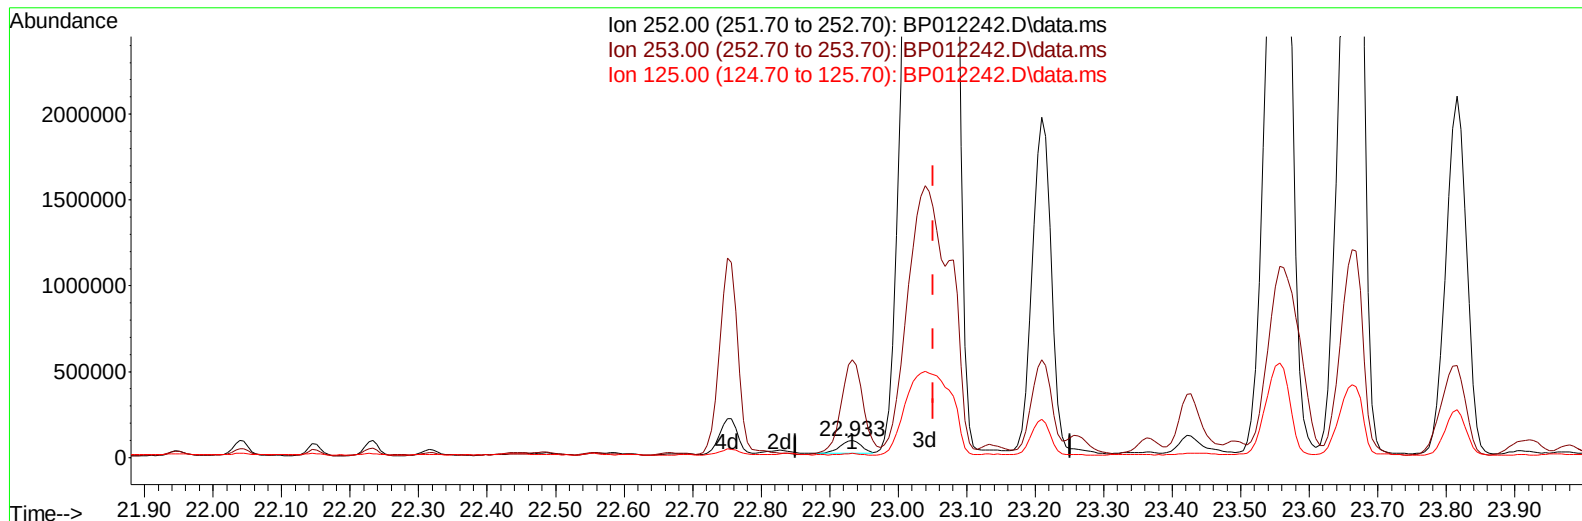

TIC: BP012242.D\data.ms

(91) Benzo(k)fluoranthene

22.933min (-0.118) 1.55 ng/u1

response 166396

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	574.98#
125.00	10.80	23.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

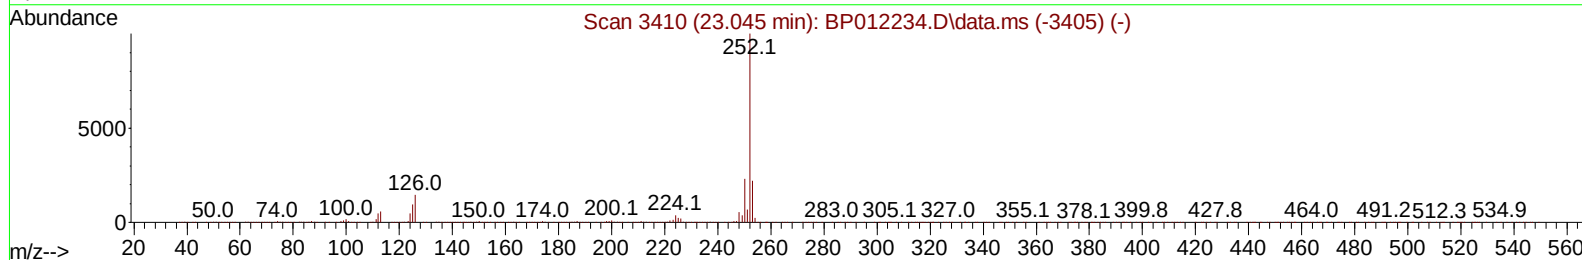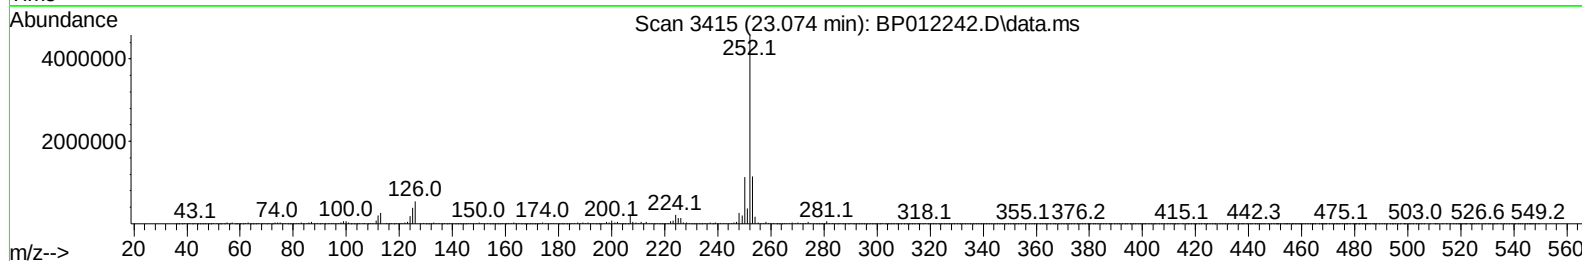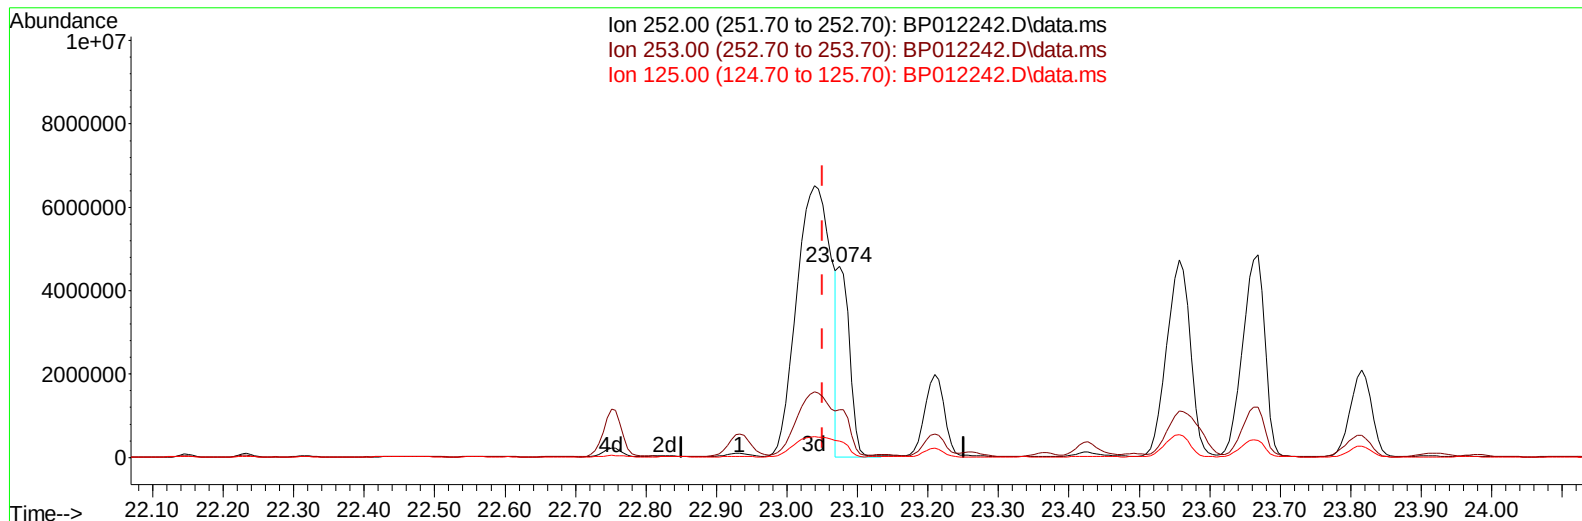

TIC: BP012242.D\data.ms

(91) Benzo(k)fluoranthene

23.074min (+ 0.024) 50.16 ng/ul m

response 5387510

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	25.05
125.00	10.80	8.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

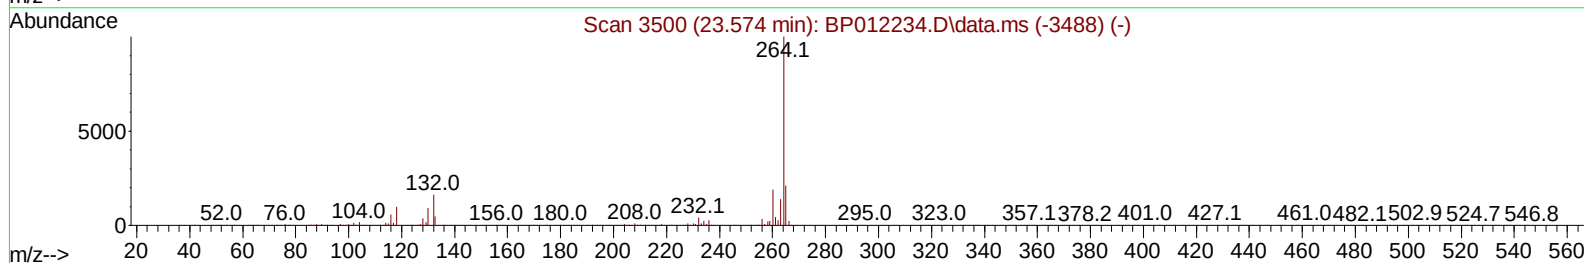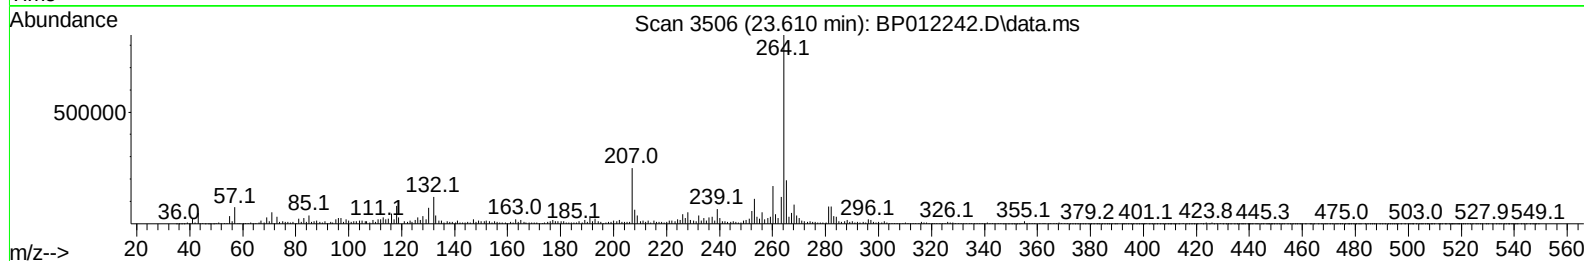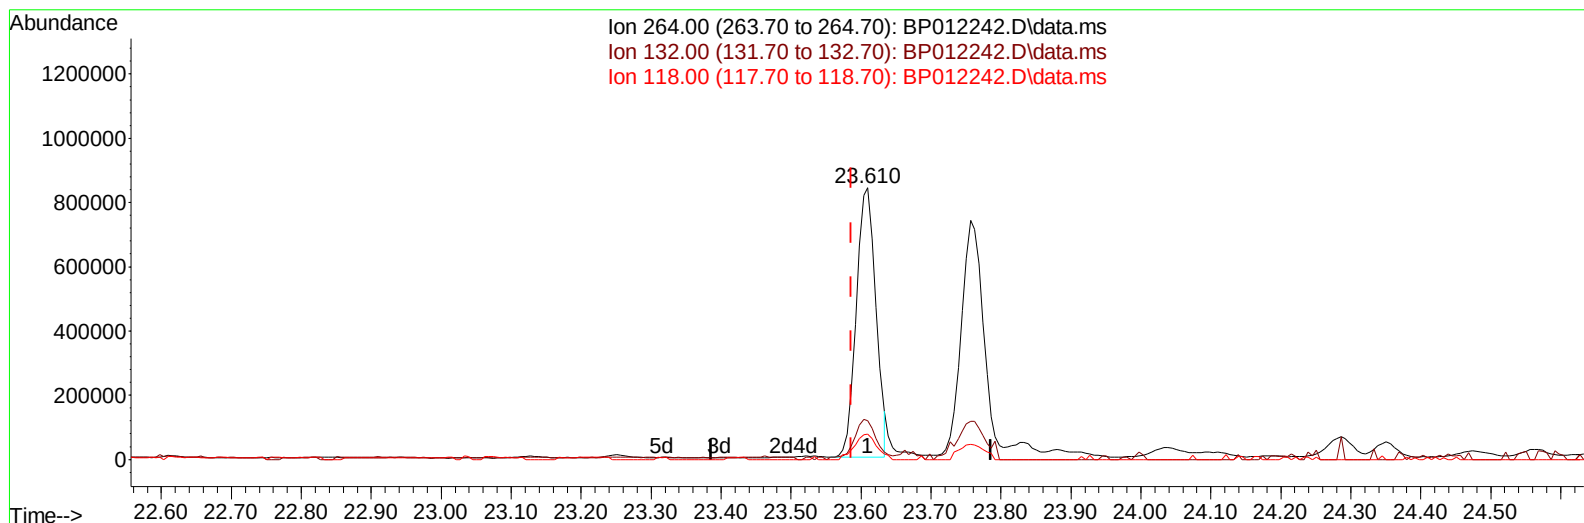

TIC: BP012242.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.610min (+ 0.024) 19.77 ng/u1

response 1621343

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	16.90	14.33
118.00	9.80	9.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

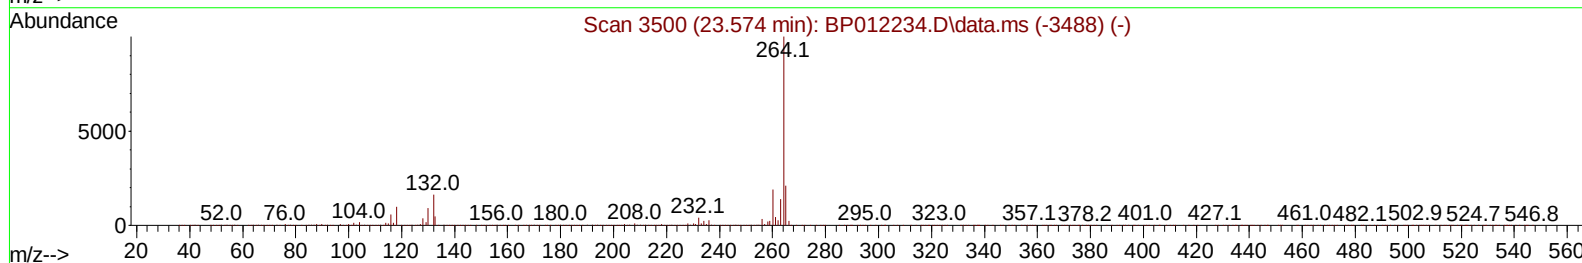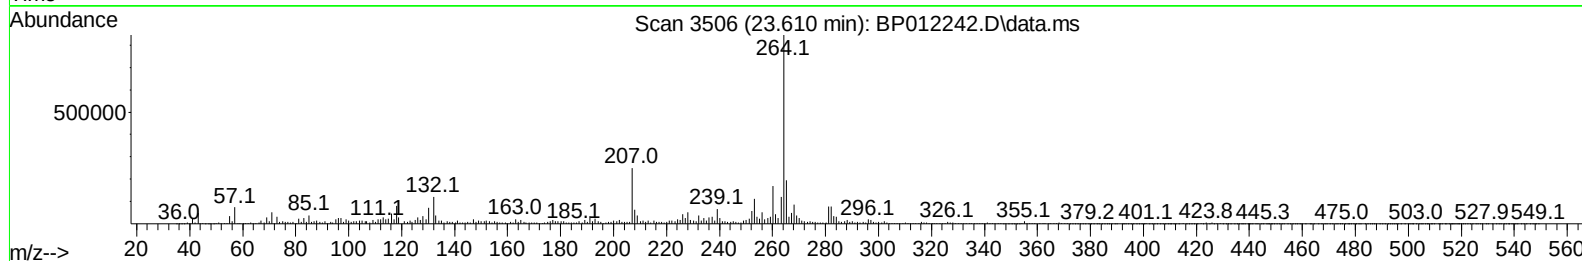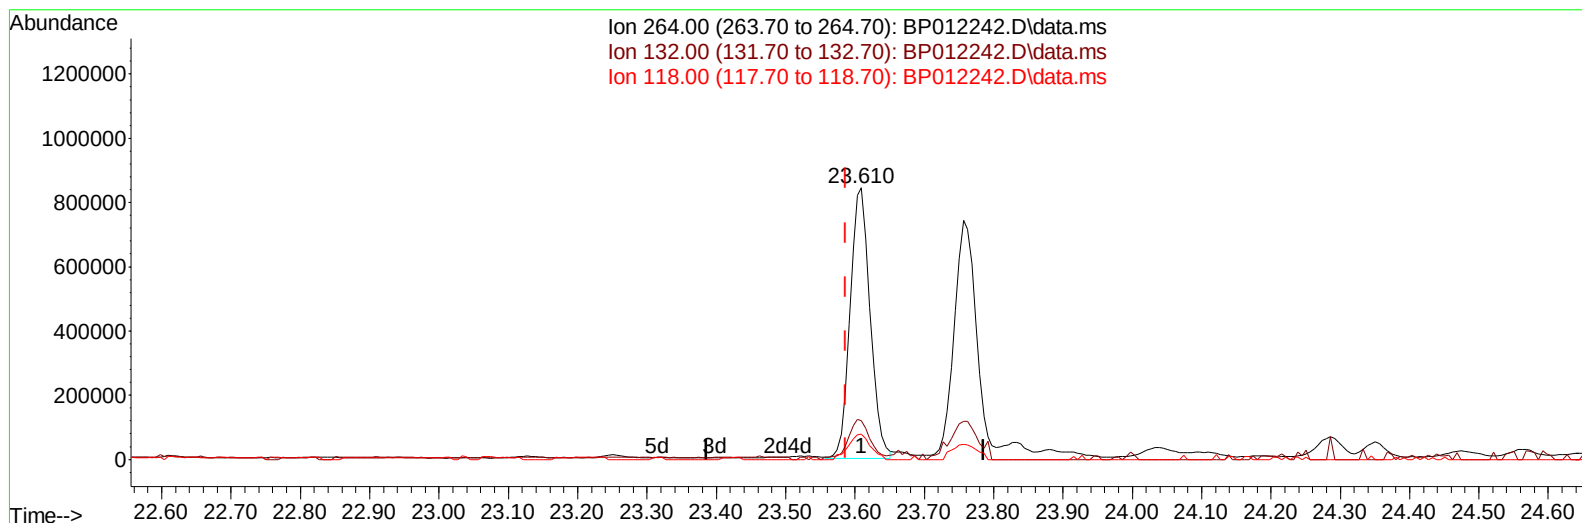

TIC: BP012242.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.610min (+ 0.024) 20.50 ng/ul m

response 1681026

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	16.90	14.33
118.00	9.80	9.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

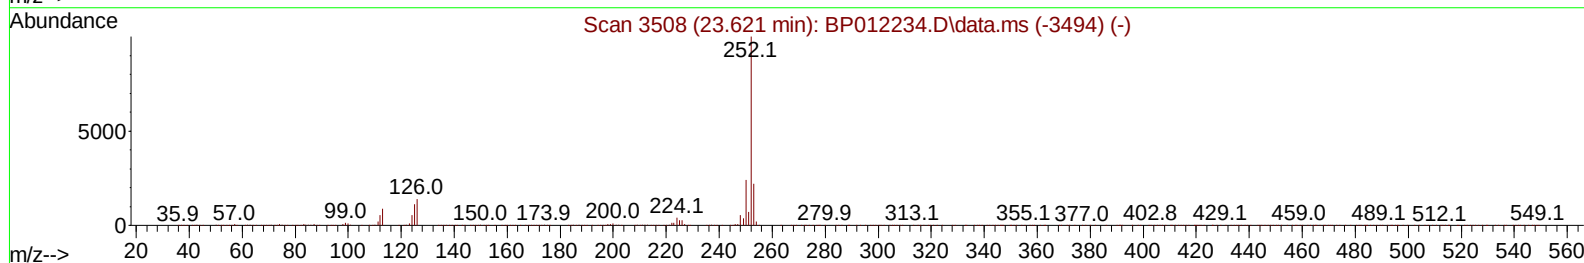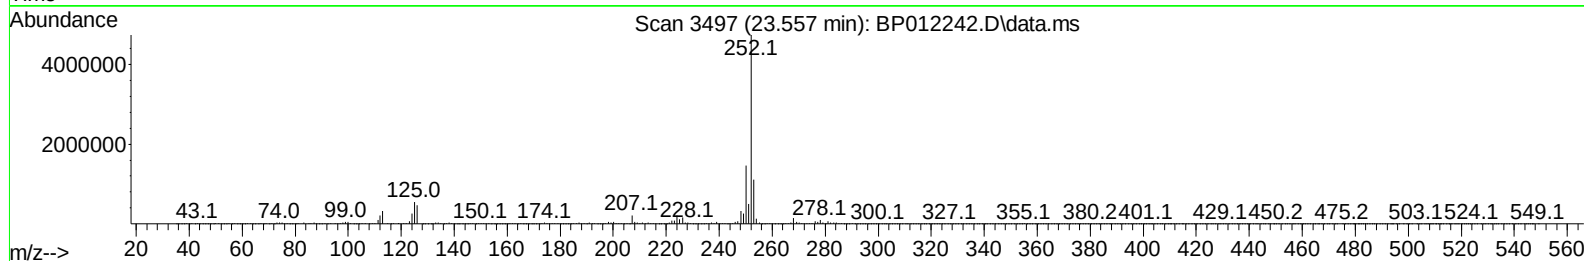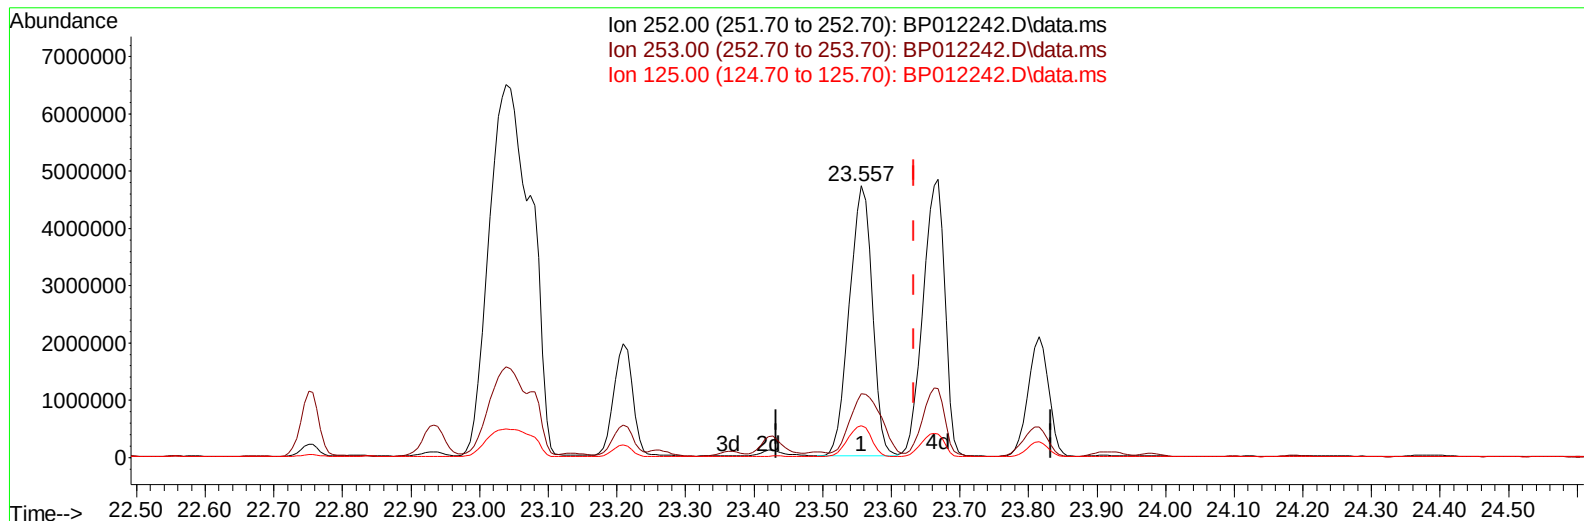

TIC: BP012242.D\data.ms

(93) Benzo(a)pyrene (C)

23.557min (-0.076) 117.65 ng/ul

response 10962144

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	23.50
125.00	12.10	11.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

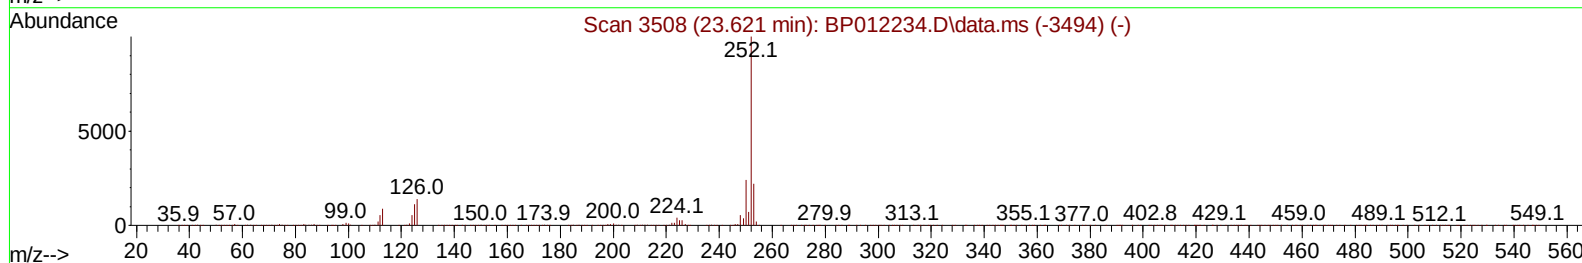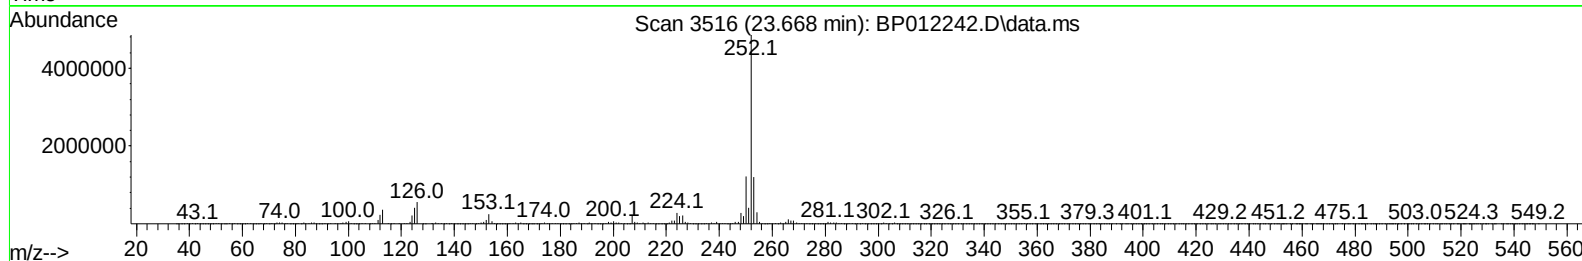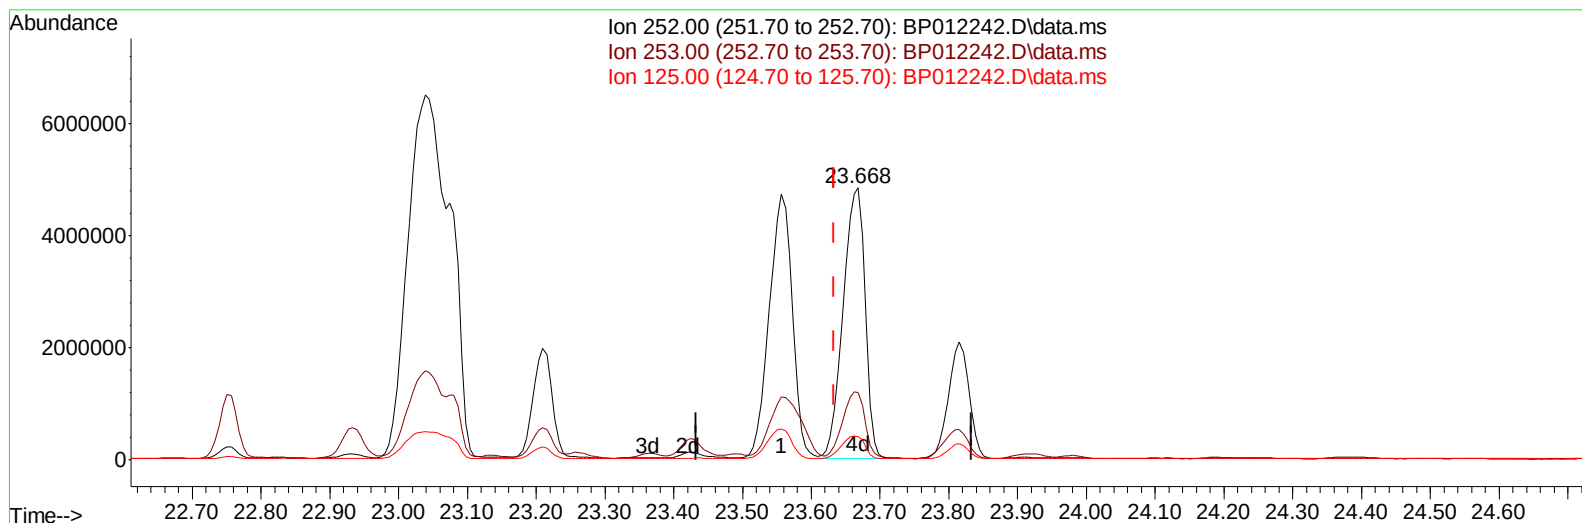

TIC: BP012242.D\data.ms

(93) Benzo(a)pyrene (C)

23.668min (+ 0.035) 115.85 ng/ul m

response 10794414

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	24.75
125.00	12.10	8.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

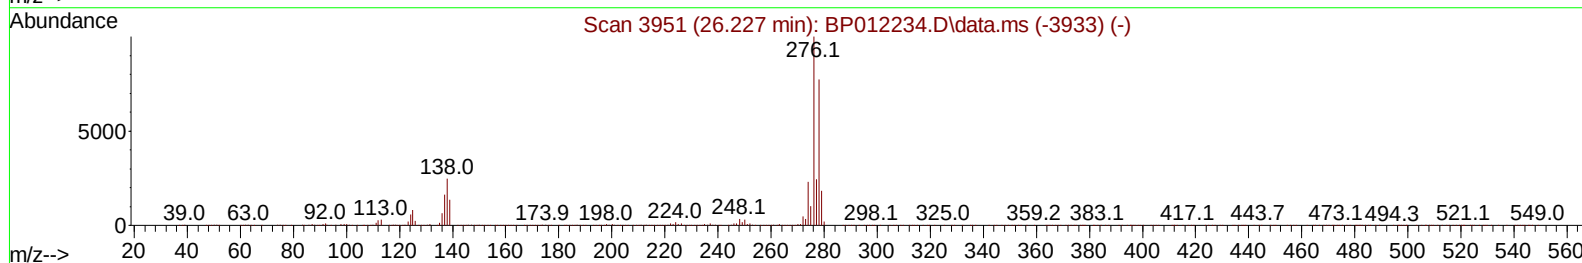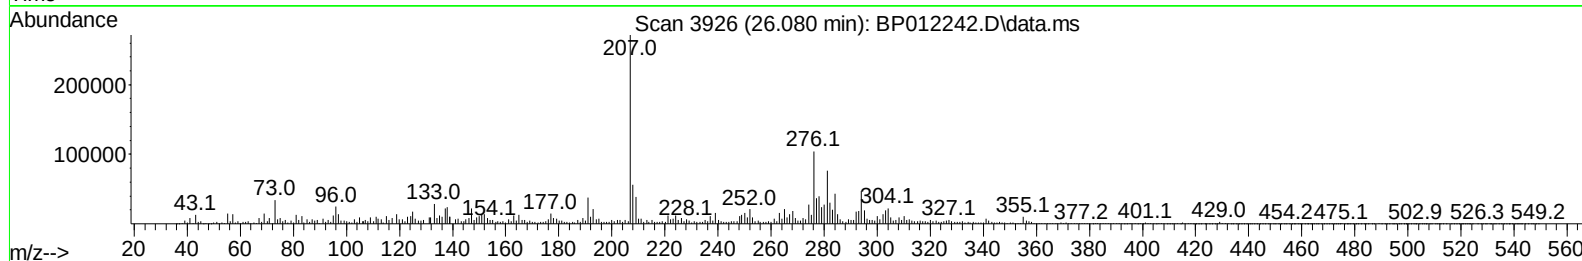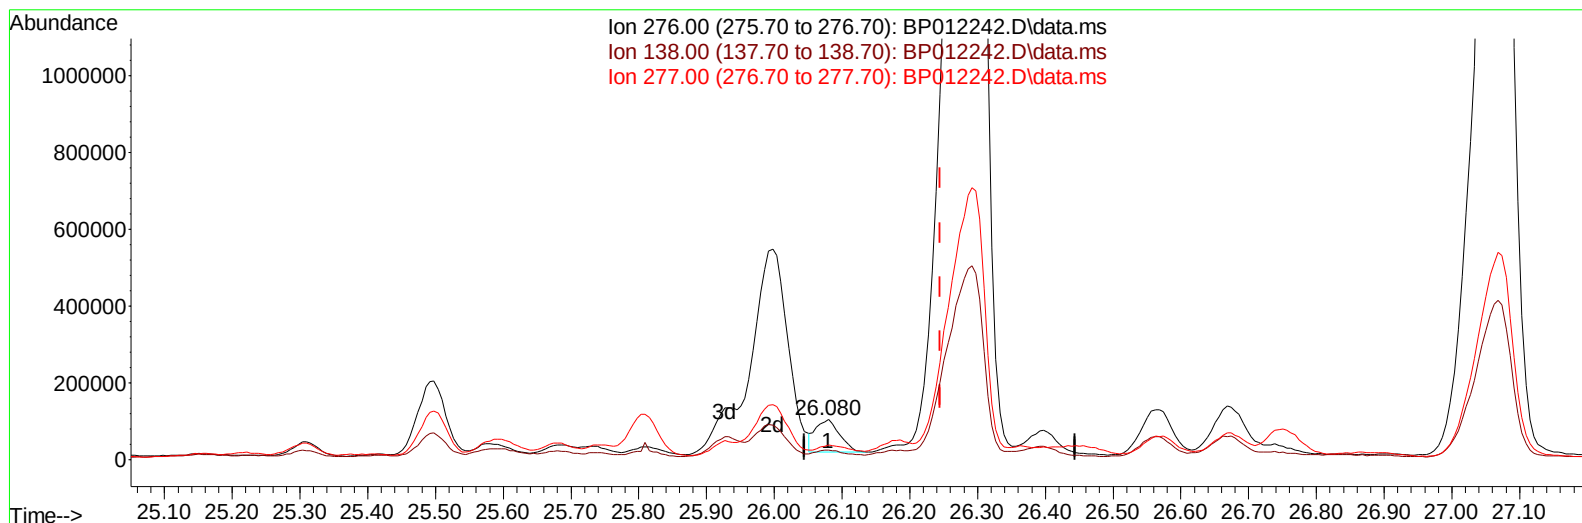

TIC: BP012242.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

26.080min (-0.165) 1.97 ng/u1

response 212457

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.40	22.85
277.00	25.30	35.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

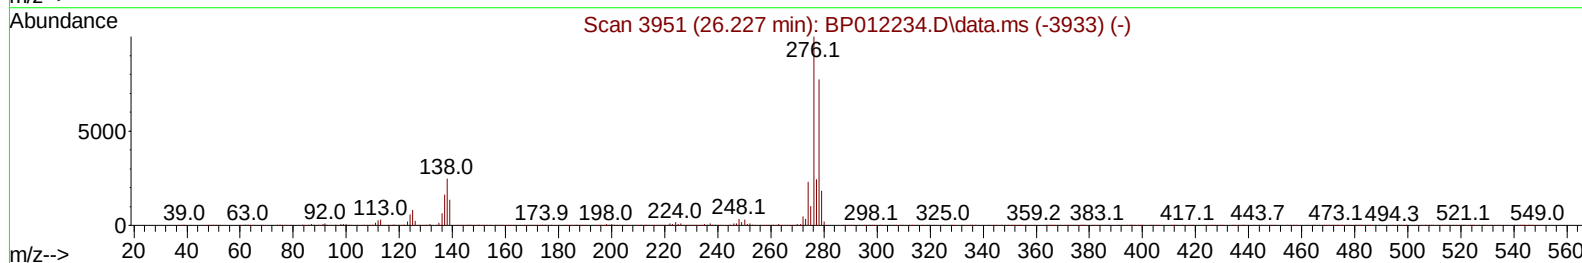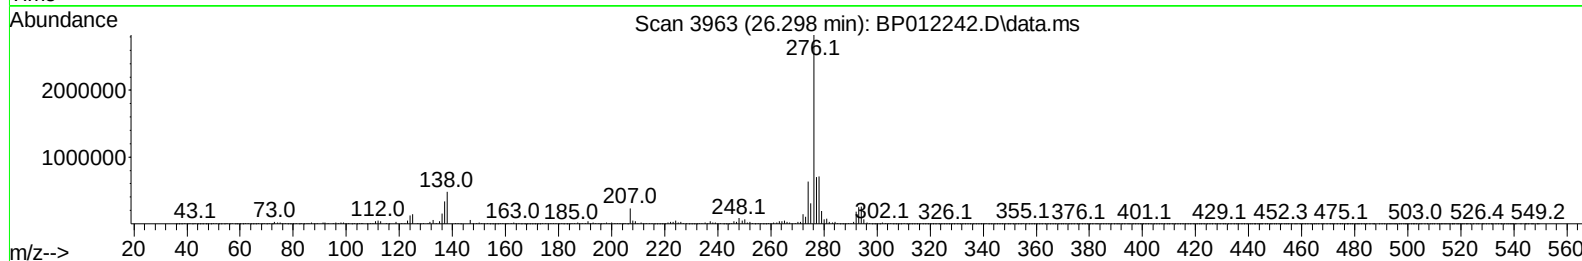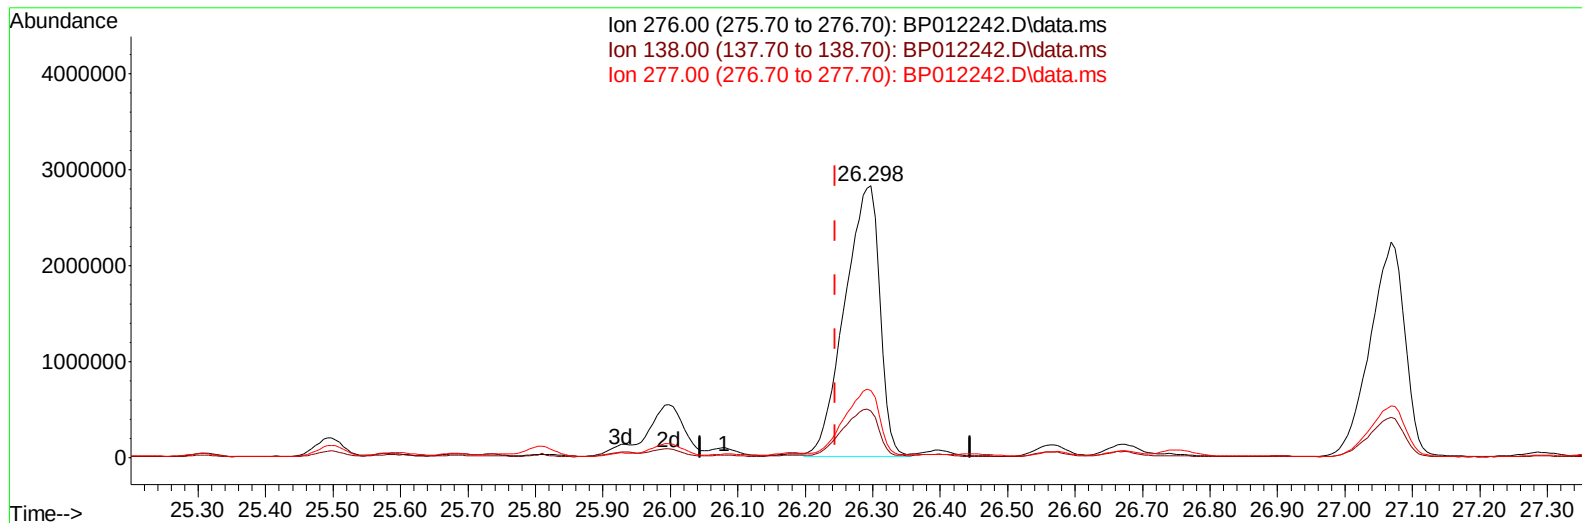

TIC: BP012242.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

26.298min (+ 0.053) 94.82 ng/ul m

response 10228081

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	25.40	17.12#
277.00	25.30	24.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

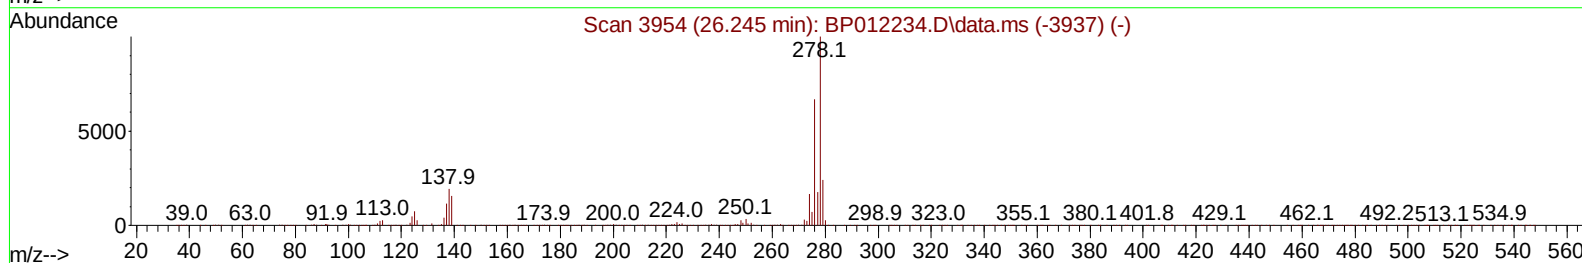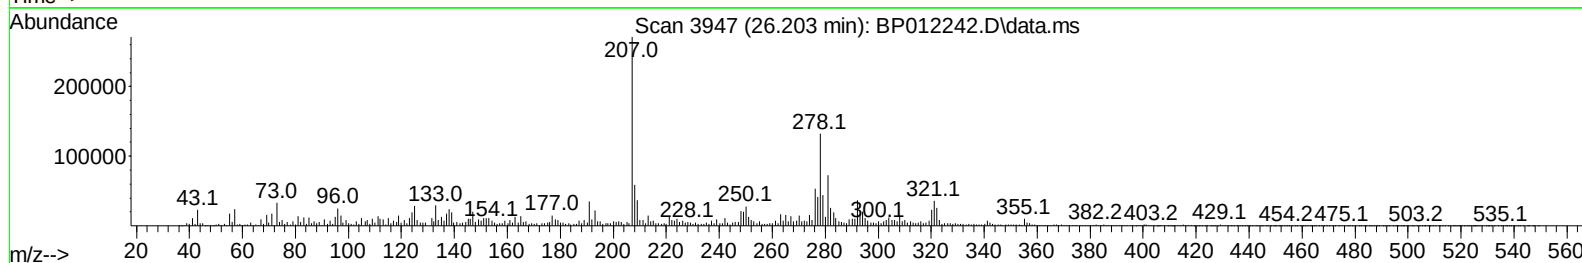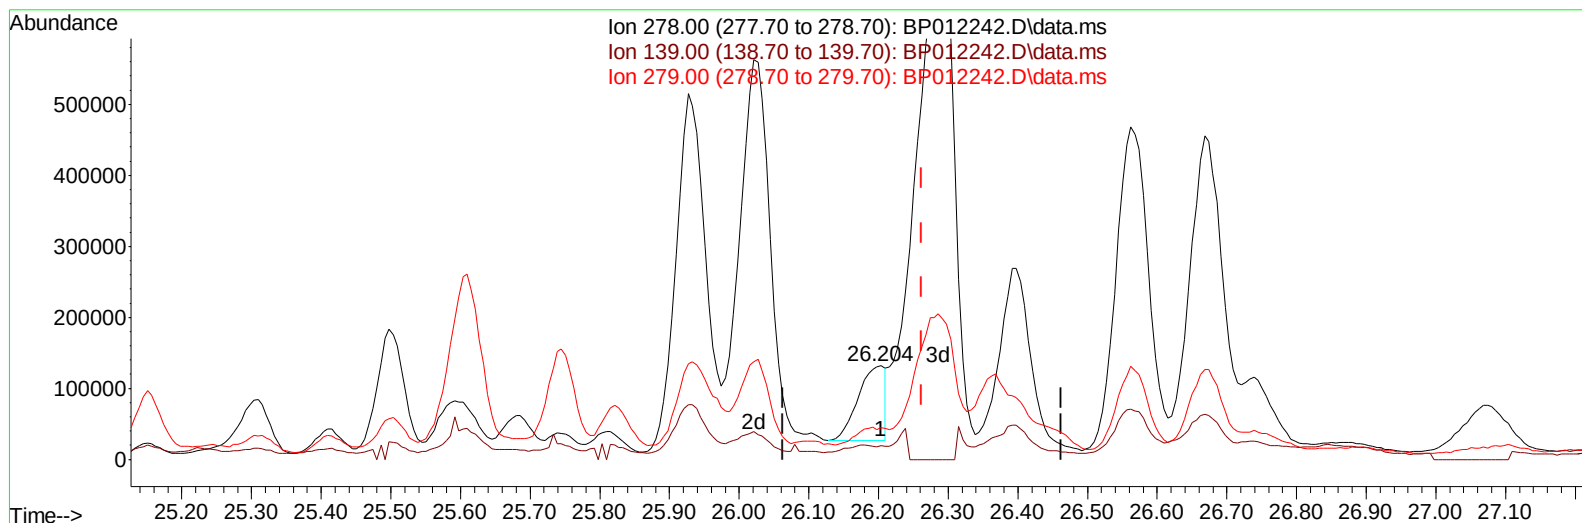

TIC: BP012242.D\data.ms

(95) Dibenzo(a,h)anthracene

26.203min (-0.059) 2.94 ng/u1

response 285977

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	16.10	18.29
279.00	23.70	33.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

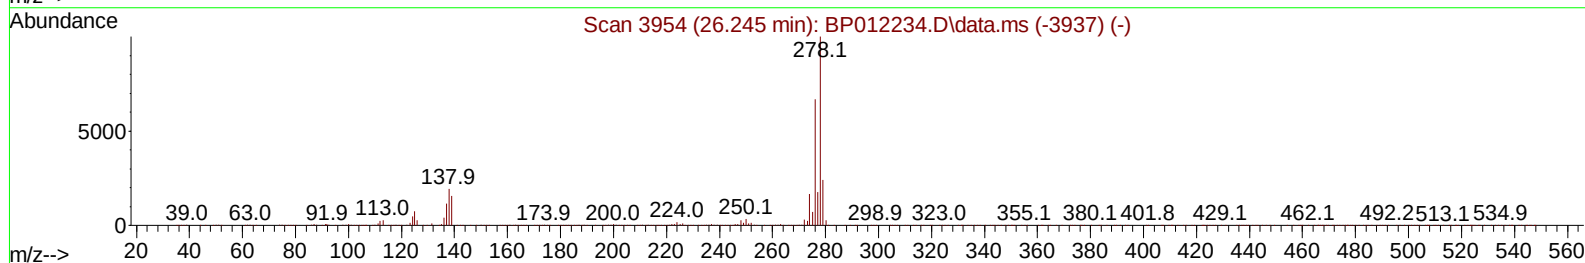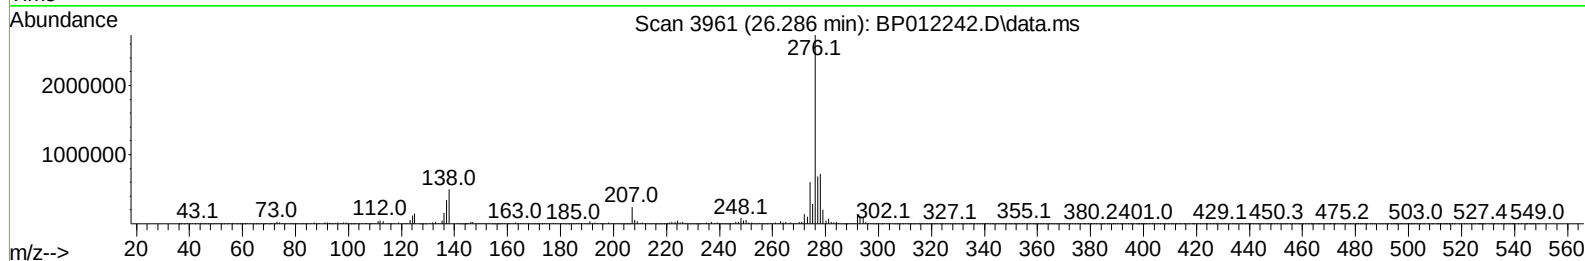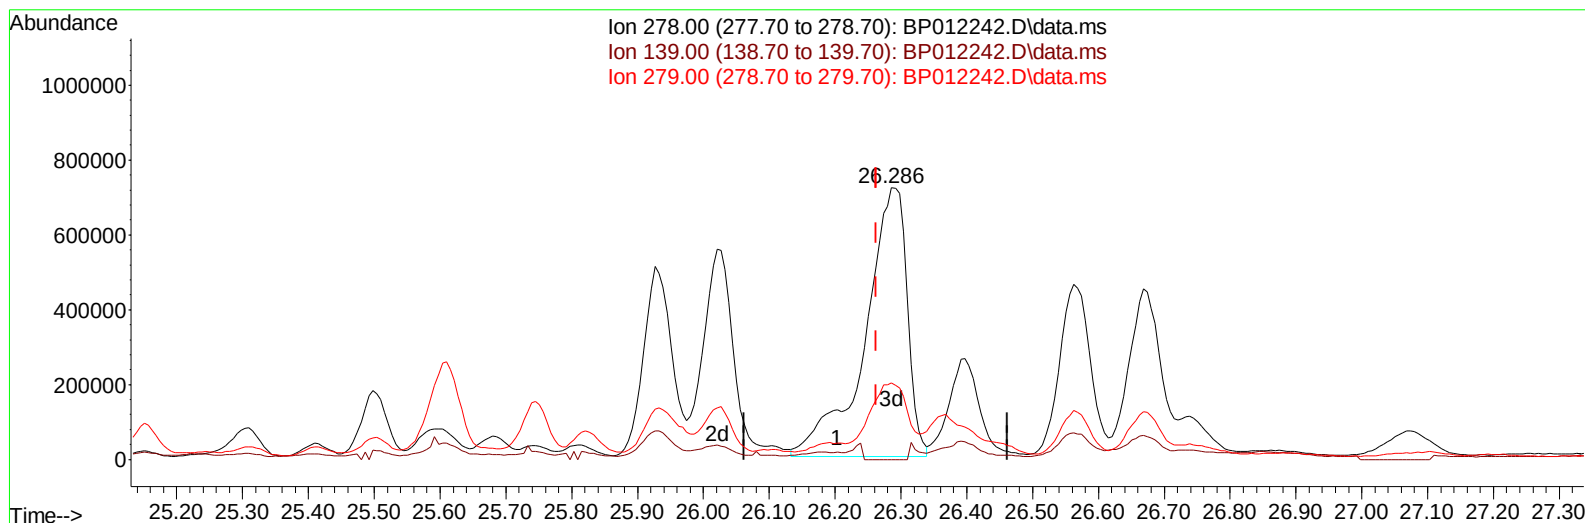

TIC: BP012242.D\data.ms

(95) Dibenzo(a,h)anthracene

26.286min (+ 0.024) 32.75 ng/ul m

response 3185231

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	16.10	0.00#
279.00	23.70	28.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

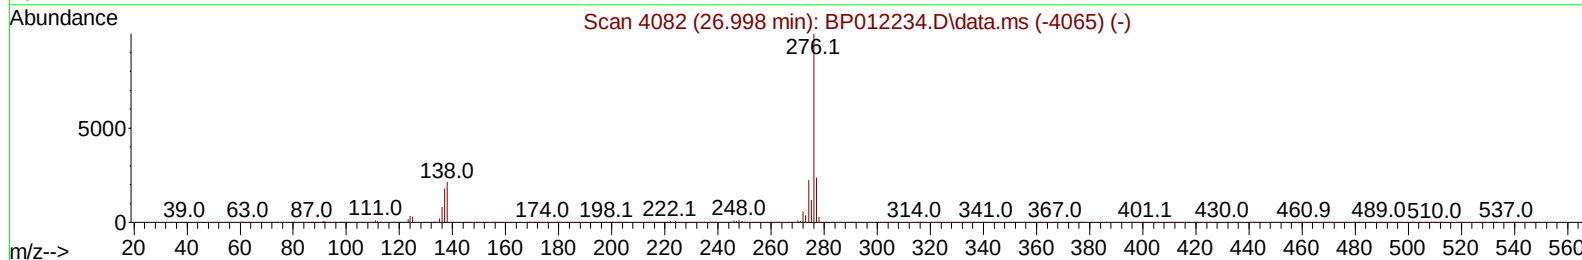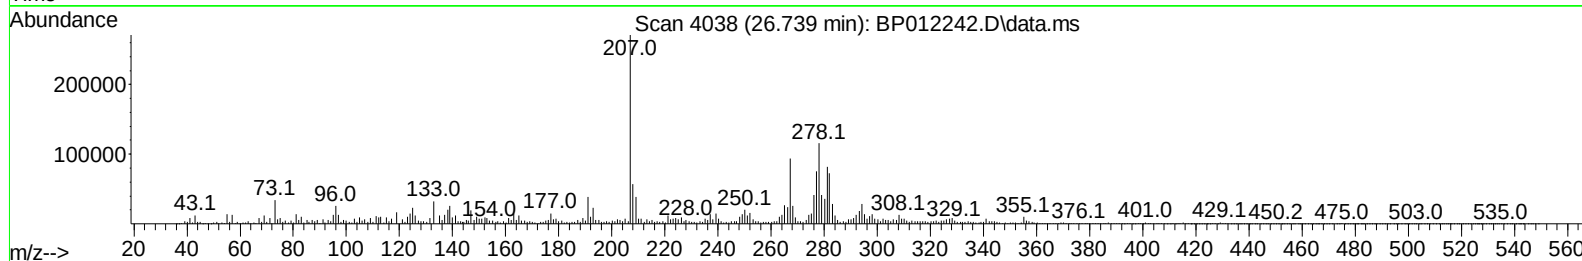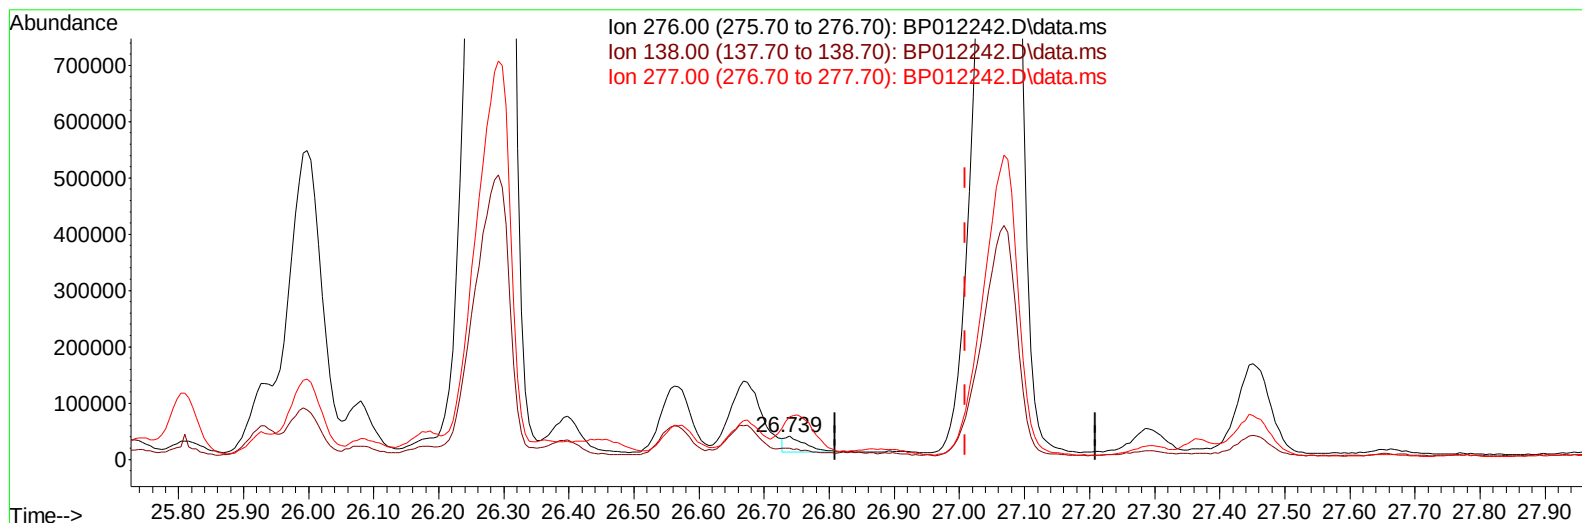

TIC: BP012242.D\data.ms

(96) Benzo(g,h,i)perylene

26.739min (-0.271) 0.61 ng/u1

response 61412

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.40	49.42#
277.00	23.60	182.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012242.D
Acq On : 21 Oct 2022 13:13
Operator : CG/JU
Sample : N4755-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWK5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 22:31:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/24/2022
Supervised By :mohammad ahmed 10/24/2022

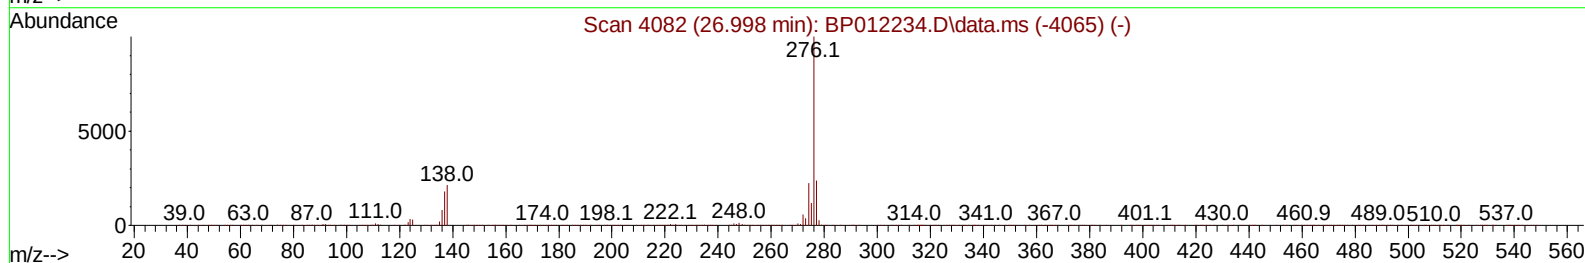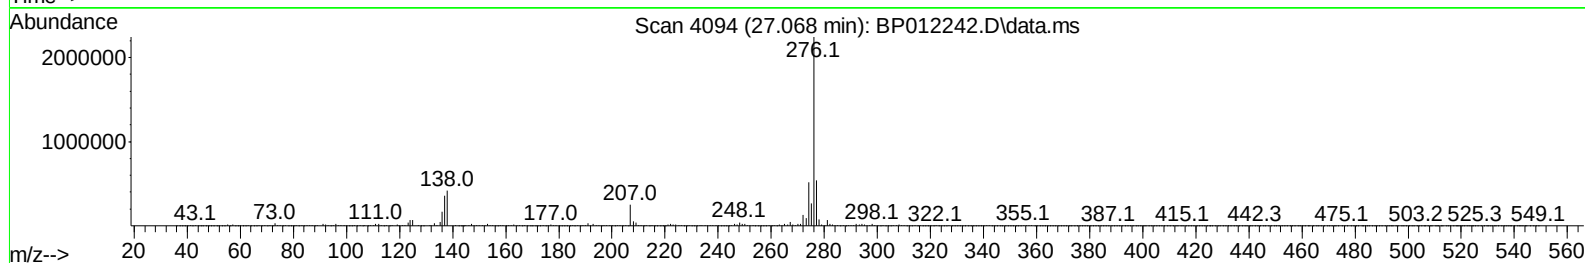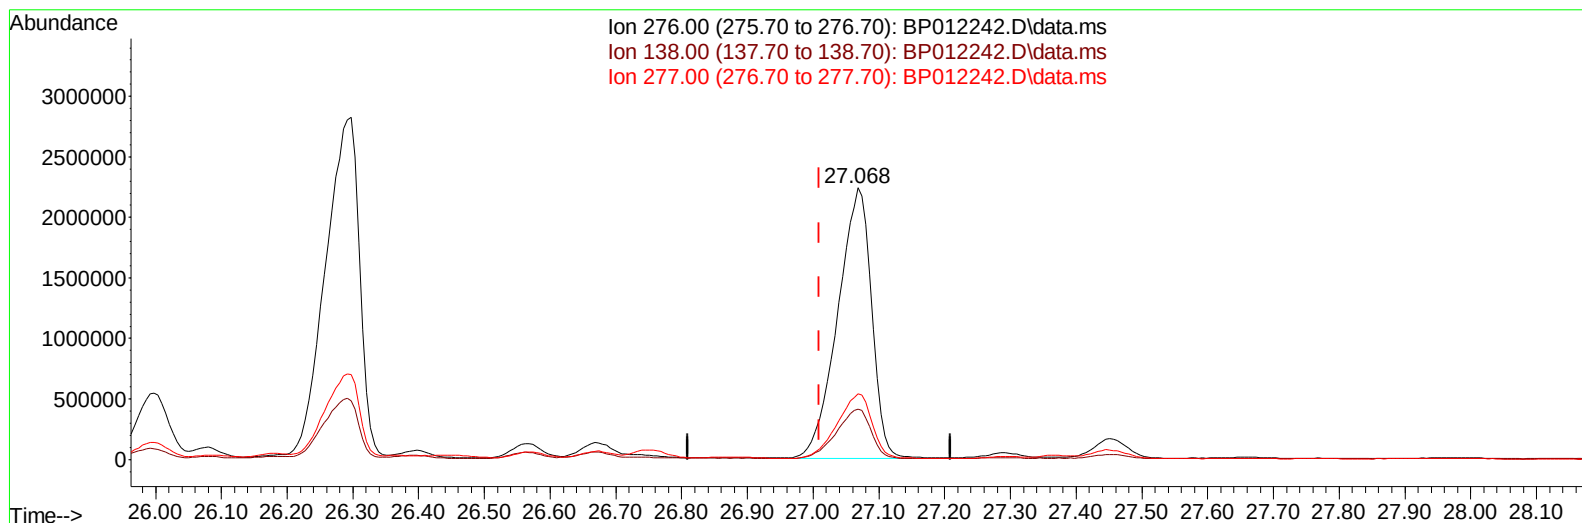

TIC: BP012242.D\data.ms

(96) Benzo(g,h,i)perylene

27.068min (+ 0.059) 79.45 ng/ul m

response 8046582

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.40	18.51
277.00	23.60	24.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	414009	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	1720678	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.475	164	974049	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	1550613	20.000	ng/ul	0.00
79) Chrysene-d12	21.339	240	1164982	20.000	ng/ul	0.00
88) Perylene-d12	23.757	264	1635014m	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	31790	3.108	ng/uL	0.00
4) Pyridine-d5	3.687	84	224464	7.615	ng/ul	0.00
7) Phenol-d5	6.993	99	727740	20.361	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	397762	18.350	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	570669	20.976	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	573161	20.633	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	276023	21.672	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	311819	22.692	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	564852	21.914	ng/ul	0.00
31) 4-Chloroaniline-d4	10.775	131	465108	12.700	ng/ul	0.00
46) Dimethylphthalate-d6	13.887	166	1541644	22.753	ng/ul	0.00
49) Acenaphthylene-d8	14.169	160	1739137	22.487	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143	195082	15.368	ng/ul	0.00
60) Fluorene-d10	15.475	176	1239335	21.261	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	114665	12.999	ng/ul	0.00
73) Anthracene-d10	17.357	188	1223089	17.995	ng/ul	0.02
81) Pyrene-d10	19.580	212	1395524	21.040	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.610	264	1681026m	20.502	ng/ul	0.02
Target Compounds						
					Qvalue	
30) Naphthalene	10.681	128	4393154	47.738	ng/ul	100
36) 2-Methylnaphthalene	12.292	142	2885960	46.092	ng/ul	99
37) 1-Methylnaphthalene	12.510	142	303639	4.857	ng/ul	99
50) Acenaphthylene	14.198	152	2220874	25.772	ng/ul	100
52) Acenaphthene	14.539	153	1322076	21.693	ng/ul	99
61) Fluorene	15.533	166	8867847	134.161	ng/ul	99
71) Pentachlorophenol	16.892	266	267088	22.864	ng/ul	99
72) Phenanthrene	17.292	178	17638723	211.649	ng/ul	94
74) Anthracene	17.386	178	37936156m	460.068	ng/ul	
80) Fluoranthene	19.263	202	15383297m	187.690	ng/ul	
82) Pyrene	19.616	202	15768533m	188.044	ng/ul	
85) Benzo(a)anthracene	21.327	228	7593012	100.005	ng/ul	94
87) Chrysene	21.386	228	12375014	174.658	ng/ul	96
90) Benzo(b)fluoranthene	23.039	252	22199393m	203.732	ng/ul	
91) Benzo(k)fluoranthene	23.074	252	5387510m	50.160	ng/ul	
93) Benzo(a)pyrene	23.668	252	10794414m	115.847	ng/ul	
94) Indeno(1,2,3-cd)pyrene	26.298	276	10228081m	94.823	ng/ul	
95) Dibenzo(a,h)anthracene	26.286	278	3185231m	32.755	ng/ul	
96) Benzo(g,h,i)perylene	27.068	276	8046582m	79.450	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012242.D
 Acq On : 21 Oct 2022 13:13
 Operator : CG/JU
 Sample : N4755-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWK5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/24/2022
 Supervised By :mohammad ahmed 10/24/2022

Quant Time: Oct 21 22:31:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

