
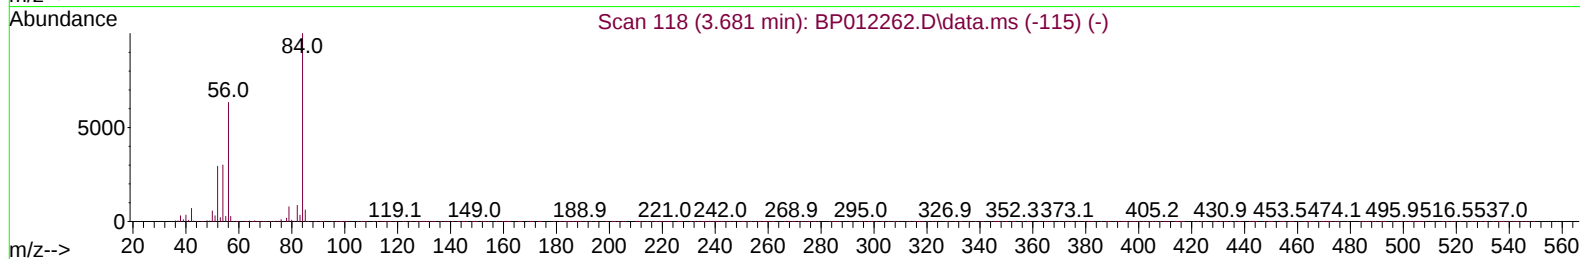
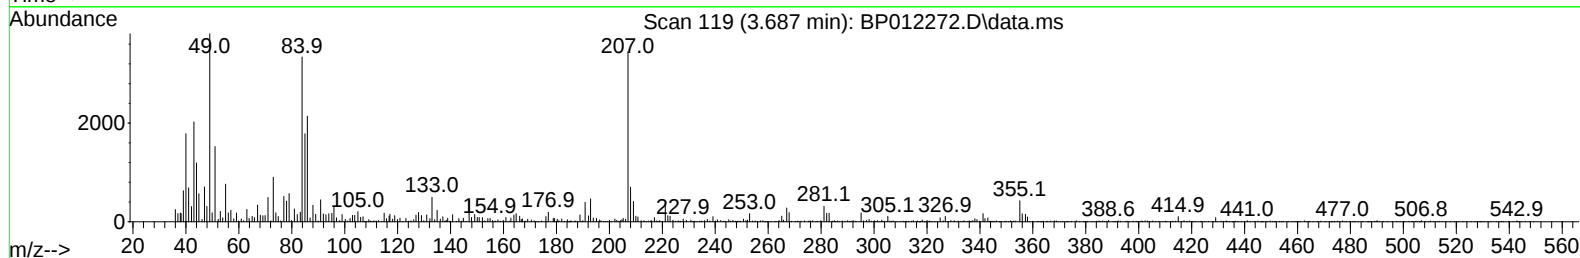


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 25 17:55:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

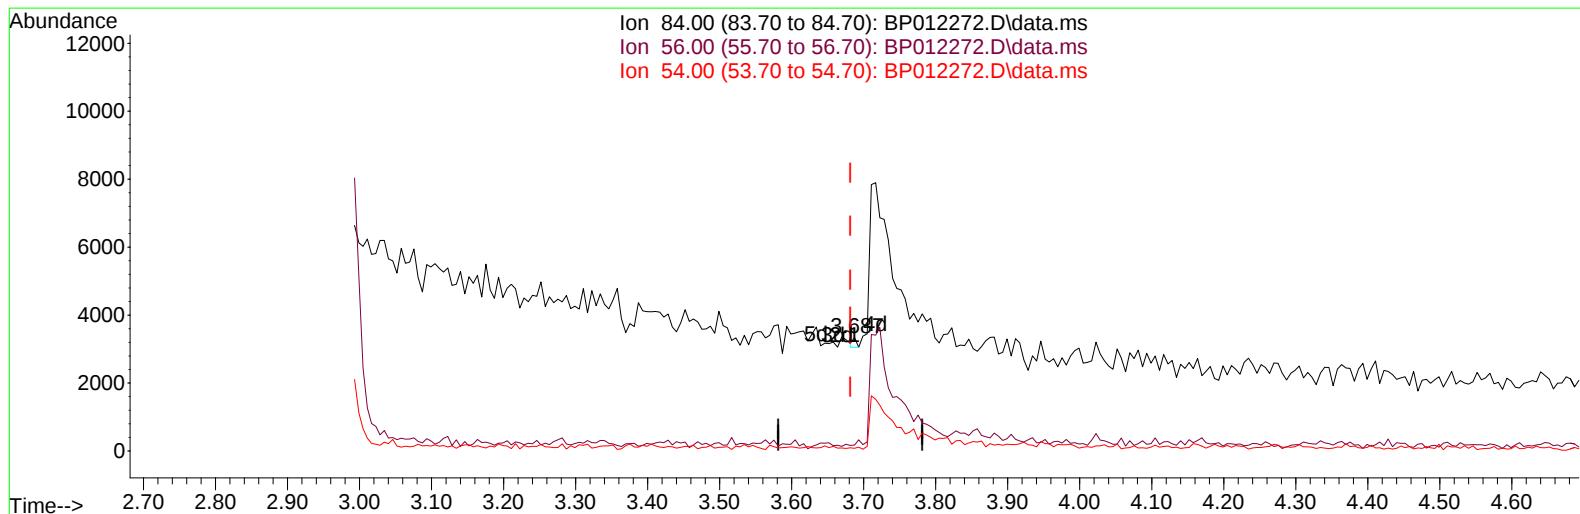

TIC: BP012272.D\data.ms

(4) Pyridine-d5 (S)




3.687min (+ 0.006) 0.00 ng/u1

response 101

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	63.60	5.30#
54.00	29.70	2.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 22 10:19:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

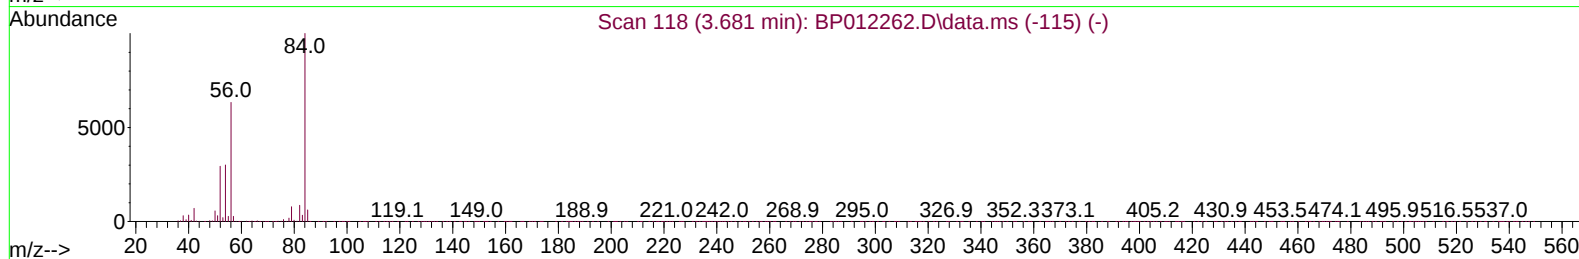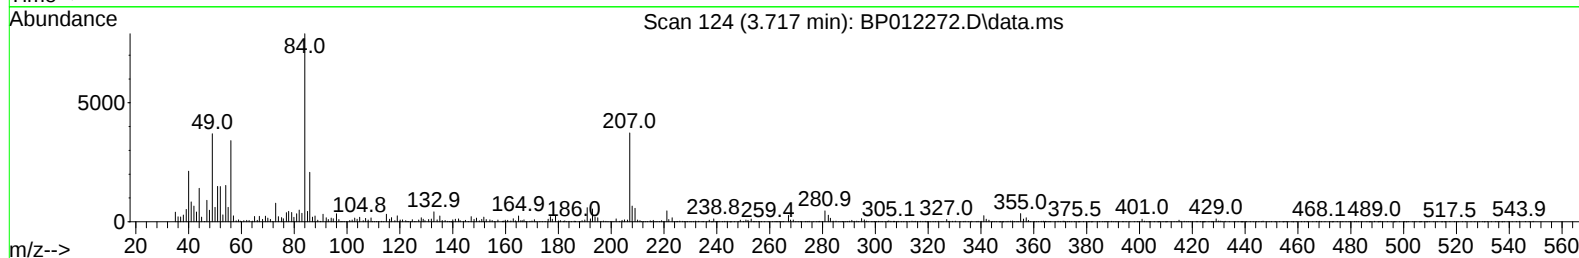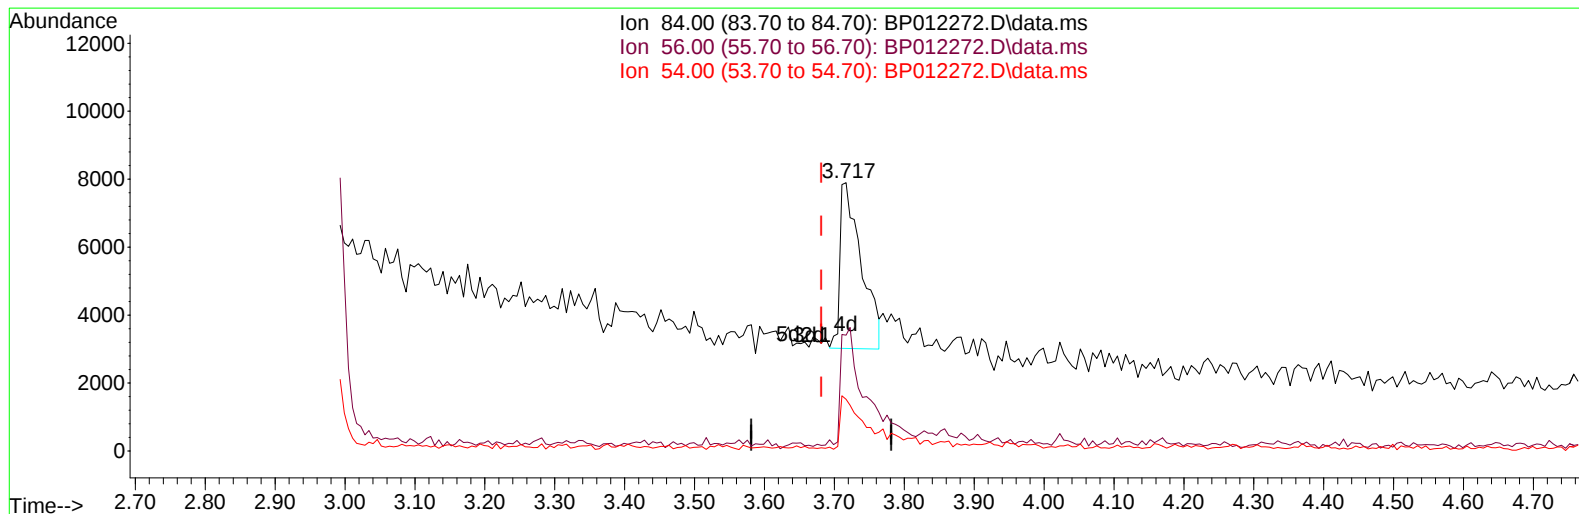

TIC: BP012272.D\data.ms

(4) Pyridine-d5 (S)




3.717min (+ 0.035) 0.39 ng/ul m

response 10322

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	63.60	43.17#
54.00	29.70	19.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 25 17:55:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

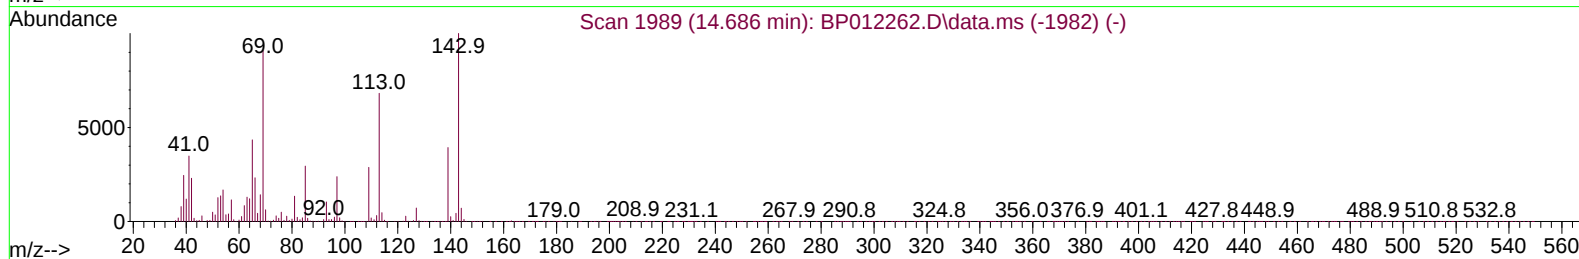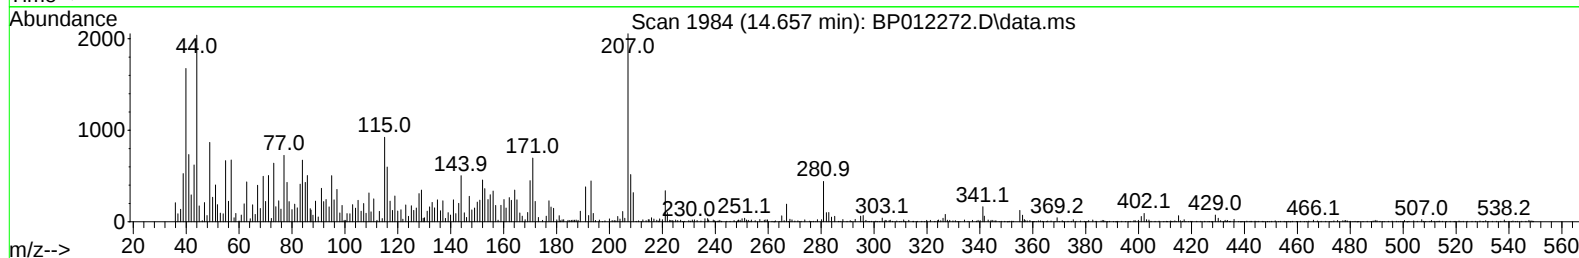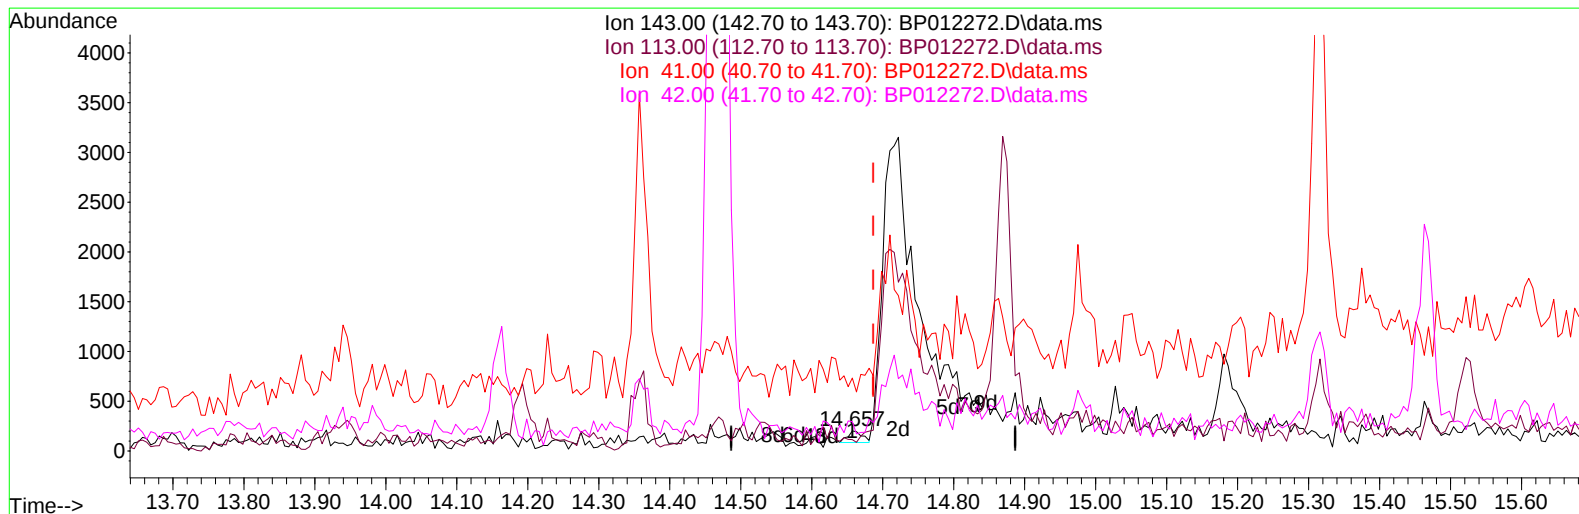

TIC: BP012272.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.657min (-0.029) 0.02 ng/u1

response 168

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	56.72
41.00	35.10	365.17#
42.00	23.90	146.27#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 22 10:19:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

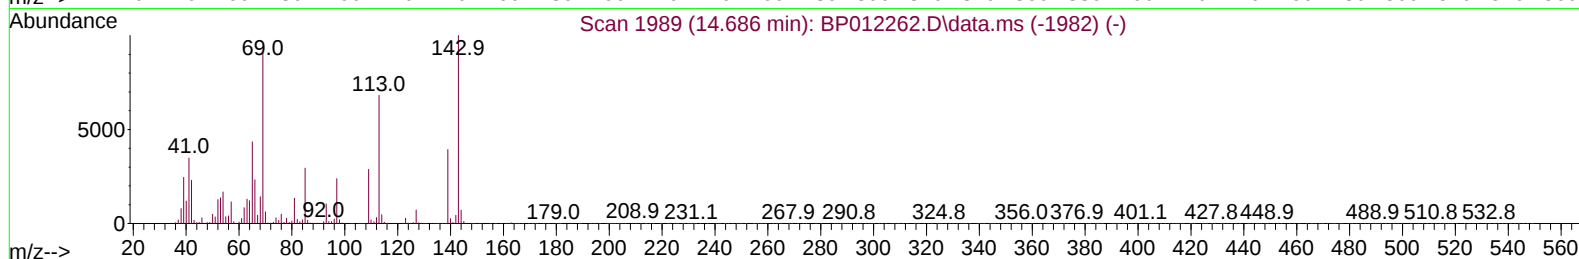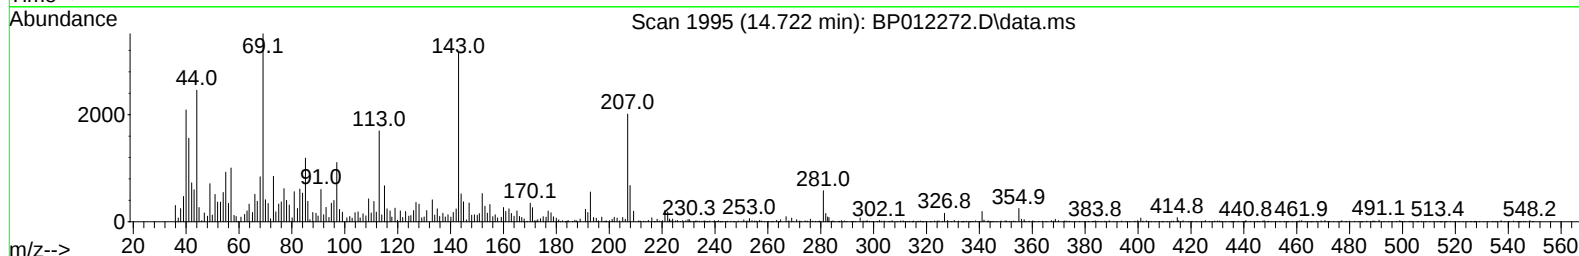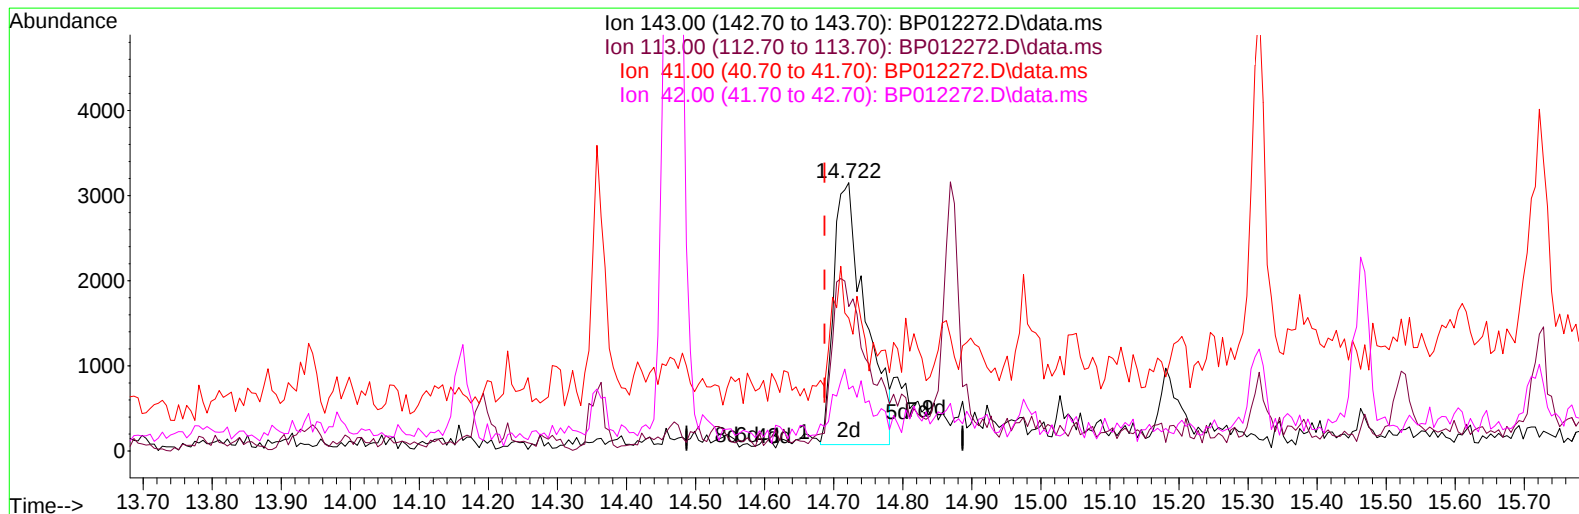

TIC: BP012272.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.722min (+ 0.035) 0.90 ng/u1 m

response 9786

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.20	53.84
41.00	35.10	49.52#
42.00	23.90	23.06

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\  
Data File : BP012272.D  
Acq On    : 22 Oct 2022 06:56  
Operator  : CG/JU  
Sample    : N4755-08DL 10X  
Misc      :  
ALS Vial  : 68    Sample Multiplier: 1
```

Quant Time: Oct 25 17:55:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

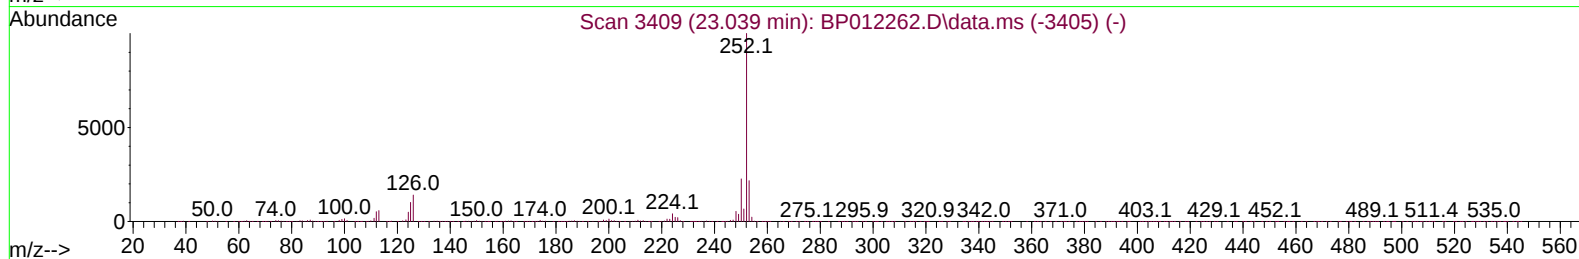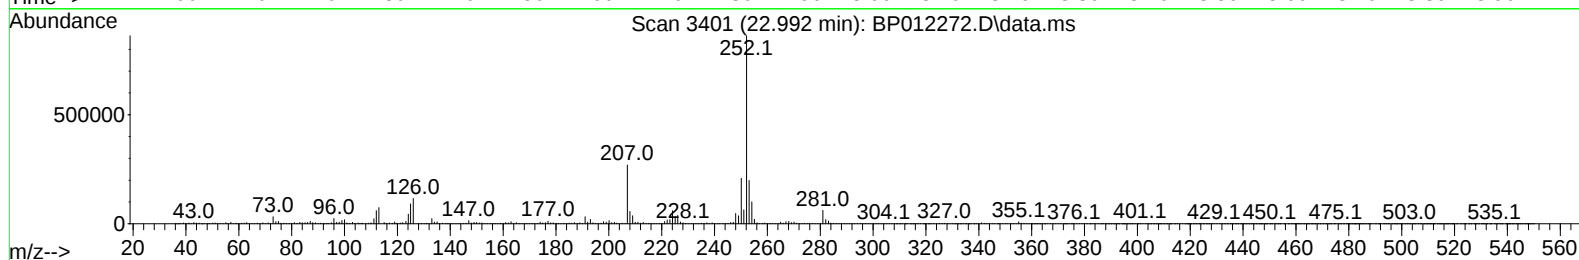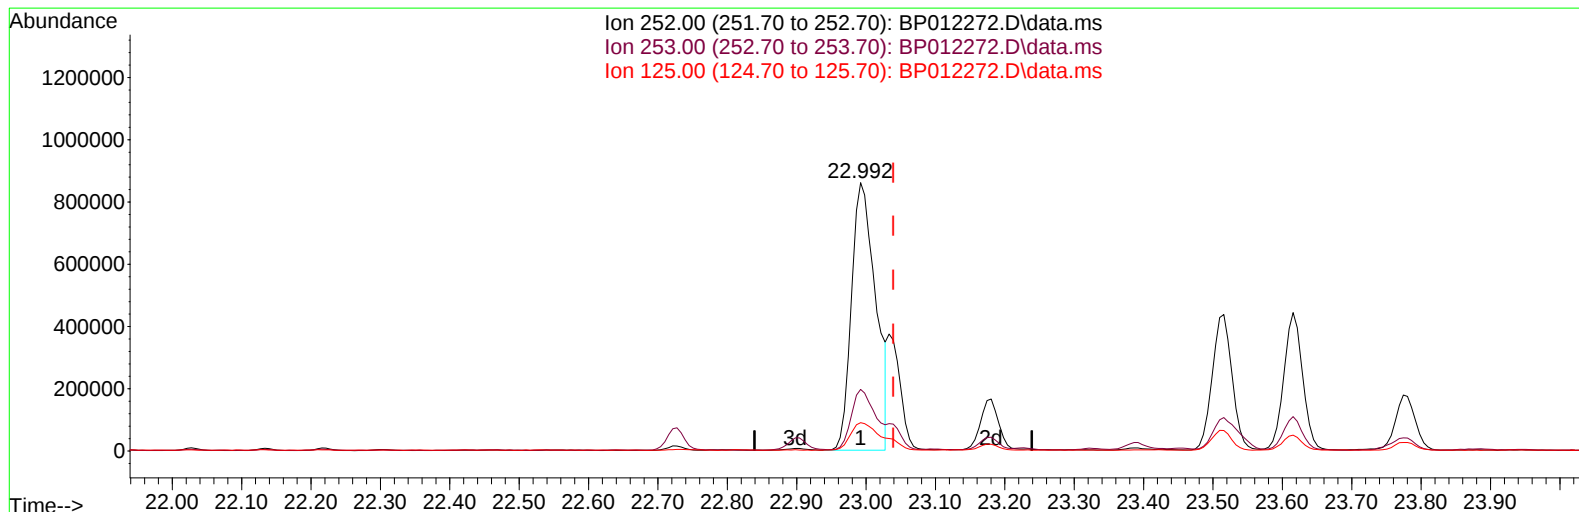

TIC: BP012272.D\data.ms

(91) Benzo(k)fluoranthene




22.992min (-0.047) 16.84 ng/ul

response 2087749

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	22.94
125.00	10.80	10.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 22 10:19:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

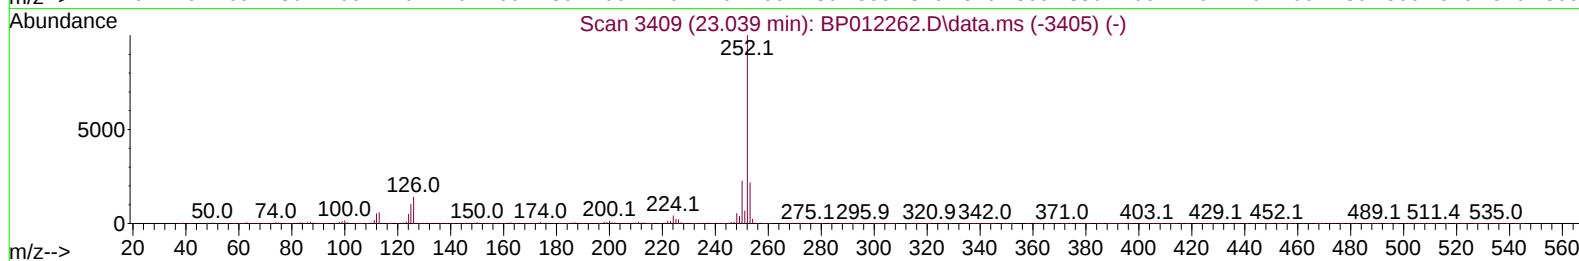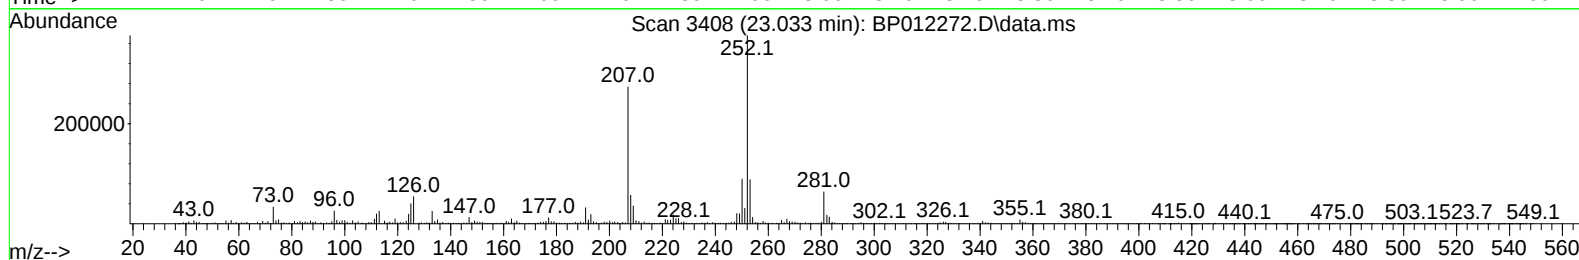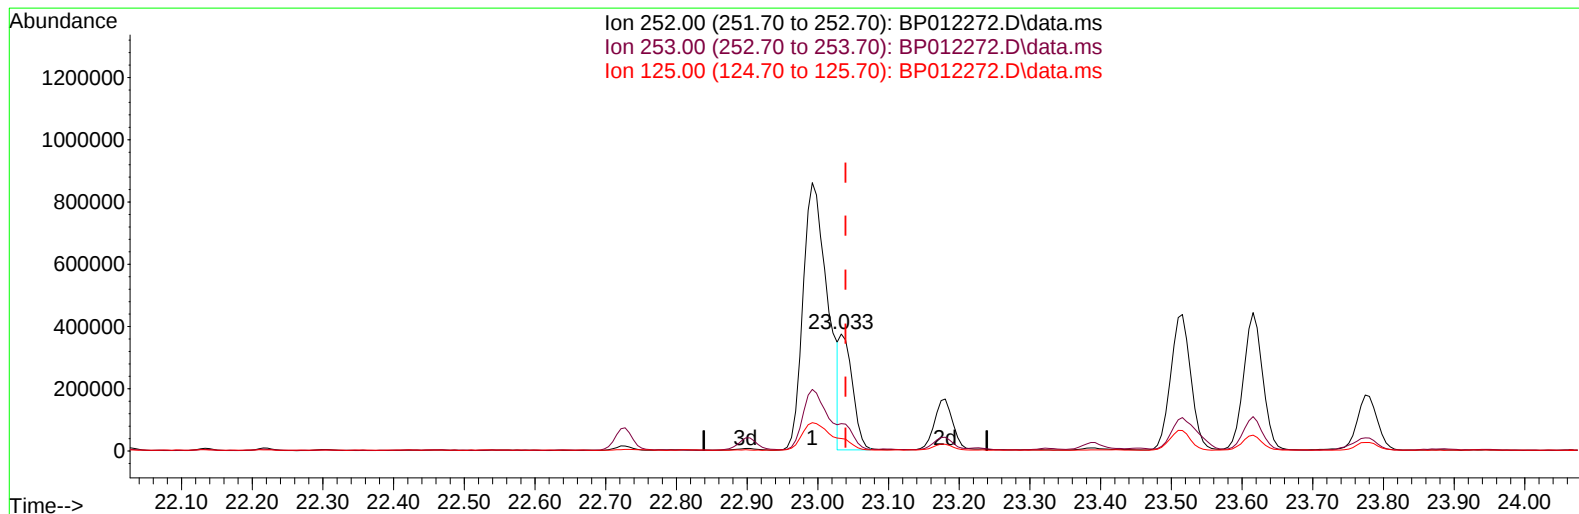

TIC: BP012272.D\data.ms

(91) Benzo(k)fluoranthene

23.033min (-0.006) 3.79 ng/u1 m

response 470188

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.40	23.40
125.00	10.80	10.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012272.D
 Acq On : 22 Oct 2022 06:56
 Operator : CG/JU
 Sample : N4755-08DL 10X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 22 10:19:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 22 01:24:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	370899	20.000	ng/u1	0.00
20) Naphthalene-d8	10.622	136	1466723	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.469	164	834336	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	1660141	20.000	ng/u1	0.00
79) Chrysene-d12	21.322	240	1681423	20.000	ng/u1	0.00
88) Perylene-d12	23.727	264	1887289	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	3040	0.332	ng/uL	0.00
4) Pyridine-d5	3.717	84	10322m	0.391	ng/u1	0.04
7) Phenol-d5	6.993	99	59991	1.874	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.158	67	34453	1.774	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	49161	2.017	ng/u1	0.00
15) 4-Methylphenol-d8	8.540	113	41121	1.652	ng/u1	0.00
21) Nitrobenzene-d5	8.987	128	19648	1.810	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	21196	1.810	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	41809	1.903	ng/u1	0.00
31) 4-Chloroaniline-d4	10.781	131	27580	0.883	ng/u1	0.01
46) Dimethylphthalate-d6	13.887	166	139943	2.411	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	152135	2.296	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	9786m	0.900	ng/u1	0.04
60) Fluorene-d10	15.469	176	127161	2.547	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	7247	0.767	ng/u1	0.00
73) Anthracene-d10	17.328	188	194316	2.670	ng/u1	0.00
81) Pyrene-d10	19.569	212	226407	2.365	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.568	264	240373	2.540	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.675	128	118999	1.517	ng/u1	97
50) Acenaphthylene	14.193	152	259219	3.512	ng/u1	100
61) Fluorene	15.522	166	57598	1.017	ng/u1	99
72) Phenanthrene	17.269	178	352489	3.951	ng/u1	99
74) Anthracene	17.363	178	1513724	17.146	ng/u1	100
80) Fluoranthene	19.245	202	1808518	15.288	ng/u1	96
82) Pyrene	19.598	202	3244438	26.807	ng/u1	96
85) Benzo(a)anthracene	21.304	228	849155	7.749	ng/u1	98
87) Chrysene	21.357	228	1185137	11.589	ng/u1	99
90) Benzo(b)fluoranthene	22.992	252	2087749	16.599	ng/u1	99
91) Benzo(k)fluoranthene	23.033	252	470188m	3.792	ng/u1	
93) Benzo(a)pyrene	23.616	252	824281	7.664	ng/u1	96
94) Indeno(1,2,3-cd)pyrene	26.215	276	955437	7.674	ng/u1	94
95) Dibenzo(a,h)anthracene	26.221	278	225070	2.005	ng/u1#	80
96) Benzo(g,h,i)perylene	26.986	276	773035	6.612	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012272.D
Acq On : 22 Oct 2022 06:56
Operator : CG/JU
Sample : N4755-08DL 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Oct 22 10:19:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 22 01:24:49 2022
Response via : Initial Calibration

