

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012226.D
 Acq On : 20 Oct 2022 22:15
 Operator : CG/JU
 Sample : N5103-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BX1

Quant Time: Oct 20 23:27:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 00:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	418588	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	1766938	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.475	164	1030555	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.234	188	1851171	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	1498349	20.000	ng/u1	0.00
88) Perylene-d12	23.733	264	1688826	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	40371	3.903	ng/uL	0.00
4) Pyridine-d5	3.687	84	163282	5.479	ng/u1	0.00
7) Phenol-d5	6.993	99	196310	5.432	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.158	67	603766	27.549	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	598803	21.769	ng/u1	0.00
15) 4-Methylphenol-d8	8.540	113	362807	12.918	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	411798	31.485	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	428733	30.383	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	668705	25.264	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	623514	16.580	ng/u1	0.00
46) Dimethylphthalate-d6	13.887	166	2194872	30.618	ng/u1	0.00
49) Acenaphthylene-d8	14.169	160	2480758	30.317	ng/u1	0.00
54) 4-Nitrophenol-d4	14.698	143	45120	3.360	ng/u1	0.00
60) Fluorene-d10	15.469	176	1845412	29.923	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	235481	22.361	ng/u1	0.00
73) Anthracene-d10	17.334	188	2794901	34.444	ng/u1	0.00
81) Pyrene-d10	19.575	212	2847101	33.374	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.580	264	3000195	35.425	ng/u1	0.00
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.233	149	79149	1.347	ng/u1#	98
96) Benzo(g,h,i)perylene	26.998	276	117561	1.124	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012226.D
Acq On : 20 Oct 2022 22:15
Operator : CG/JU
Sample : N5103-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX1

Quant Time: Oct 20 23:27:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 00:51:41 2022
Response via : Initial Calibration




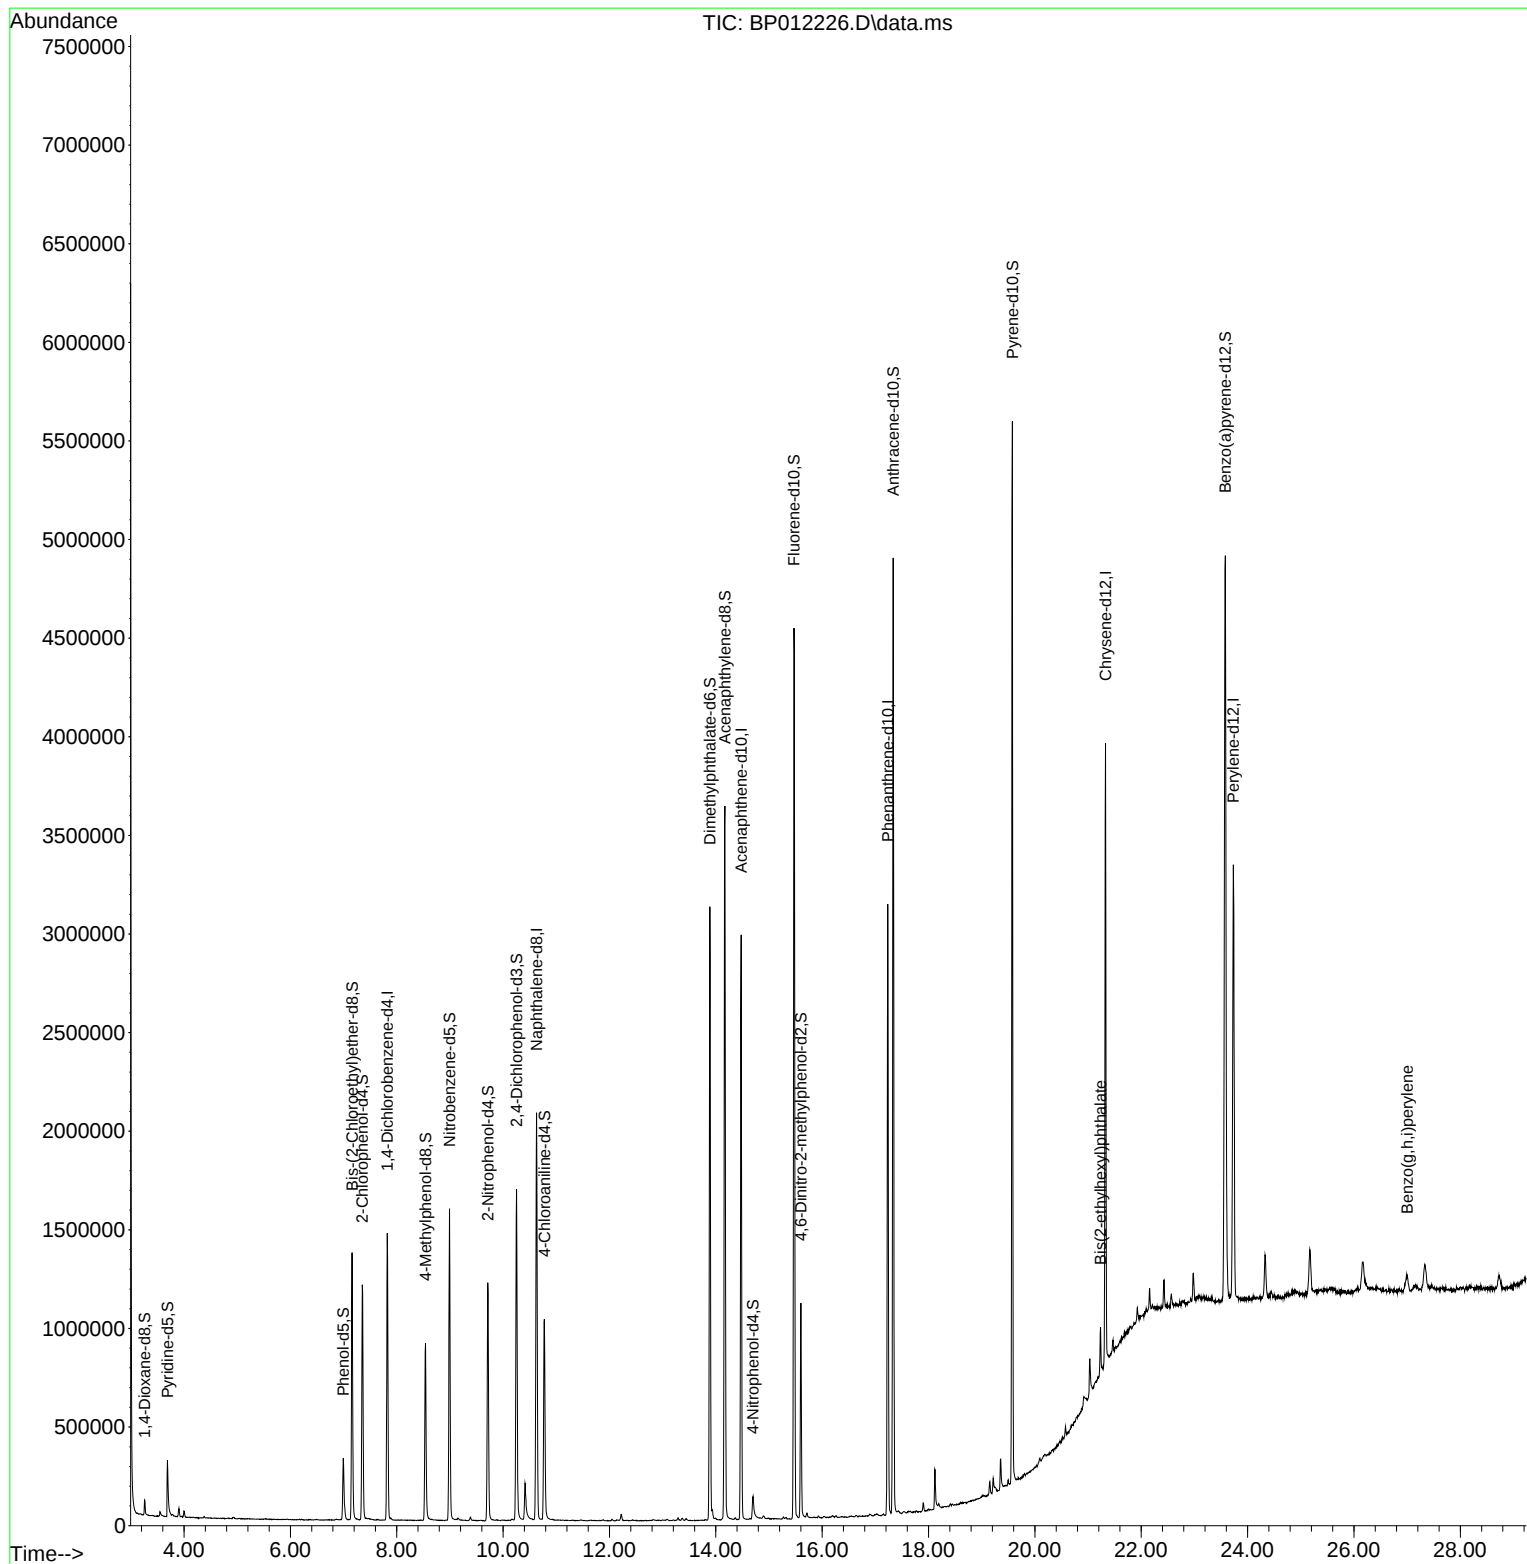


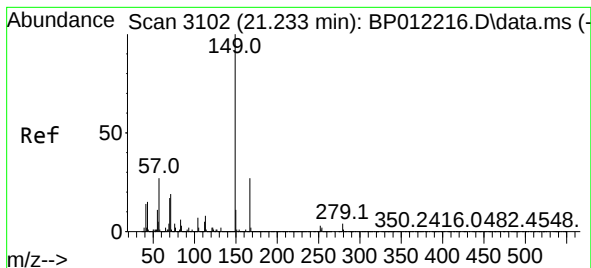

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.347 ng/ul
RT: 21.233 min Scan# 3102
Delta R.T. -0.006 min
Lab File: BP012226.D
Acq: 20 Oct 2022 22:15

Instrument :
BNA_P
ClientSampleId :
C0BX1

Tgt Ion:149 Resp: 79149
Ion Ratio Lower Upper
149 100
167 27.7 21.6 32.4
279 5.3 3.4 5.0#

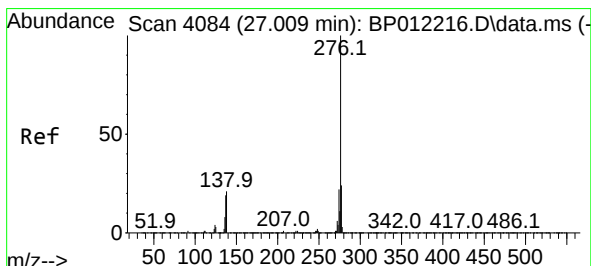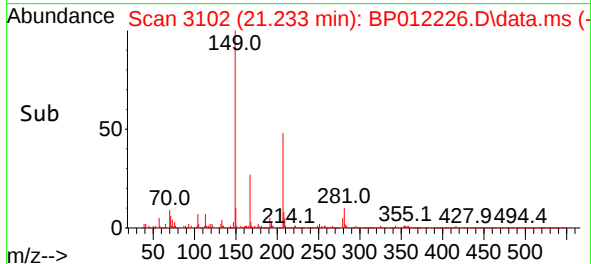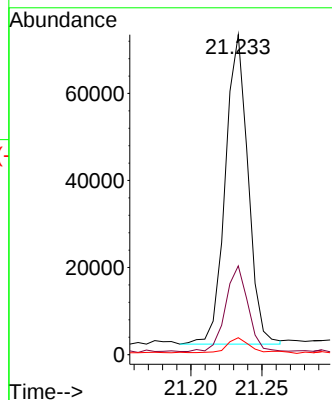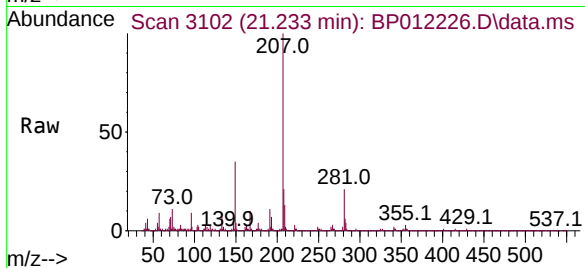

#96
Benzo(g,h,i)perylene
Concen: 1.124 ng/ul
RT: 26.998 min Scan# 4082
Delta R.T. -0.012 min
Lab File: BP012226.D
Acq: 20 Oct 2022 22:15

Tgt Ion:276 Resp: 117561
Ion Ratio Lower Upper
276 100
138 21.4 17.9 26.9
277 23.1 18.9 28.3

