

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012208.D
 Acq On : 20 Oct 2022 09:59
 Operator : CG/JU
 Sample : PB148325BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	43	46	57	rVB	104718	139549	1.47%	0.147%
2	3.681	114	118	140	rBV	1110047	1731349	18.22%	1.820%
3	3.999	167	172	180	rVB	32555	50964	0.54%	0.054%
4	6.993	674	681	693	rBV	1429844	2317636	24.40%	2.436%
5	7.158	703	709	724	rVB	1227041	2000356	21.06%	2.103%
6	7.352	735	742	756	rBV	1410961	2359218	24.83%	2.480%
7	7.822	815	822	838	rBV	1259623	2063065	21.72%	2.169%
8	8.540	935	944	960	rBV	1789124	2981960	31.39%	3.135%
9	8.993	1013	1021	1037	rBV	1408229	2340616	24.64%	2.461%
10	9.716	1136	1144	1158	rBV	1105022	1900475	20.00%	1.998%
11	10.252	1222	1235	1252	rBV	1706703	3027935	31.87%	3.183%
12	10.628	1291	1299	1314	rVB	1846853	3156467	33.23%	3.318%
13	10.775	1316	1324	1341	rBV	1619840	2980584	31.37%	3.133%
14	12.234	1565	1572	1585	rBV2	23449	57058	0.60%	0.060%
15	13.451	1774	1779	1784	rBV7	7085	12363	0.13%	0.013%
16	13.893	1846	1854	1866	rBV	3352228	4879255	51.36%	5.129%
17	14.169	1893	1901	1918	rBV	3924004	5761663	60.65%	6.057%
18	14.475	1946	1953	1968	rBV	3085620	4478496	47.14%	4.708%
19	14.687	1982	1989	2011	rBV	1300584	2247139	23.65%	2.362%
20	14.887	2021	2023	2032	rVB10	11198	18763	0.20%	0.020%
21	15.475	2115	2123	2137	rBV	5151560	7487787	78.82%	7.871%
22	15.598	2138	2144	2159	rVV	1450210	2126778	22.39%	2.236%
23	15.710	2159	2163	2172	rVB3	28769	54583	0.57%	0.057%
24	16.910	2361	2367	2373	rBV10	11531	22389	0.24%	0.024%
25	17.022	2380	2386	2392	rBV5	10807	25338	0.27%	0.027%
26	17.234	2416	2422	2432	rBV	3684296	5406073	56.90%	5.683%
27	17.334	2433	2439	2458	rVB	5641612	8343186	87.82%	8.771%
28	19.151	2744	2748	2755	rBV2	72455	108592	1.14%	0.114%
29	19.222	2757	2760	2764	rVB	55302	76002	0.80%	0.080%
30	19.575	2814	2820	2831	rBV	7228120	9500243	100.00%	9.987%
31	21.327	3113	3118	3128	rBV	4359435	5428272	57.14%	5.706%
32	23.580	3494	3501	3512	rVB2	3728640	7567858	79.66%	7.956%
33	23.733	3521	3527	3541	rVB	2243090	4475189	47.11%	4.704%




Sum of corrected areas: 95127201

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012208.D
Acq On : 20 Oct 2022 09:59
Operator : CG/JU
Sample : PB148325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

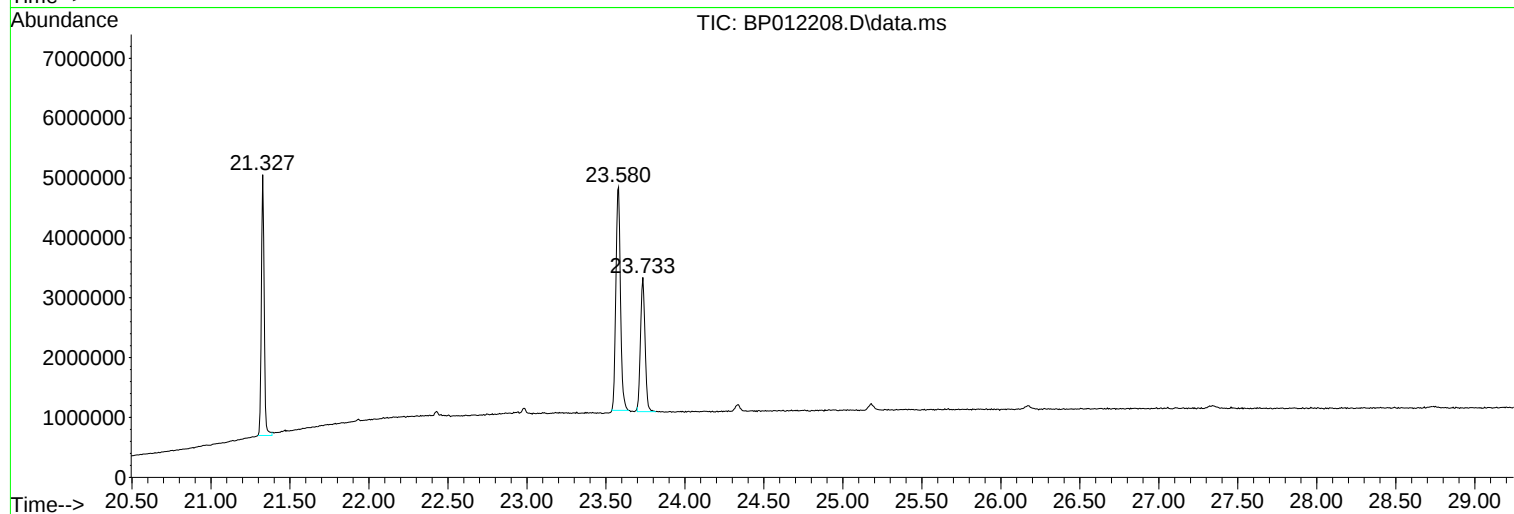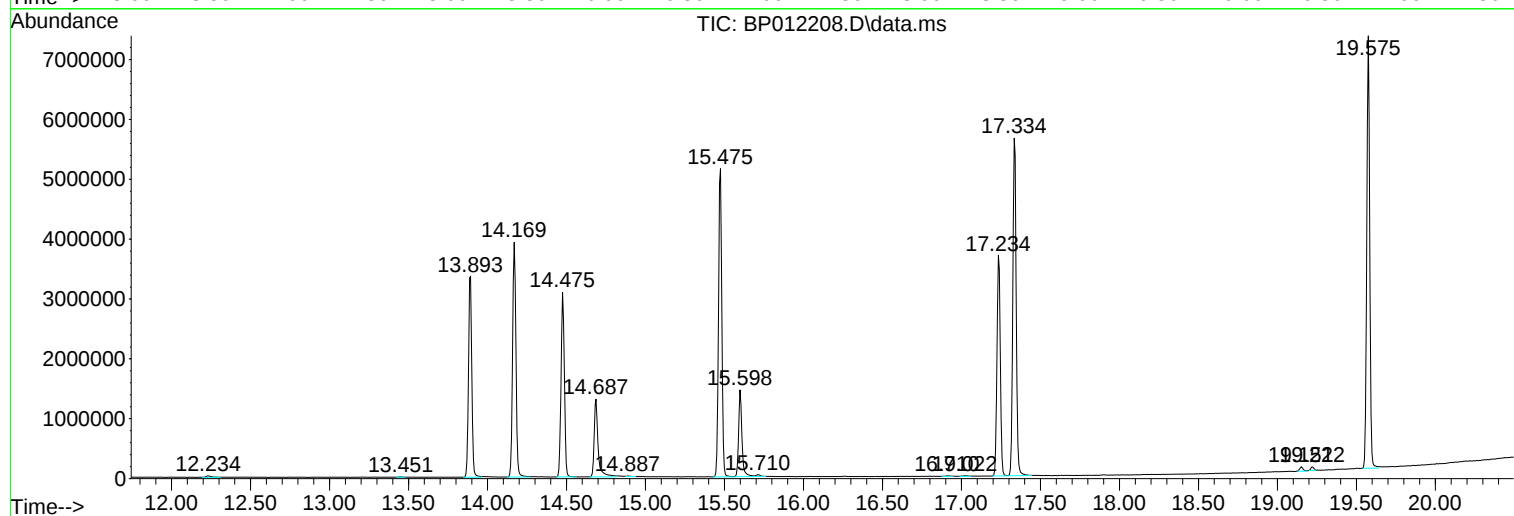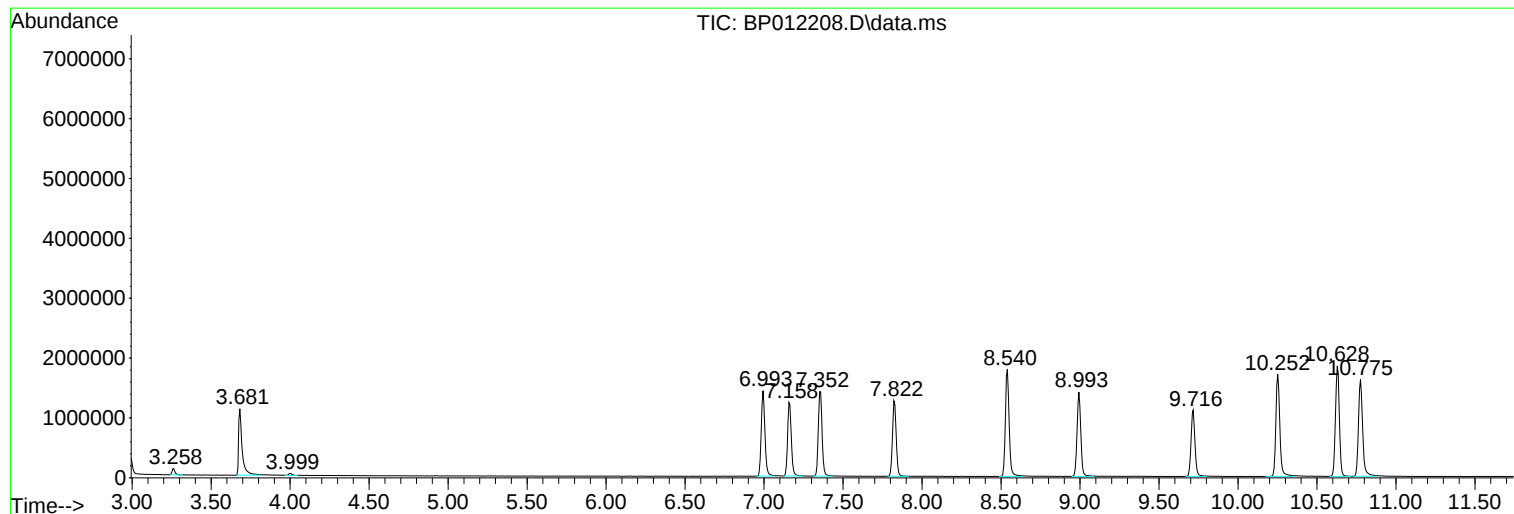

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012208.D
Acq On : 20 Oct 2022 09:59
Operator : CG/JU
Sample : PB148325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012208.D
Acq On : 20 Oct 2022 09:59
Operator : CG/JU
Sample : PB148325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc