

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012209.D
 Acq On : 20 Oct 2022 10:33
 Operator : CG/JU
 Sample : PB148327BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	43	46	53	rVB	117494	154546	1.41%	0.141%
2	3.681	115	118	144	rBV	1302322	2069157	18.90%	1.893%
3	3.999	168	172	178	rVB	34536	45914	0.42%	0.042%
4	6.993	674	681	694	rBV	1663172	2684889	24.52%	2.457%
5	7.164	703	710	723	rVB	1394855	2343101	21.40%	2.144%
6	7.358	735	743	755	rBV	1669158	2728797	24.93%	2.497%
7	7.822	815	822	835	rBV	1351479	2233633	20.40%	2.044%
8	8.540	936	944	958	rBV	2035529	3426475	31.30%	3.135%
9	8.993	1014	1021	1037	rBV	1623264	2710199	24.76%	2.480%
10	9.716	1137	1144	1166	rBV	1306059	2209140	20.18%	2.021%
11	10.252	1224	1235	1253	rBV	1986187	3464361	31.64%	3.170%
12	10.628	1292	1299	1316	rVB	2016821	3399469	31.05%	3.110%
13	10.775	1316	1324	1345	rBV	1898152	3429532	31.33%	3.138%
14	12.234	1565	1572	1579	rBV	24322	56278	0.51%	0.051%
15	13.457	1775	1780	1789	rVB5	6961	13956	0.13%	0.013%
16	13.893	1847	1854	1867	rBV	3830517	5564785	50.83%	5.092%
17	14.169	1893	1901	1923	rBV	4439098	6639685	60.65%	6.075%
18	14.475	1946	1953	1963	rBV	3313118	4738900	43.29%	4.336%
19	14.687	1982	1989	2011	rBV	1613037	2631338	24.04%	2.408%
20	15.475	2115	2123	2135	rBV	5641573	8456611	77.24%	7.738%
21	15.598	2138	2144	2159	rVV	1830610	2642599	24.14%	2.418%
22	15.710	2160	2163	2171	rVB2	31525	56402	0.52%	0.052%
23	16.263	2253	2257	2261	rVB7	7738	11550	0.11%	0.011%
24	16.910	2363	2367	2371	rVB7	8578	13952	0.13%	0.013%
25	17.022	2383	2386	2392	rVB2	8150	12008	0.11%	0.011%
26	17.234	2415	2422	2432	rBV	3964583	5723250	52.28%	5.237%
27	17.334	2432	2439	2461	rVV	6553594	9500873	86.78%	8.693%
28	19.151	2744	2748	2754	rBV3	82398	112304	1.03%	0.103%
29	19.222	2756	2760	2764	rVV	66936	92449	0.84%	0.085%
30	19.575	2814	2820	2830	rBV	8143776	10947891	100.00%	10.017%
31	21.328	3113	3118	3129	rBV	4575669	6098765	55.71%	5.580%
32	23.580	3494	3501	3515	rVB2	4807776	9763313	89.18%	8.933%
33	23.733	3521	3527	3539	rVB2	2729187	5315988	48.56%	4.864%




Sum of corrected areas: 109292110

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012209.D
Acq On : 20 Oct 2022 10:33
Operator : CG/JU
Sample : PB148327BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

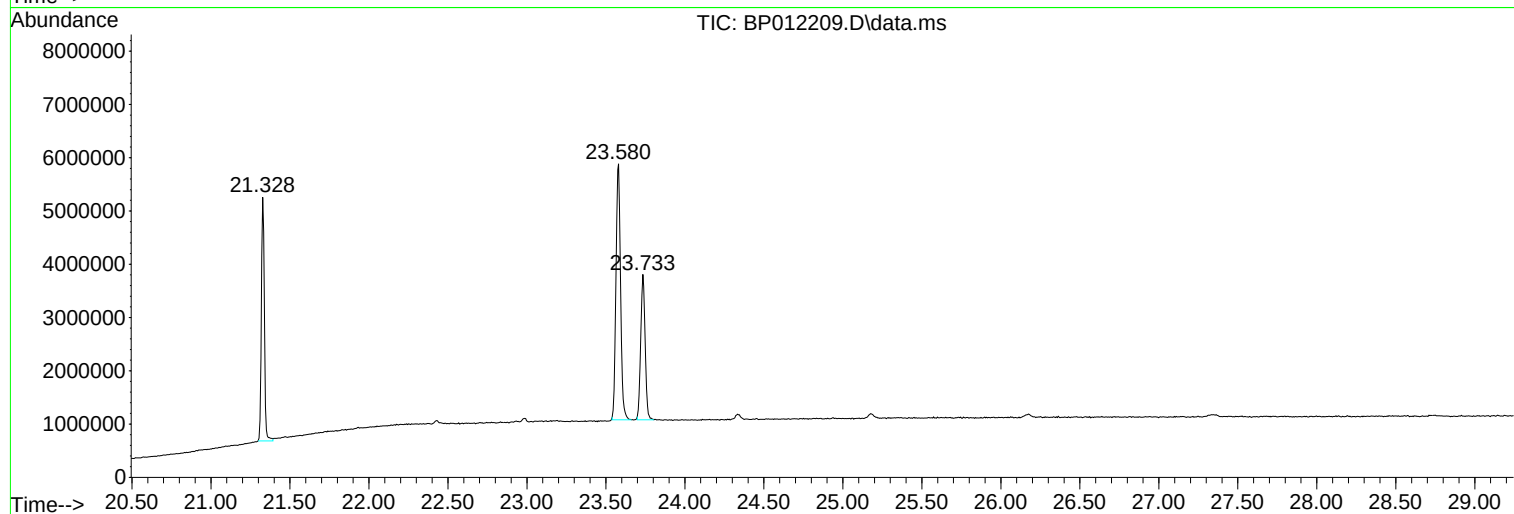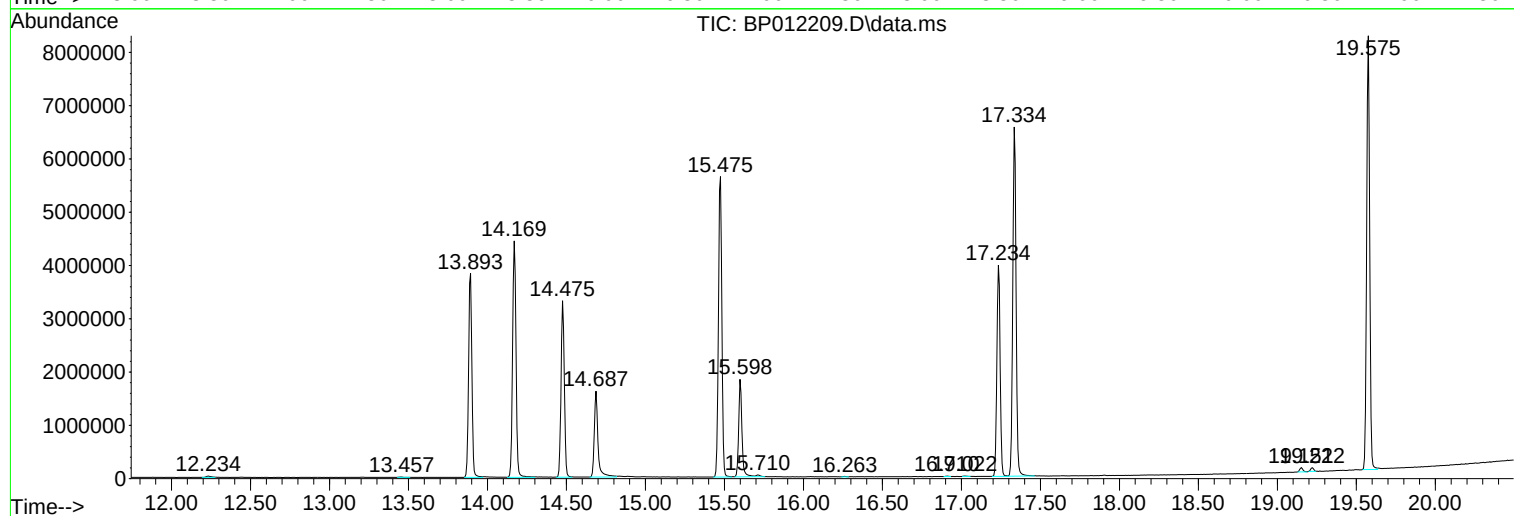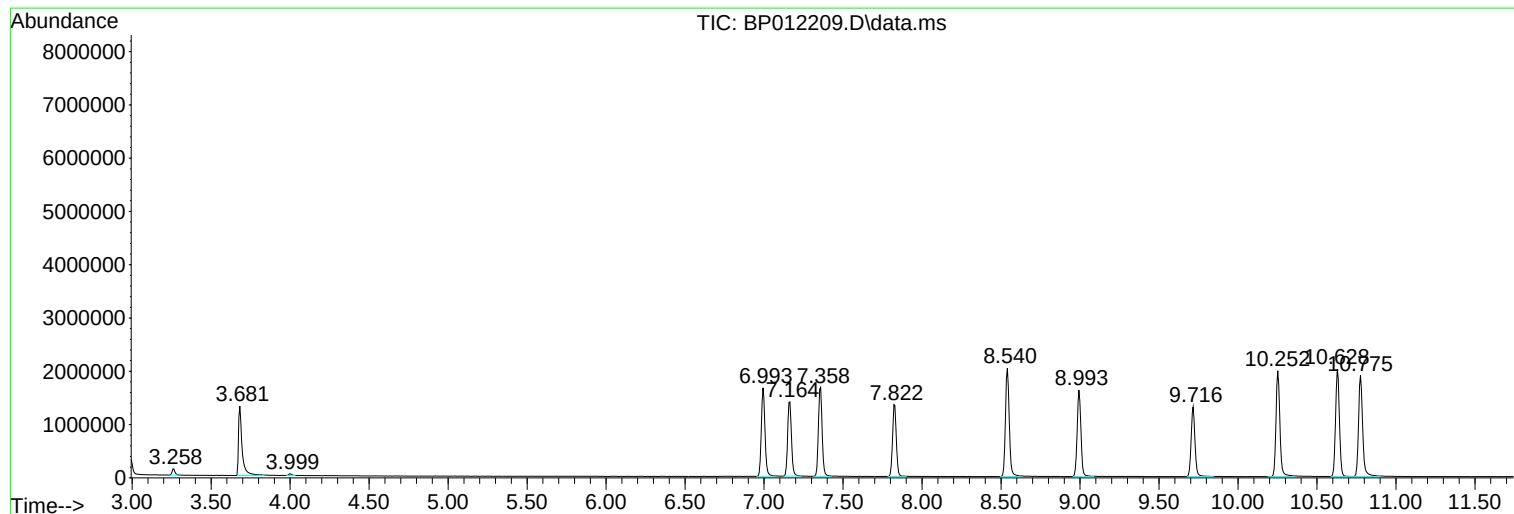

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012209.D
Acq On : 20 Oct 2022 10:33
Operator : CG/JU
Sample : PB148327BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012209.D
Acq On : 20 Oct 2022 10:33
Operator : CG/JU
Sample : PB148327BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK327

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc