

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012217.D
 Acq On : 20 Oct 2022 17:06
 Operator : CG/JU
 Sample : PB148363BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK363

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	43	46	52	rVB	120966	149029	2.03%	0.178%
2	3.681	115	118	135	rBV	862712	1317843	17.99%	1.577%
3	3.999	168	172	176	rBV	24648	31850	0.43%	0.038%
4	6.993	675	681	700	rBV	1544533	2524304	34.46%	3.021%
5	7.163	703	710	727	rVB	1287021	2158508	29.47%	2.583%
6	7.357	736	743	761	rBV	1563634	2586822	35.31%	3.095%
7	7.822	815	822	834	rBV	1203199	1984977	27.10%	2.375%
8	8.540	936	944	962	rBV	1879533	3130679	42.74%	3.746%
9	8.993	1014	1021	1032	rBV	1491748	2405560	32.84%	2.879%
10	9.716	1136	1144	1158	rBV	1158392	1954588	26.68%	2.339%
11	10.251	1228	1235	1249	rBV	1750340	3084607	42.11%	3.691%
12	10.628	1291	1299	1315	rBV	1713260	2914832	39.79%	3.488%
13	10.775	1317	1324	1348	rBV	1067092	2028429	27.69%	2.427%
14	12.228	1565	1571	1582	rBV2	22696	54313	0.74%	0.065%
15	13.198	1734	1736	1742	rVB7	4426	7732	0.11%	0.009%
16	13.451	1773	1779	1784	rBV7	5019	11008	0.15%	0.013%
17	13.887	1845	1853	1867	rBV	3083047	4368547	59.64%	5.227%
18	14.169	1893	1901	1915	rBV	3823920	5426108	74.07%	6.493%
19	14.475	1946	1953	1965	rBV	2514913	3783446	51.65%	4.527%
20	14.687	1982	1989	2012	rBV	1007110	1847173	25.22%	2.210%
21	15.475	2116	2123	2138	rBV	4636087	6798257	92.80%	8.135%
22	15.598	2138	2144	2159	rVV	1236420	1773902	24.22%	2.123%
23	15.710	2159	2163	2169	rVB	23944	40336	0.55%	0.048%
24	16.263	2253	2257	2264	rVB10	7176	12616	0.17%	0.015%
25	16.916	2363	2368	2372	rBV8	7650	14015	0.19%	0.017%
26	17.022	2383	2386	2392	rBV3	7266	10950	0.15%	0.013%
27	17.233	2416	2422	2432	rBV	2783682	4093666	55.88%	4.899%
28	17.333	2433	2439	2457	rVV2	4659291	6883551	93.97%	8.237%
29	17.898	2533	2535	2540	rBV6	7673	10523	0.14%	0.013%
30	18.133	2573	2575	2580	rBV5	9985	13147	0.18%	0.016%
31	19.151	2744	2748	2753	rBV3	60851	86897	1.19%	0.104%
32	19.222	2757	2760	2764	rVV	43682	54502	0.74%	0.065%
33	19.574	2814	2820	2832	rBV	5637617	7325346	100.00%	8.766%
34	21.327	3114	3118	3126	rBV	2952306	3707147	50.61%	4.436%
35	23.580	3494	3501	3516	rVB2	3500872	7069993	96.51%	8.460%
36	23.733	3521	3527	3537	rVB2	1945832	3903995	53.29%	4.672%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012217.D
Acq On : 20 Oct 2022 17:06
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK363

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Title : SVOA CALIBRATION




Sum of corrected areas: 83569198

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012217.D
Acq On : 20 Oct 2022 17:06
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

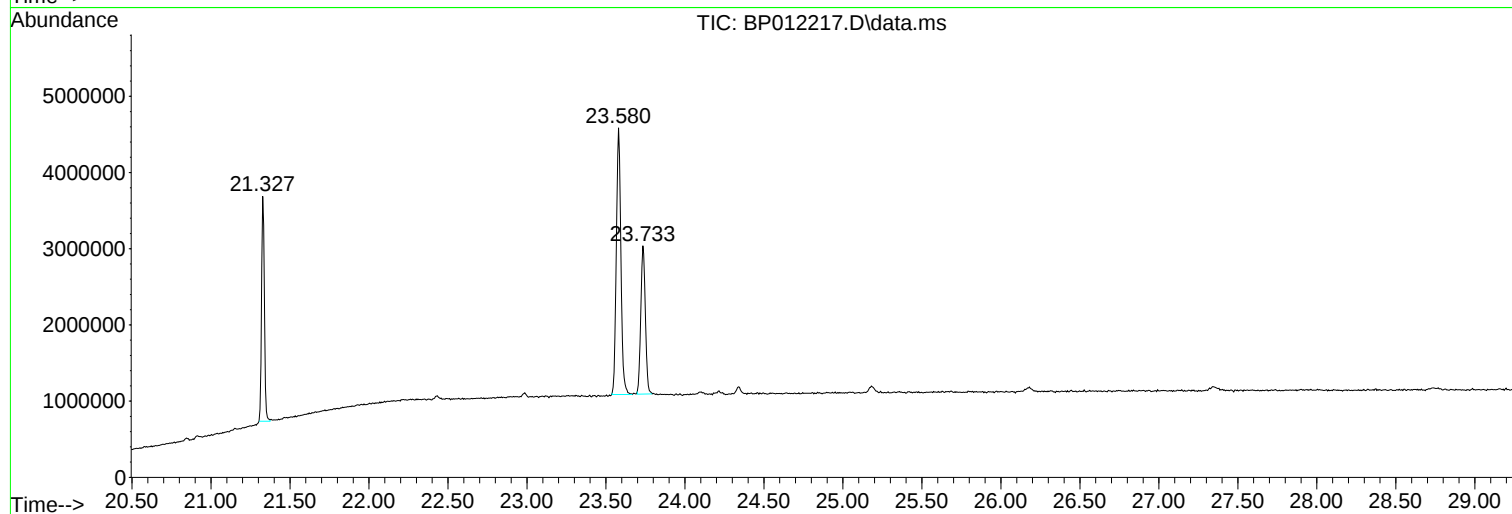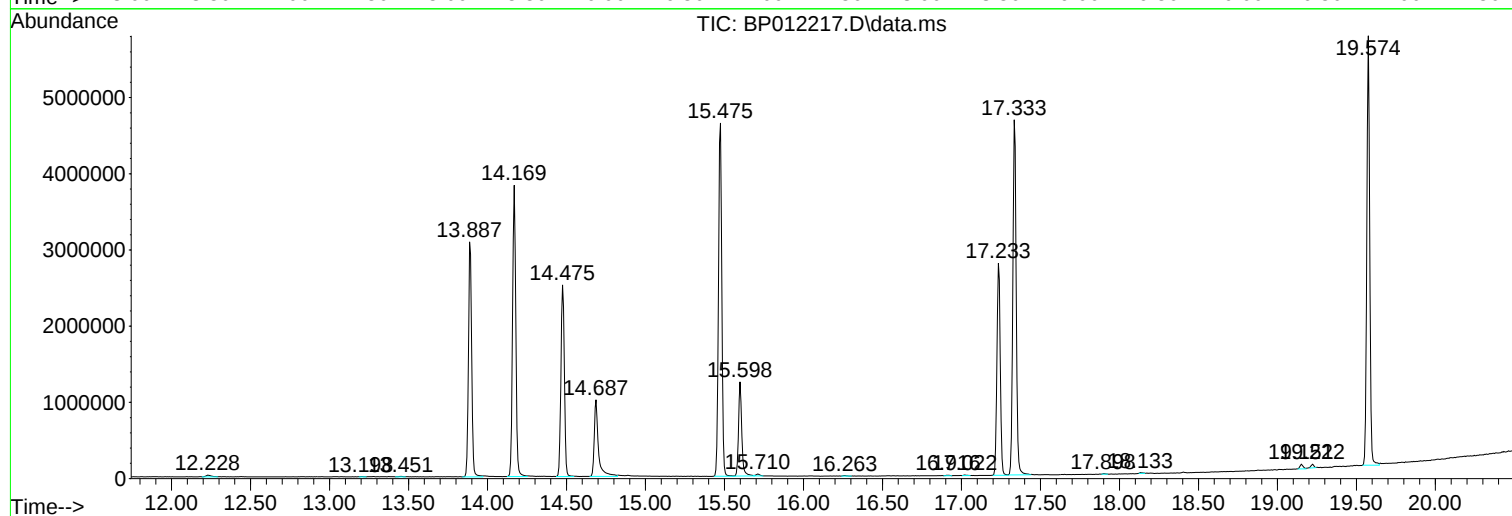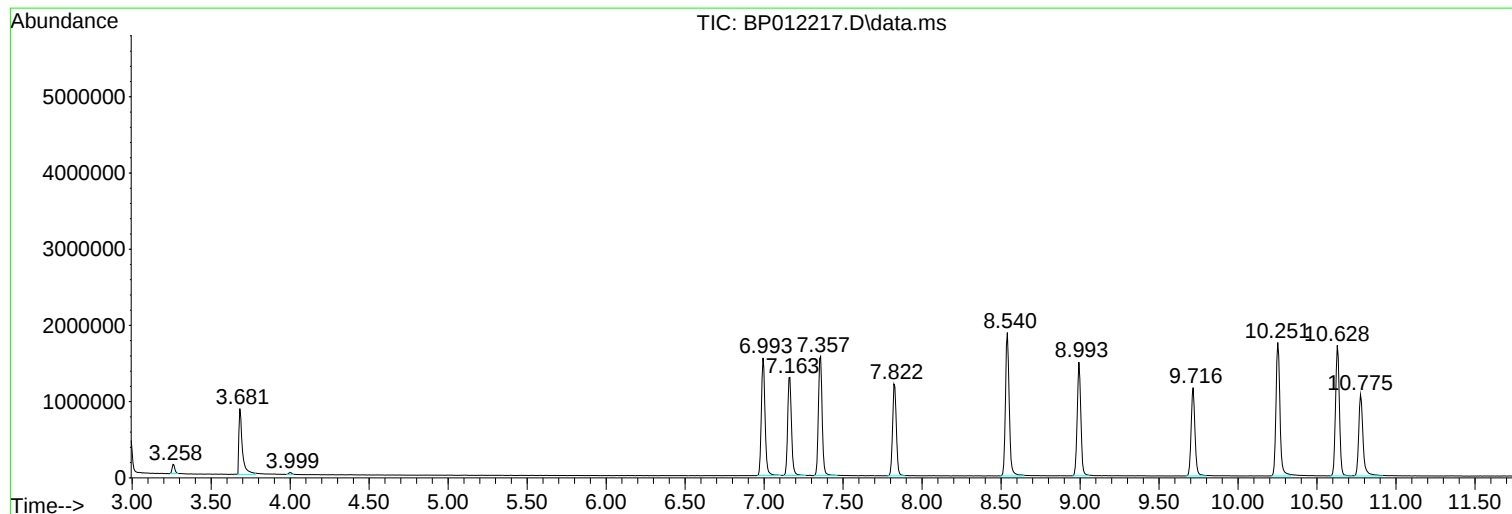

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012217.D
Acq On : 20 Oct 2022 17:06
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012217.D
Acq On : 20 Oct 2022 17:06
Operator : CG/JU
Sample : PB148363BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc