

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012229.D
 Acq On : 20 Oct 2022 23:57
 Operator : CG/JU
 Sample : N5103-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	51	rBV	84234	109078	1.20%	0.113%
2	3.546	92	95	104	rBV	29943	47434	0.52%	0.049%
3	3.681	116	118	134	rBV	449484	723752	7.93%	0.748%
4	3.905	150	156	161	rBV	45784	69160	0.76%	0.072%
5	3.999	167	172	178	rVB	31652	43070	0.47%	0.045%
6	4.375	231	236	241	rVB4	9589	15518	0.17%	0.016%
7	4.917	323	328	335	rBV2	10925	23102	0.25%	0.024%
8	6.993	674	681	694	rBV	332620	616379	6.76%	0.637%
9	7.158	702	709	727	rBV	1502182	2426406	26.60%	2.509%
10	7.352	736	742	753	rBV	1322693	2131221	23.36%	2.204%
11	7.822	814	822	830	rBV	1593564	2551514	27.97%	2.639%
12	8.534	936	943	962	rBV	992648	1743586	19.11%	1.803%
13	8.993	1013	1021	1038	rBV	1706169	2909376	31.89%	3.009%
14	9.152	1044	1048	1053	rVB7	10347	16864	0.18%	0.017%
15	9.381	1082	1087	1093	rBV2	23891	40072	0.44%	0.041%
16	9.710	1134	1143	1157	rBV	1303337	2263326	24.81%	2.341%
17	10.252	1226	1235	1256	rBV	1867993	3360893	36.84%	3.476%
18	10.410	1256	1262	1280	rBV	136193	339447	3.72%	0.351%
19	10.628	1291	1299	1313	rBV	2300391	3872282	42.45%	4.005%
20	10.775	1316	1324	1340	rVV	1464727	2648596	29.03%	2.739%
21	11.875	1508	1511	1516	rVB5	6875	10285	0.11%	0.011%
22	12.052	1535	1541	1545	rBV9	6359	11337	0.12%	0.012%
23	12.222	1564	1570	1579	rVB	35736	64451	0.71%	0.067%
24	13.081	1711	1716	1723	rBV8	6730	14469	0.16%	0.015%
25	13.204	1731	1737	1741	rVB7	6842	13127	0.14%	0.014%
26	13.287	1745	1751	1759	rVV2	25031	43761	0.48%	0.045%
27	13.369	1759	1765	1770	rVV3	13037	23557	0.26%	0.024%
28	13.440	1773	1777	1782	rVB3	10319	15442	0.17%	0.016%
29	13.887	1846	1853	1867	rBV	3883981	5464661	59.90%	5.651%
30	14.169	1889	1901	1918	rBV	4237810	6681241	73.24%	6.909%
31	14.363	1931	1934	1938	rVB3	16392	18602	0.20%	0.019%
32	14.475	1943	1953	1968	rBV	3386561	5120826	56.13%	5.296%
33	14.640	1977	1981	1985	rBV5	10382	17073	0.19%	0.018%
34	14.693	1985	1990	2006	rVV2	144639	359691	3.94%	0.372%
35	14.893	2019	2024	2033	rVB2	17904	42561	0.47%	0.044%
36	15.269	2083	2088	2091	rBV3	9877	17438	0.19%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012229.D
 Acq On : 20 Oct 2022 23:57
 Operator : CG/JU
 Sample : N5103-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	15.322	2093	2097	2102	rVB2	13885	21866	0.24%	0.023%
38	15.469	2115	2122	2137	rBV	5735419	8402116	92.10%	8.689%
39	15.598	2138	2144	2157	rVV	1323495	1852003	20.30%	1.915%
40	15.710	2159	2163	2170	rVB2	32044	51294	0.56%	0.053%
41	15.928	2196	2200	2206	rVB6	10107	15757	0.17%	0.016%
42	16.040	2213	2219	2223	rBV7	8834	17547	0.19%	0.018%
43	16.187	2240	2244	2247	rBV5	11252	14754	0.16%	0.015%
44	16.257	2252	2256	2260	rVB6	12671	17864	0.20%	0.018%
45	16.634	2317	2320	2325	rVB7	6142	10421	0.11%	0.011%
46	16.904	2364	2366	2371	rVB6	7677	10129	0.11%	0.010%
47	17.016	2382	2385	2388	rBV3	10455	14764	0.16%	0.015%
48	17.234	2415	2422	2432	rBV	3936345	5501357	60.31%	5.689%
49	17.334	2432	2439	2450	rBV2	6288914	9101720	99.77%	9.413%
50	17.522	2468	2471	2480	rVB6	12402	21535	0.24%	0.022%
51	17.898	2532	2535	2541	rVB	54566	62993	0.69%	0.065%
52	18.116	2568	2572	2582	rBV	245585	409894	4.49%	0.424%
53	19.145	2743	2747	2753	rBV2	84815	130014	1.43%	0.134%
54	19.216	2755	2759	2762	rBV	91903	128548	1.41%	0.133%
55	19.351	2779	2782	2792	rBV2	166571	263572	2.89%	0.273%
56	19.575	2814	2820	2833	rBV	6659662	9122481	100.00%	9.434%
57	21.033	3064	3068	3077	rBV	324219	604690	6.63%	0.625%
58	21.322	3113	3117	3129	rBV	3283024	4375461	47.96%	4.525%
59	23.574	3493	3500	3514	rVB2	3841488	8266120	90.61%	8.548%
60	23.727	3520	3526	3536	rVB2	2219231	4410404	48.35%	4.561%




Sum of corrected areas: 96696902

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012229.D
Acq On : 20 Oct 2022 23:57
Operator : CG/JU
Sample : N5103-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COBB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

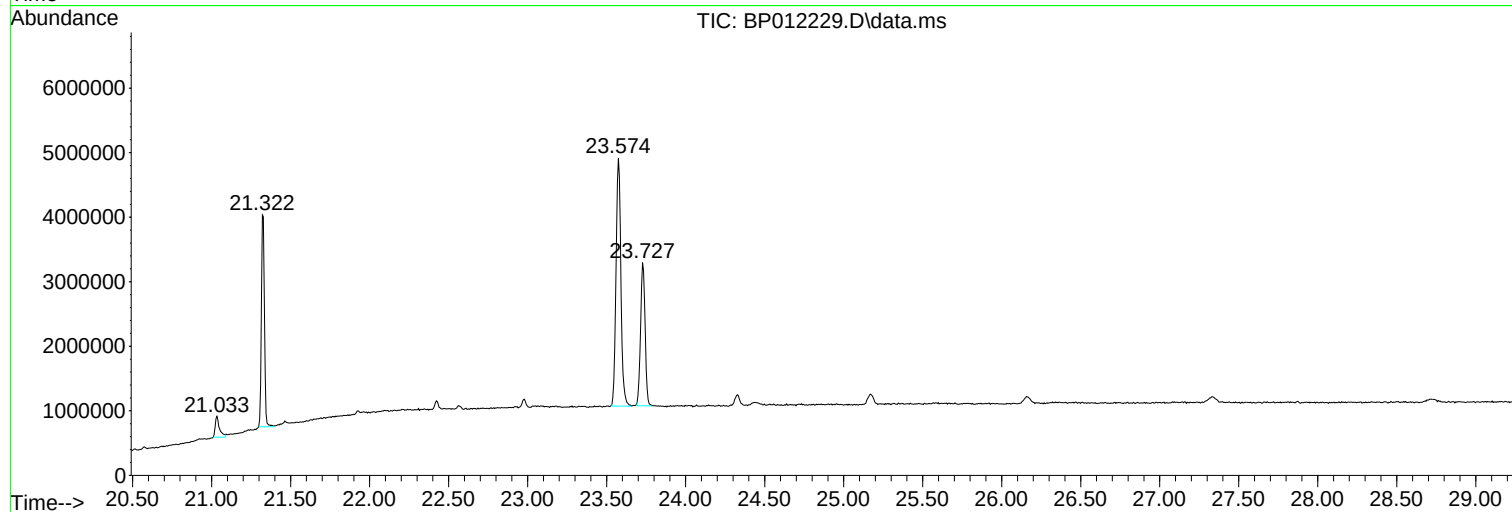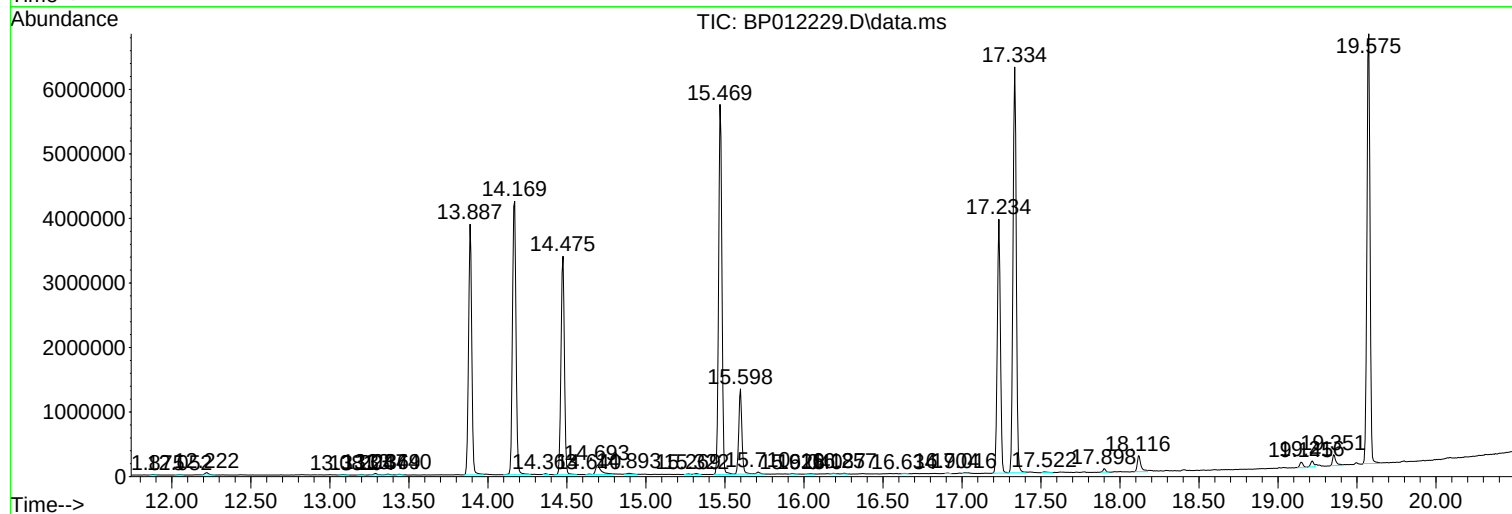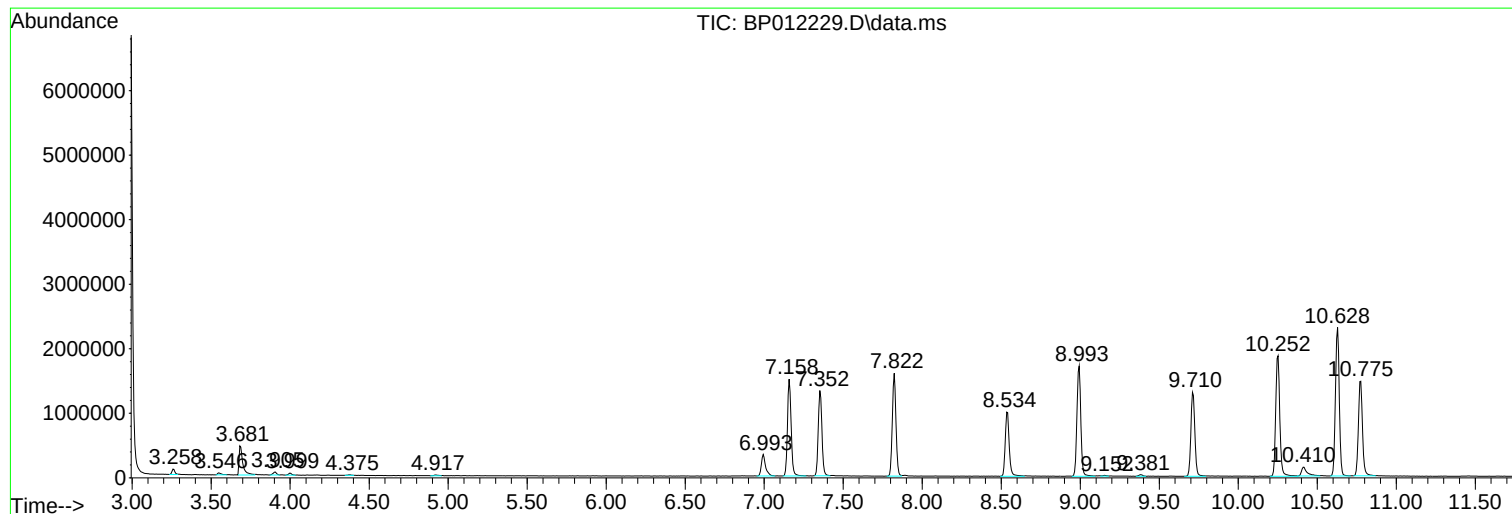

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012229.D
Acq On : 20 Oct 2022 23:57
Operator : CG/JU
Sample : N5103-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COBB0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.033	2.76 ng/ul	604690	Chrysene-d12	21.328

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			Cyclopentadecane	210	C15H30	000295-48-7	94
3			Behenic alcohol	326	C22H46O	000661-19-8	94
4			1-Heneicosanol	312	C21H44O	015594-90-8	94
5			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94

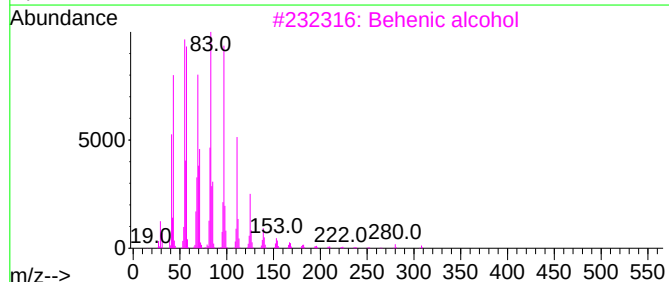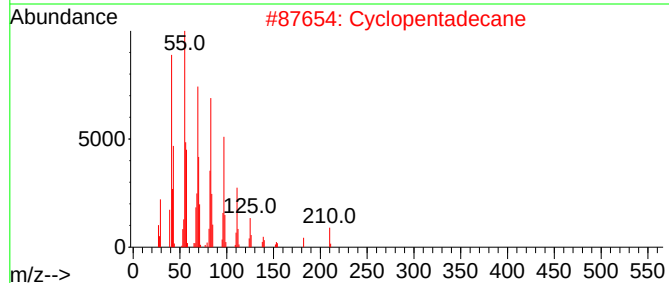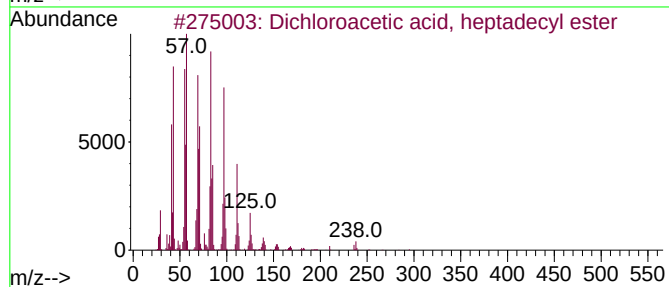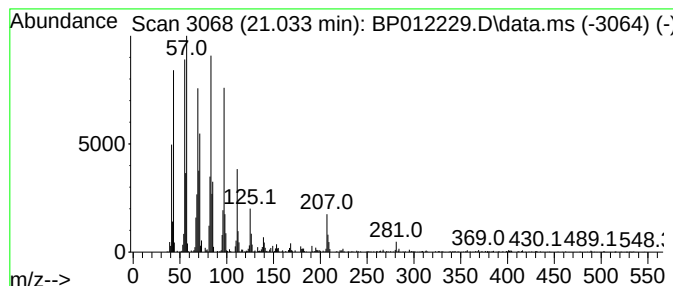

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012229.D
Acq On : 20 Oct 2022 23:57
Operator : CG/JU
Sample : N5103-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	21.033	2.8	ng/u1	604690	5	21.328	4375460	20.0