

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012230.D
 Acq On : 21 Oct 2022 00:31
 Operator : CG/JU
 Sample : N5103-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	51	rBV	88849	107236	1.31%	0.123%
2	3.546	92	95	102	rBV	33005	45639	0.56%	0.053%
3	3.687	116	119	134	rBV	293823	469240	5.74%	0.540%
4	3.905	150	156	162	rVB	47877	76933	0.94%	0.089%
5	3.999	168	172	176	rBV	32692	42079	0.51%	0.048%
6	4.375	232	236	242	rBV7	10720	16531	0.20%	0.019%
7	4.922	325	329	337	rBV4	10485	20779	0.25%	0.024%
8	6.993	675	681	697	rBV2	354431	660525	8.08%	0.760%
9	7.158	701	709	722	rBV	1485469	2380948	29.12%	2.741%
10	7.352	735	742	752	rBV	1329007	2151618	26.31%	2.477%
11	7.428	753	755	764	rVB8	10632	19087	0.23%	0.022%
12	7.822	813	822	830	rBV	1439520	2282139	27.91%	2.627%
13	7.893	830	834	842	rVB	14471	26917	0.33%	0.031%
14	8.534	936	943	961	rBV	976063	1697735	20.76%	1.955%
15	8.657	961	964	974	rVB9	5205	12825	0.16%	0.015%
16	8.993	1013	1021	1036	rBV	1719701	2823588	34.53%	3.251%
17	9.152	1044	1048	1057	rVB9	10562	21226	0.26%	0.024%
18	9.381	1081	1087	1094	rVB2	38231	63656	0.78%	0.073%
19	9.710	1135	1143	1155	rBV	1302246	2195848	26.85%	2.528%
20	10.169	1215	1221	1223	rBV7	4699	8710	0.11%	0.010%
21	10.251	1227	1235	1257	rVB	1830910	3206348	39.21%	3.691%
22	10.422	1257	1264	1278	rBV2	46151	133651	1.63%	0.154%
23	10.628	1291	1299	1313	rBV	2004588	3413601	41.75%	3.930%
24	10.769	1316	1323	1343	rBV	1197008	2185309	26.73%	2.516%
25	11.881	1507	1512	1521	rBV8	7783	13827	0.17%	0.016%
26	12.045	1534	1540	1545	rVB5	15709	25797	0.32%	0.030%
27	12.222	1564	1570	1576	rVB	31813	53032	0.65%	0.061%
28	12.857	1674	1678	1681	rVB5	7681	10532	0.13%	0.012%
29	12.998	1698	1702	1711	rVB9	7261	16219	0.20%	0.019%
30	13.075	1711	1715	1723	rBV9	4598	8237	0.10%	0.009%
31	13.287	1747	1751	1760	rVB	48933	71014	0.87%	0.082%
32	13.363	1760	1764	1768	rBV6	10351	16446	0.20%	0.019%
33	13.440	1773	1777	1784	rVB6	9418	19156	0.23%	0.022%
34	13.698	1815	1821	1825	rBV9	4450	8347	0.10%	0.010%
35	13.810	1835	1840	1845	rBV9	4141	8653	0.11%	0.010%
36	13.887	1845	1853	1866	rVV	3431681	4881512	59.70%	5.620%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012230.D
 Acq On : 21 Oct 2022 00:31
 Operator : CG/JU
 Sample : N5103-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBX3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	13.981	1867	1869	1879	rVB9	13513	28136	0.34%	0.032%
38	14.169	1893	1901	1918	rVB	3968553	6072457	74.26%	6.991%
39	14.363	1927	1934	1941	rVB2	35271	50026	0.61%	0.058%
40	14.475	1944	1953	1963	rBV	2830650	4281861	52.37%	4.930%
41	14.645	1977	1982	1984	rBV6	7077	9739	0.12%	0.011%
42	14.692	1984	1990	2008	rBV2	122419	325475	3.98%	0.375%
43	14.987	2036	2040	2048	rVB2	7972	15061	0.18%	0.017%
44	15.322	2092	2097	2102	rVB2	37809	52539	0.64%	0.060%
45	15.469	2116	2122	2137	rBV	5022390	7387101	90.34%	8.504%
46	15.598	2137	2144	2157	rVV	1111638	1623252	19.85%	1.869%
47	15.710	2158	2163	2171	rVB4	31542	58910	0.72%	0.068%
48	15.875	2189	2191	2196	rVV6	5192	8285	0.10%	0.010%
49	15.939	2197	2202	2207	rVB9	9957	17589	0.22%	0.020%
50	16.028	2212	2217	2218	rBV5	8257	12009	0.15%	0.014%
51	16.186	2240	2244	2252	rBV	56280	83659	1.02%	0.096%
52	16.251	2252	2255	2260	rVB6	13370	20742	0.25%	0.024%
53	16.533	2299	2303	2304	rBV3	6459	8244	0.10%	0.009%
54	16.639	2316	2321	2326	rVB8	7825	14544	0.18%	0.017%
55	16.981	2375	2379	2383	rBV	59112	78684	0.96%	0.091%
56	17.033	2383	2388	2396	rVB5	19407	41708	0.51%	0.048%
57	17.233	2415	2422	2432	rBV	3014880	4373381	53.48%	5.035%
58	17.333	2432	2439	2451	rVV	5225986	7612754	93.10%	8.764%
59	17.728	2502	2506	2510	rBV	56697	72684	0.89%	0.084%
60	17.898	2531	2535	2541	rBV2	54963	69588	0.85%	0.080%
61	18.116	2568	2572	2583	rBV	193503	335529	4.10%	0.386%
62	18.398	2616	2620	2625	rBV2	64490	88167	1.08%	0.102%
63	19.010	2721	2724	2726	rBV2	42630	49605	0.61%	0.057%
64	19.151	2744	2748	2754	rBV5	61239	101530	1.24%	0.117%
65	19.216	2756	2759	2762	rBV	71127	91215	1.12%	0.105%
66	19.351	2779	2782	2790	rBV	139833	212897	2.60%	0.245%
67	19.569	2814	2819	2833	rBV	5646901	7777928	95.12%	8.954%
68	21.033	3064	3068	3077	rBV3	253206	492002	6.02%	0.566%
69	21.321	3113	3117	3125	rBV	2926099	3822223	46.74%	4.400%
70	23.574	3493	3500	3515	rVB2	3882757	8176875	100.00%	9.414%
71	23.727	3520	3526	3539	rVB2	2105714	4200461	51.37%	4.836%




Sum of corrected areas: 86861800

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012230.D
Acq On : 21 Oct 2022 00:31
Operator : CG/JU
Sample : N5103-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

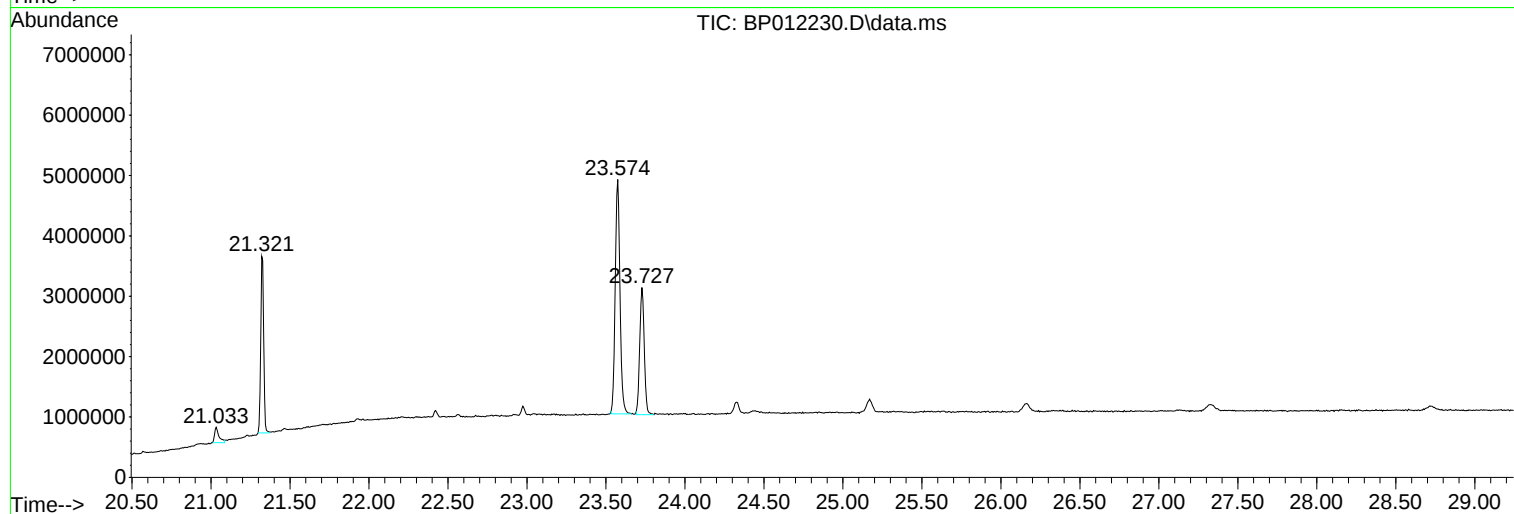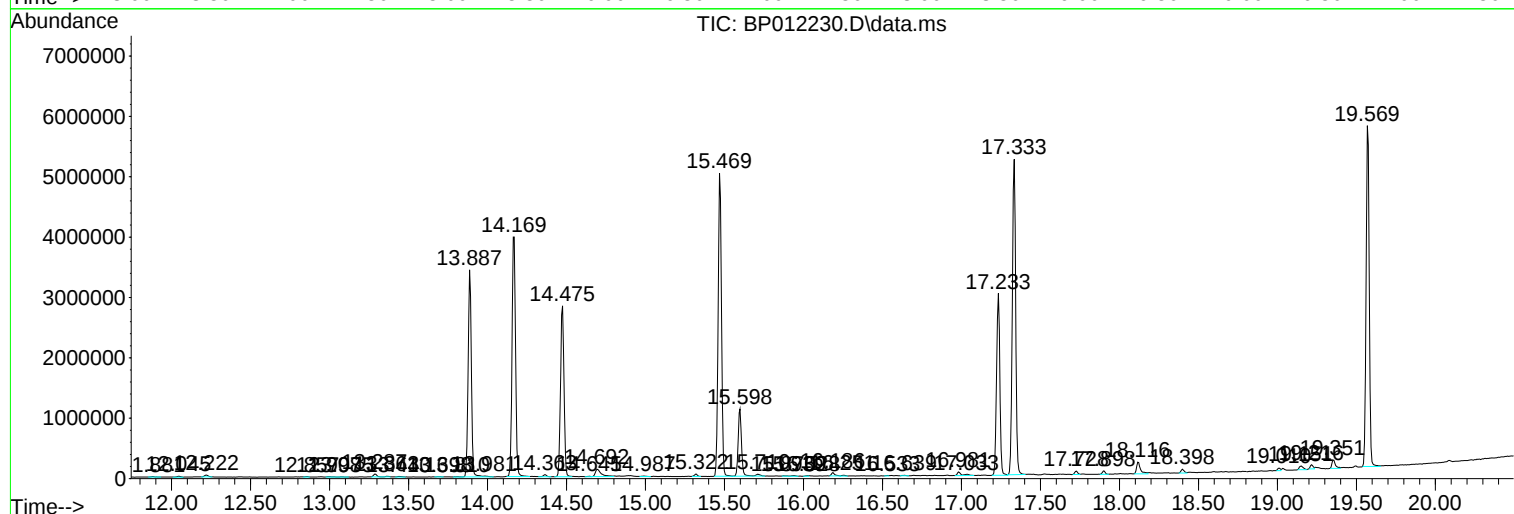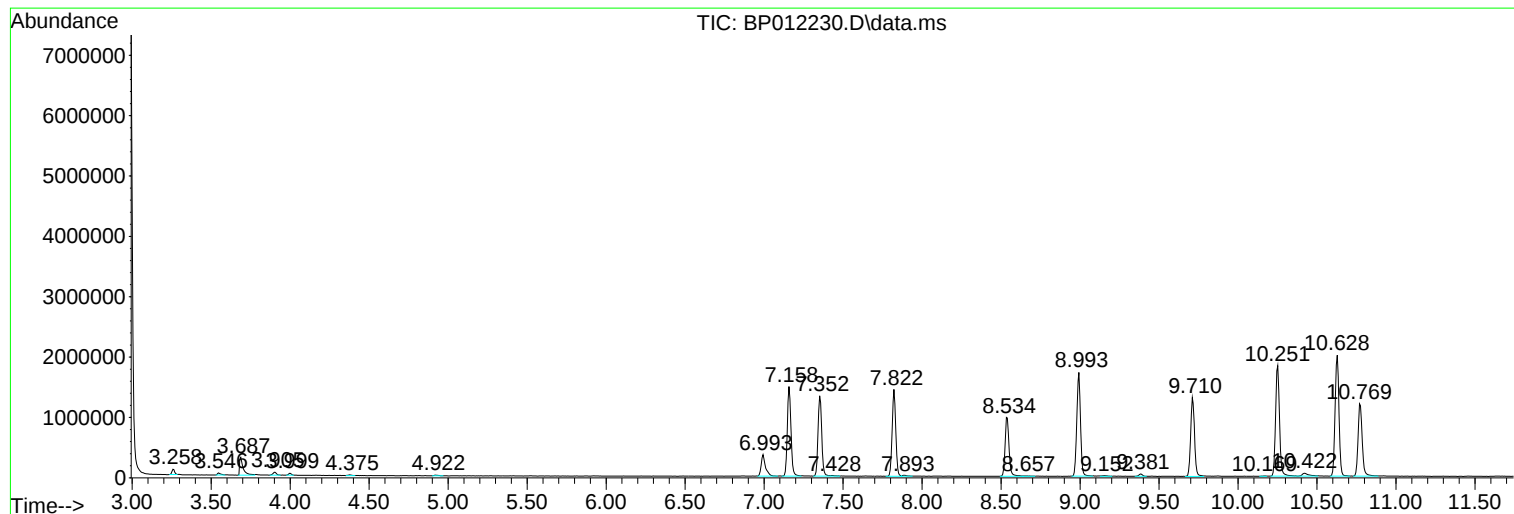

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012230.D
Acq On : 21 Oct 2022 00:31
Operator : CG/JU
Sample : N5103-06
Misc :
ALS Vial : 24 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0BX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.033	2.57 ng/ul	492002	Chrysene-d12	21.322	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene	266	C19H38	018435-45-5	94
2	Pentacos-1-ene	350	C25H50	016980-85-1	94
3	2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94
4	1-Heneicosanol	312	C21H44O	015594-90-8	94
5	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94

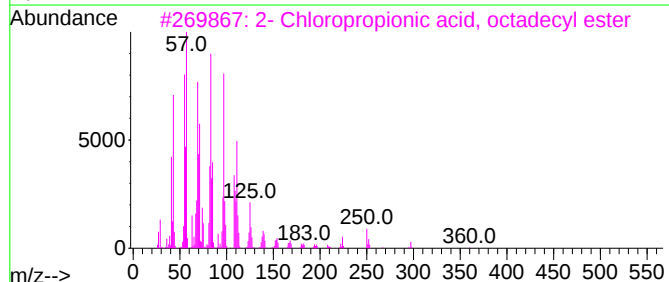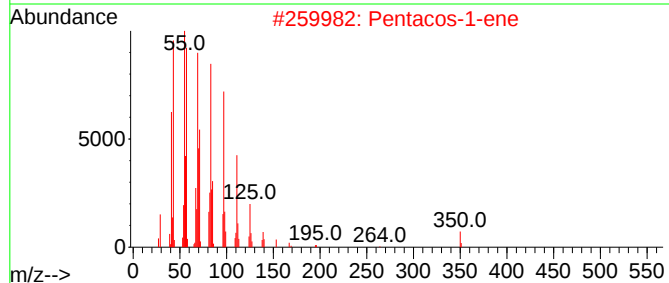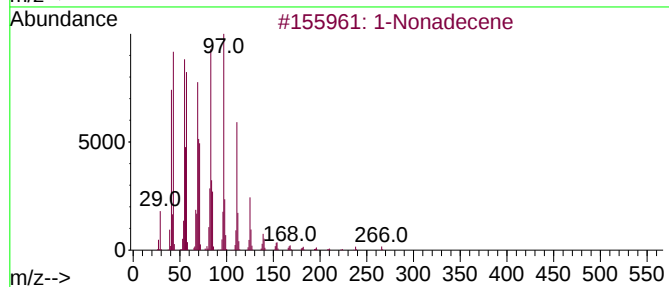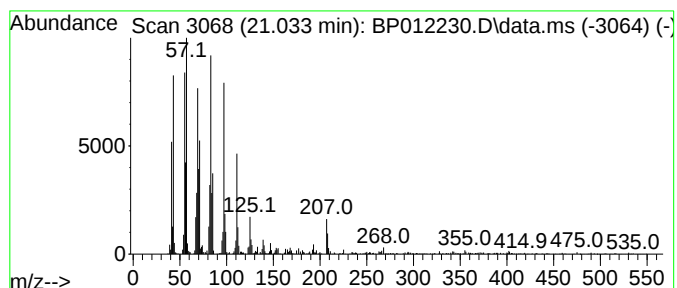

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012230.D
Acq On : 21 Oct 2022 00:31
Operator : CG/JU
Sample : N5103-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.033	2.6	ng/u1	492002	5	21.322	3822220	20.0