

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012232.D
 Acq On : 21 Oct 2022 01:39
 Operator : CG/JU
 Sample : N5103-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	43	46	56	rVB	92236	133813	1.43%	0.147%
2	3.681	116	118	138	rBV	707592	1063292	11.34%	1.172%
3	3.904	151	156	161	rVB	51243	75081	0.80%	0.083%
4	3.999	169	172	178	rVB	32393	44631	0.48%	0.049%
5	4.940	326	332	343	rVB2	18792	49031	0.52%	0.054%
6	6.993	675	681	697	rVB	323035	538024	5.74%	0.593%
7	7.157	702	709	724	rBV	1502627	2393574	25.52%	2.638%
8	7.351	735	742	752	rBV	1308650	2111389	22.51%	2.327%
9	7.822	815	822	832	rBV	1449906	2361528	25.18%	2.603%
10	8.534	936	943	955	rBV	971408	1664106	17.74%	1.834%
11	8.992	1013	1021	1033	rBV	1637230	2846892	30.36%	3.138%
12	9.381	1083	1087	1092	rVB3	12423	20531	0.22%	0.023%
13	9.710	1136	1143	1157	rBV	916107	1550621	16.53%	1.709%
14	10.251	1227	1235	1254	rBV	1758164	3151541	33.60%	3.474%
15	10.628	1290	1299	1314	rBV	2058591	3597216	38.36%	3.965%
16	10.769	1316	1323	1342	rBV	1545109	2932580	31.27%	3.232%
17	12.051	1534	1541	1549	rVB	7604	17493	0.19%	0.019%
18	12.222	1561	1570	1576	rBV	31282	56064	0.60%	0.062%
19	12.439	1598	1607	1612	rBV	4472	10486	0.11%	0.012%
20	13.075	1710	1715	1722	rBV8	5476	10832	0.12%	0.012%
21	13.439	1771	1777	1781	rBV5	9163	17511	0.19%	0.019%
22	13.798	1834	1838	1845	rBV4	18279	28914	0.31%	0.032%
23	13.886	1845	1853	1865	rBV	3753991	5281849	56.32%	5.822%
24	14.169	1893	1901	1919	rBV	4265476	6490616	69.21%	7.154%
25	14.475	1946	1953	1964	rBV	3166956	4695716	50.07%	5.176%
26	14.704	1985	1992	1997	rBV3	56788	138770	1.48%	0.153%
27	14.751	1998	2000	2011	rVB3	29556	60402	0.64%	0.067%
28	14.916	2024	2028	2032	rVB5	10051	14911	0.16%	0.016%
29	15.269	2082	2088	2091	rBV	10412	15774	0.17%	0.017%
30	15.298	2091	2093	2104	rVB6	6437	13364	0.14%	0.015%
31	15.469	2111	2122	2133	rBV	5736026	8186412	87.29%	9.023%
32	15.598	2139	2144	2153	rBV	58417	107888	1.15%	0.119%
33	15.710	2159	2163	2169	rVB	26344	39446	0.42%	0.043%
34	16.257	2253	2256	2261	rVB7	6579	10347	0.11%	0.011%
35	16.904	2364	2366	2371	rVB6	8191	12127	0.13%	0.013%
36	17.021	2383	2386	2392	rVB3	7939	13165	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012232.D
 Acq On : 21 Oct 2022 01:39
 Operator : CG/JU
 Sample : N5103-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BA2

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	17.233	2415	2422	2432	rBV	3593227	5158395	55.00%	5.686%
38	17.333	2432	2439	2452	rVV	6474175	9378194	100.00%	10.337%
39	17.433	2452	2456	2465	rVB3	63117	103064	1.10%	0.114%
40	17.521	2469	2471	2475	rVB3	9215	10679	0.11%	0.012%
41	18.121	2570	2573	2578	rBV6	12682	19697	0.21%	0.022%
42	19.145	2744	2747	2753	rBV2	79743	97509	1.04%	0.107%
43	19.215	2755	2759	2764	rBV	71625	112388	1.20%	0.124%
44	19.568	2814	2819	2832	rBV	6448995	9232281	98.44%	10.176%
45	21.321	3113	3117	3127	rBV	3179867	4176256	44.53%	4.603%
46	23.574	3493	3500	3512	rVB2	3979840	8504468	90.68%	9.374%
47	23.727	3520	3526	3537	rVB2	2042322	4179772	44.57%	4.607%




Sum of corrected areas: 90728640

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012232.D
Acq On : 21 Oct 2022 01:39
Operator : CG/JU
Sample : N5103-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

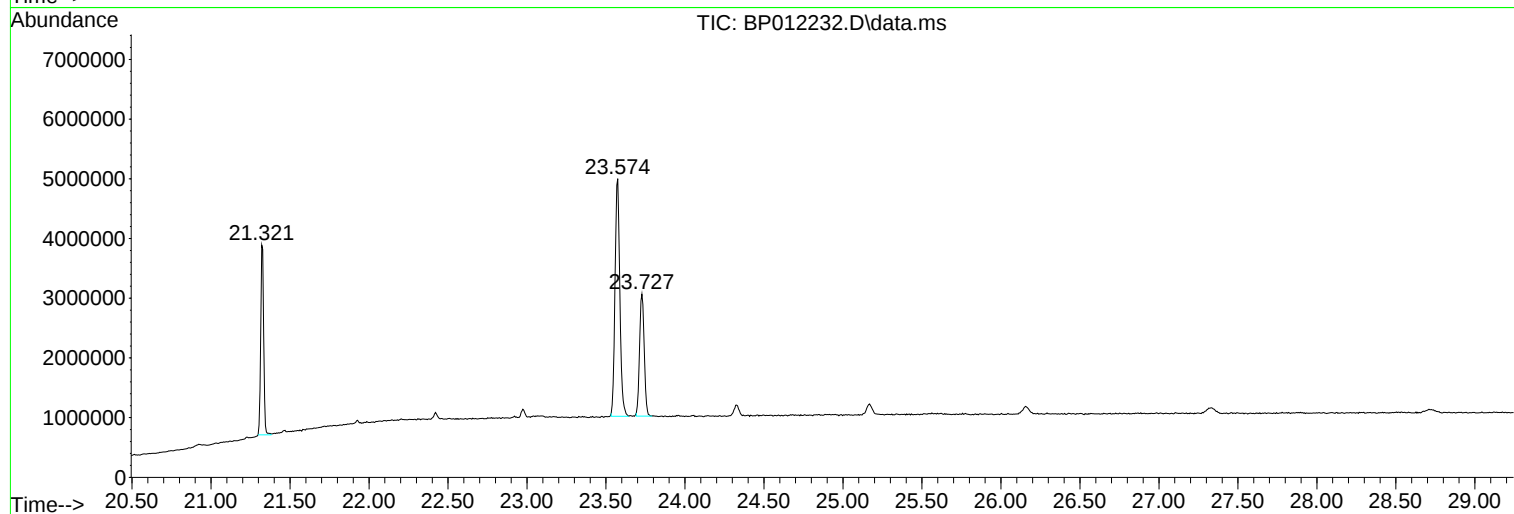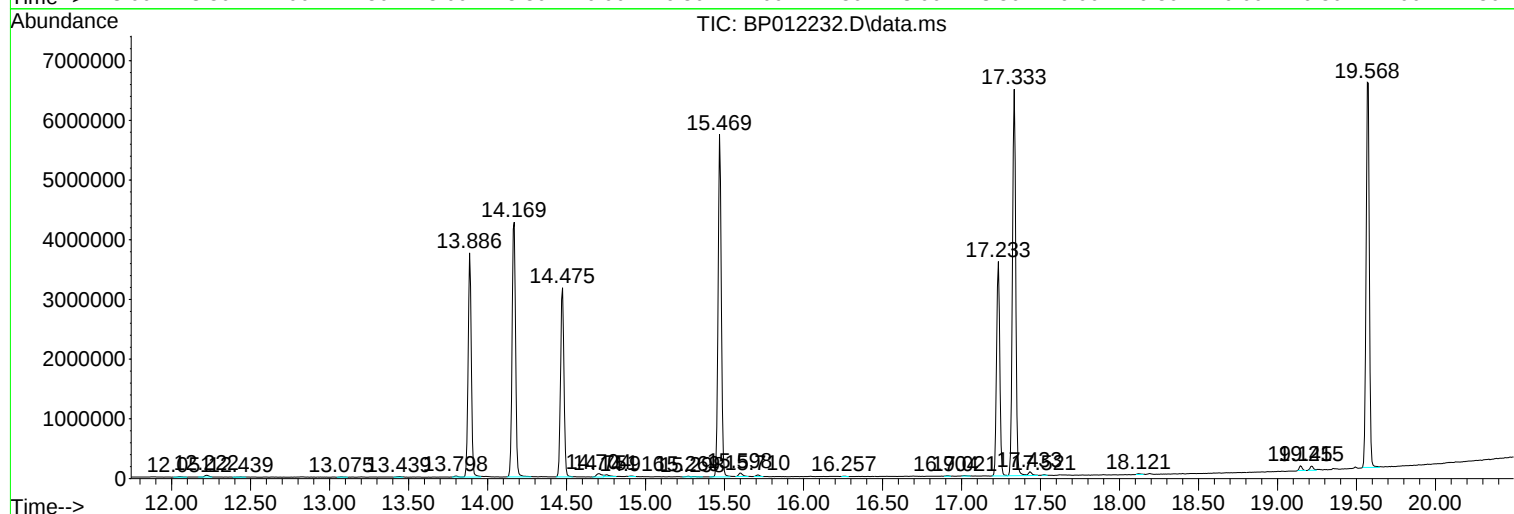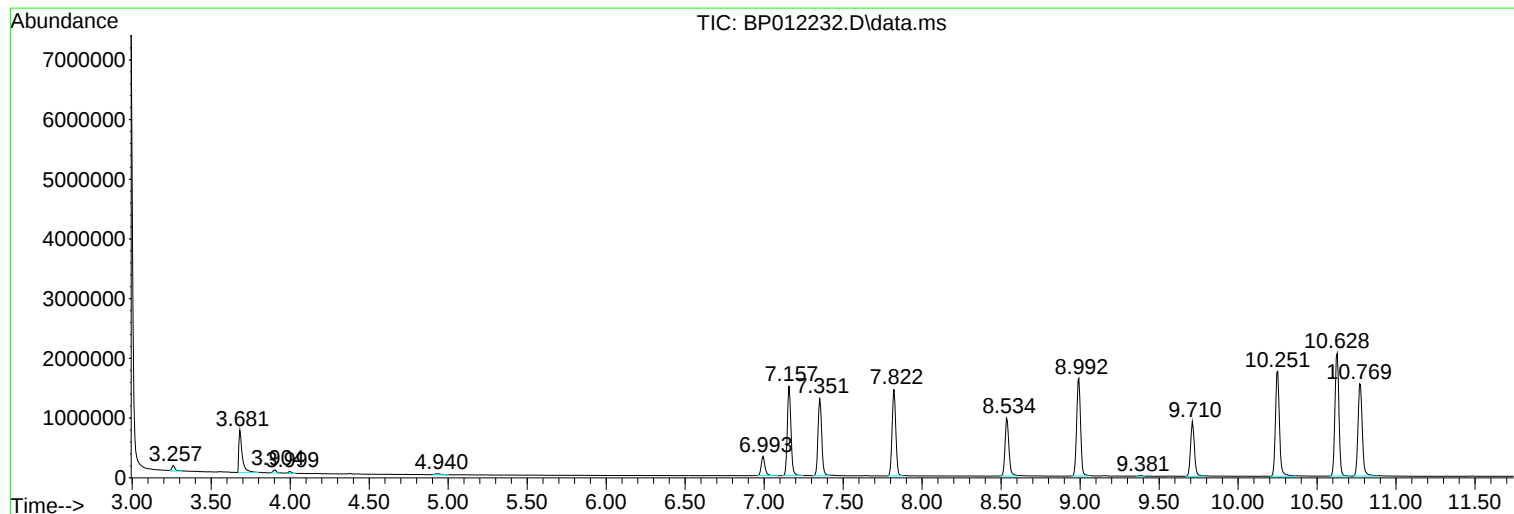

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012232.D
Acq On : 21 Oct 2022 01:39
Operator : CG/JU
Sample : N5103-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012232.D
Acq On : 21 Oct 2022 01:39
Operator : CG/JU
Sample : N5103-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc